
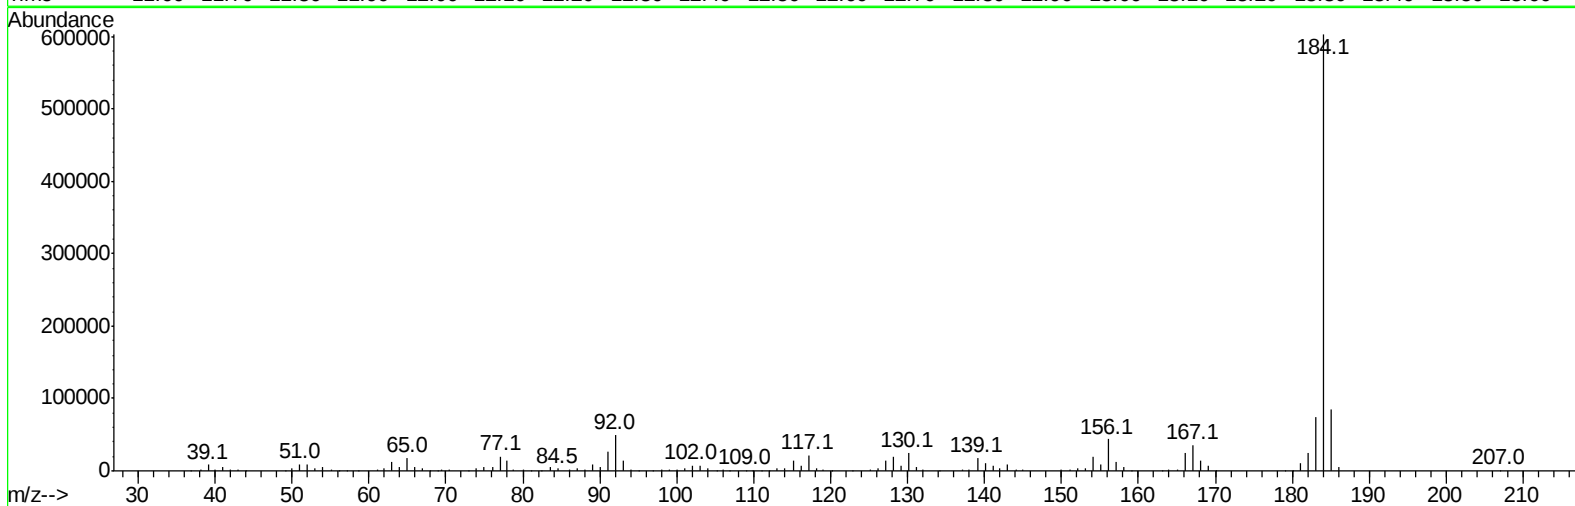


Data Path : U:\HPCHEM1\BNA F\DATA\BF011618\
Data File : BF102096.D
Acq On : 16 Jan 2018 9:16
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 17 07:00:12 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 11 12:53:54 2018
Response via : Initial Calibration

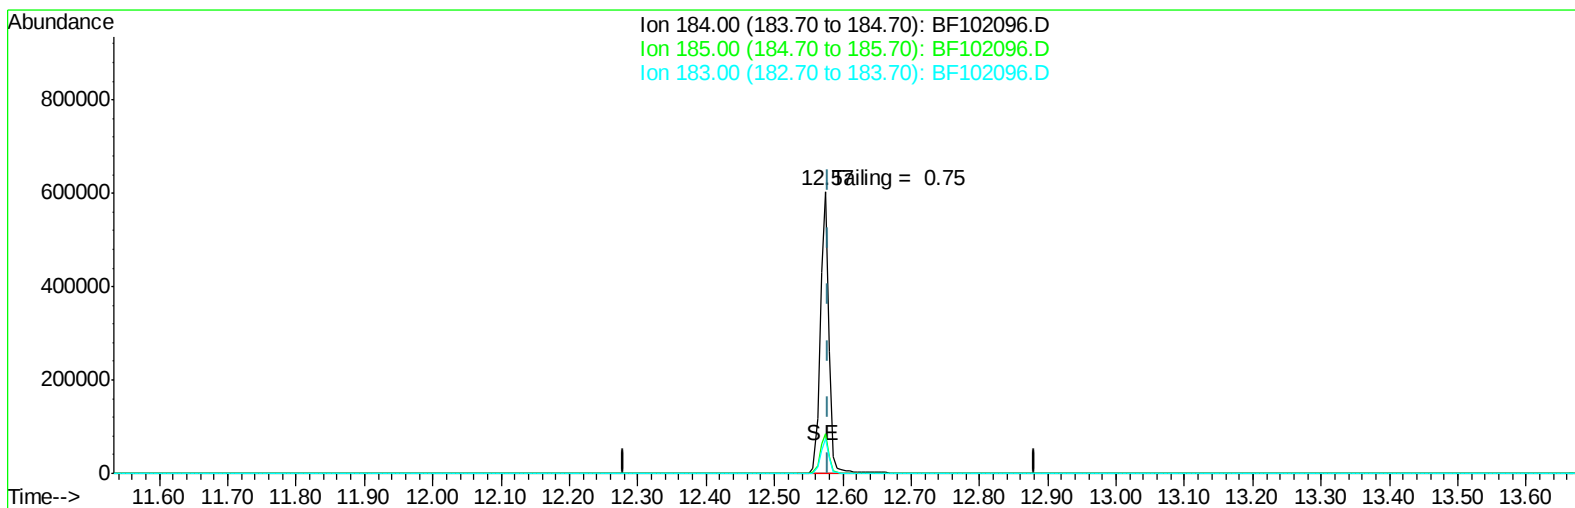

TIC: BF102096.D

(76) Benzidine



12.574min (-0.006) 0.00ng

response 534168

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.99
183.00	11.60	12.40
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA F\DATA\BF011618\
Data File : BF102096.D
Acq On : 16 Jan 2018 9:16
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 17 07:00:12 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 11 12:53:54 2018
Response via : Initial Calibration

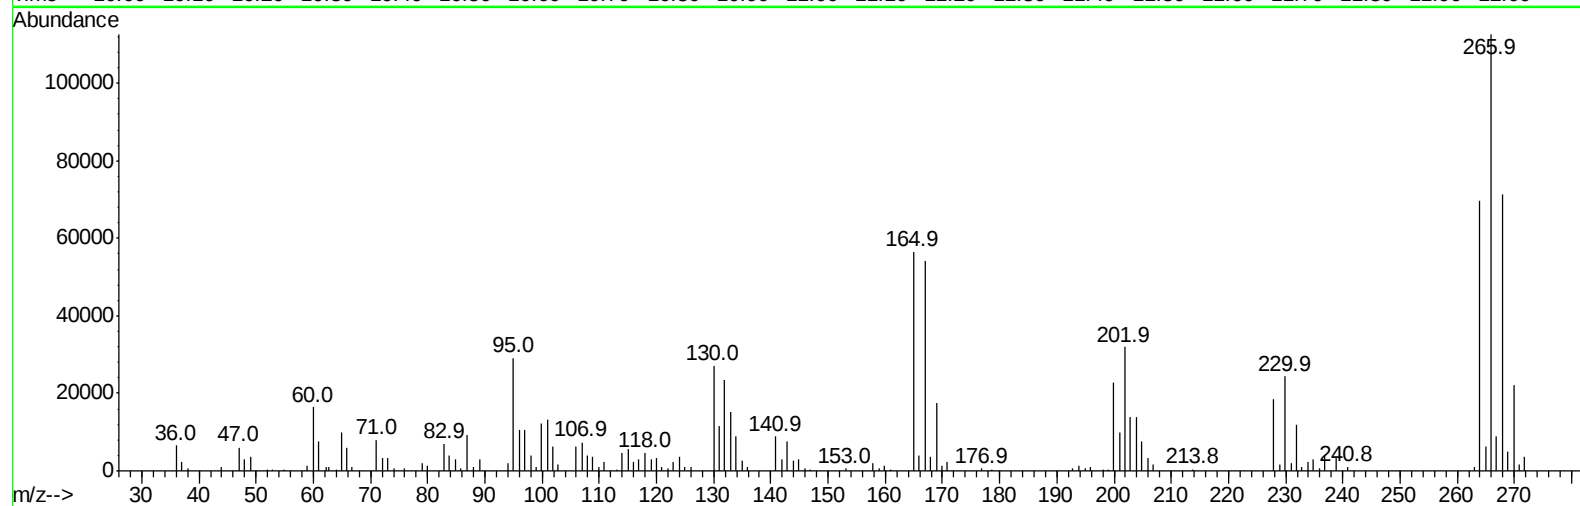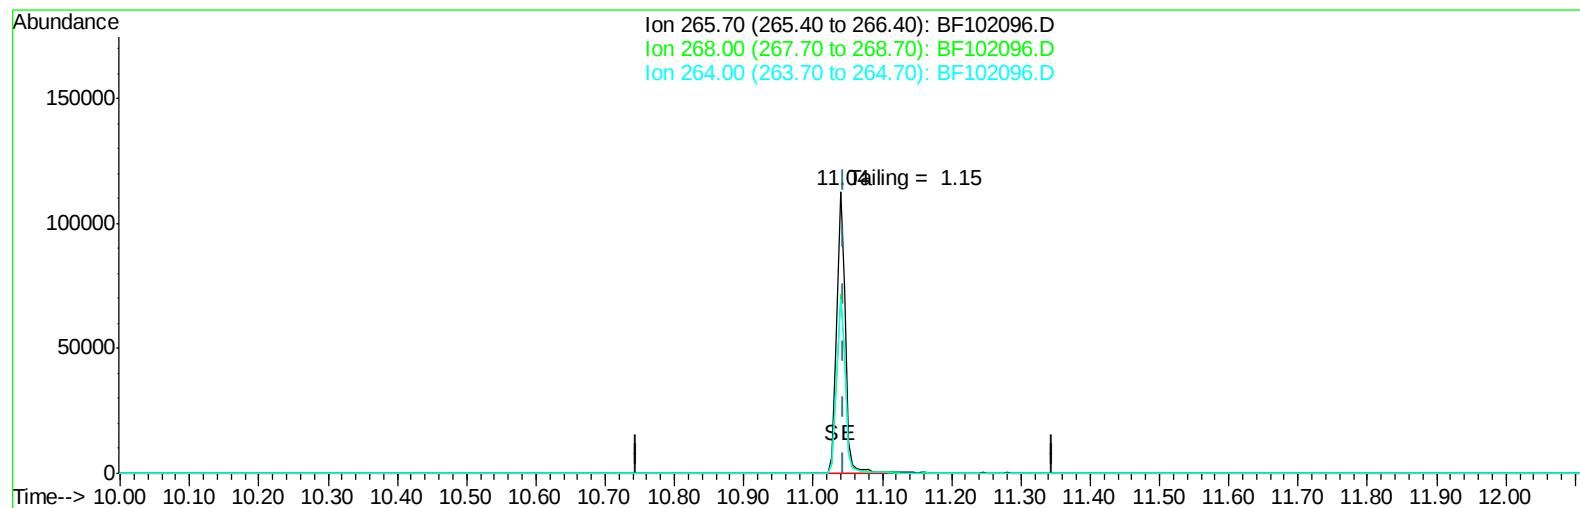

TIC: BF102096.D

(69) Pentachlorophenol (C)



11.039min (-0.006) 42408.48ng

response 94211

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.48
264.00	61.90	61.83
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA F\DATA\BF011618\
Data File : BF102096.D
Acq On : 16 Jan 2018 9:16
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 17 07:00:12 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 11 12:53:54 2018
Response via : Initial Calibration

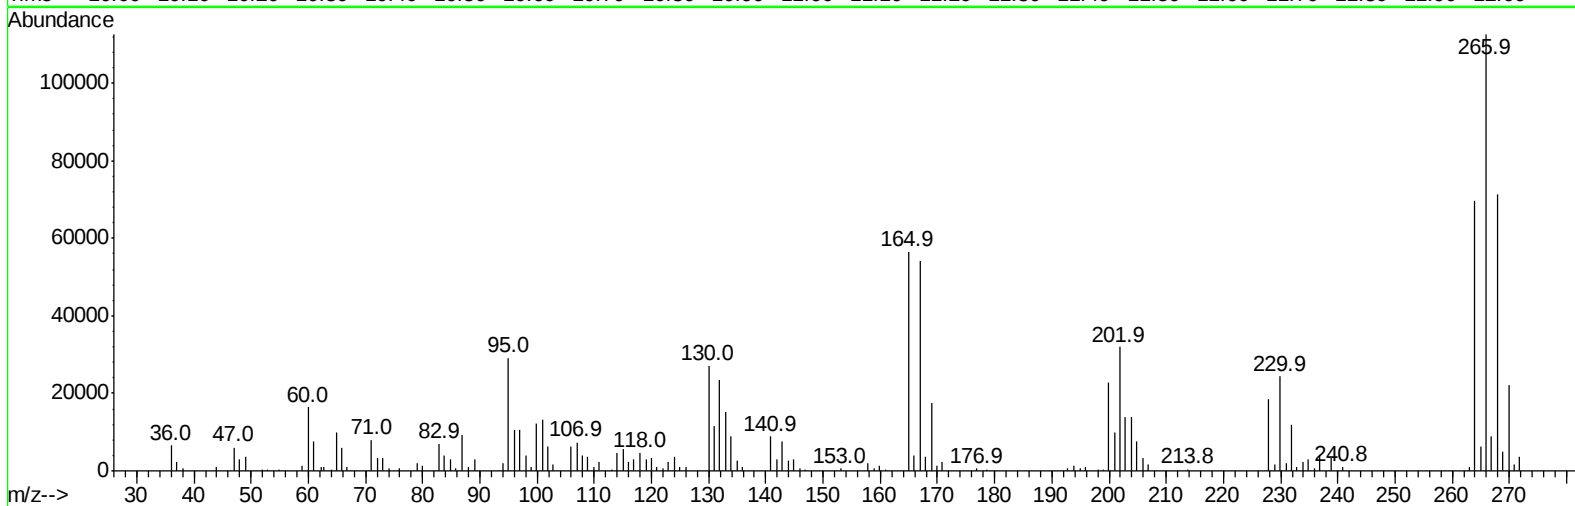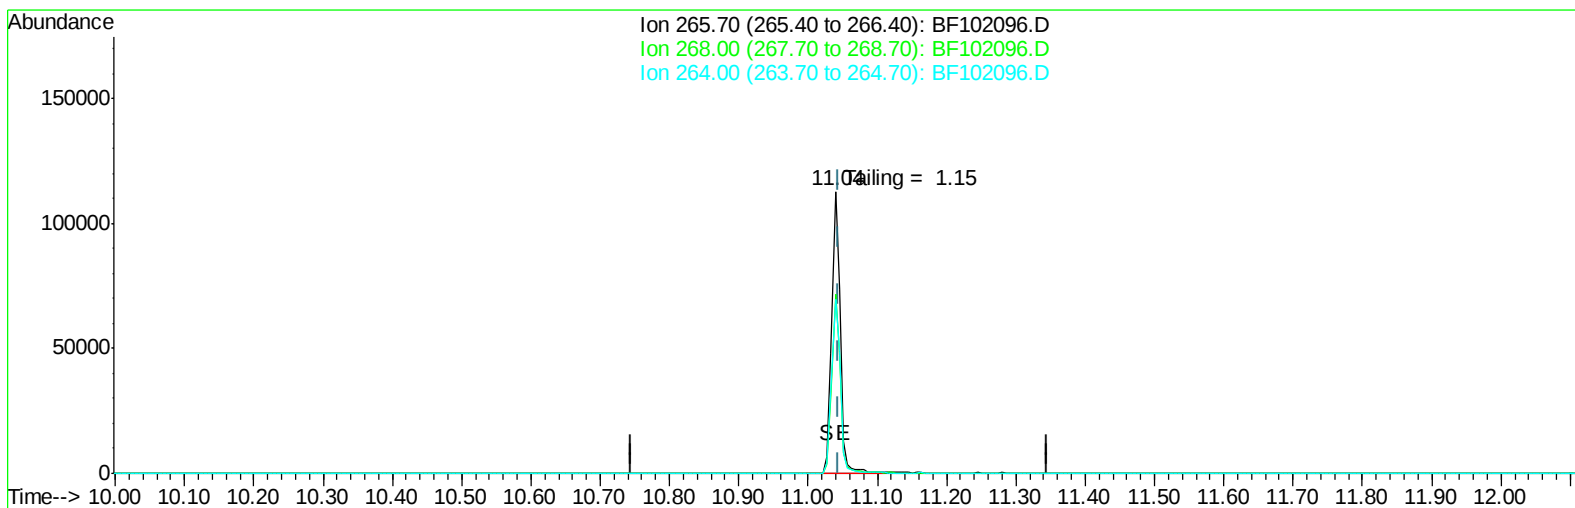

TIC: BF102096.D

(69) Pentachlorophenol (C)

11.039min (-0.006) 42408.48ng

response 94211

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.48
264.00	61.90	61.83
0.00	0.00	0.00