
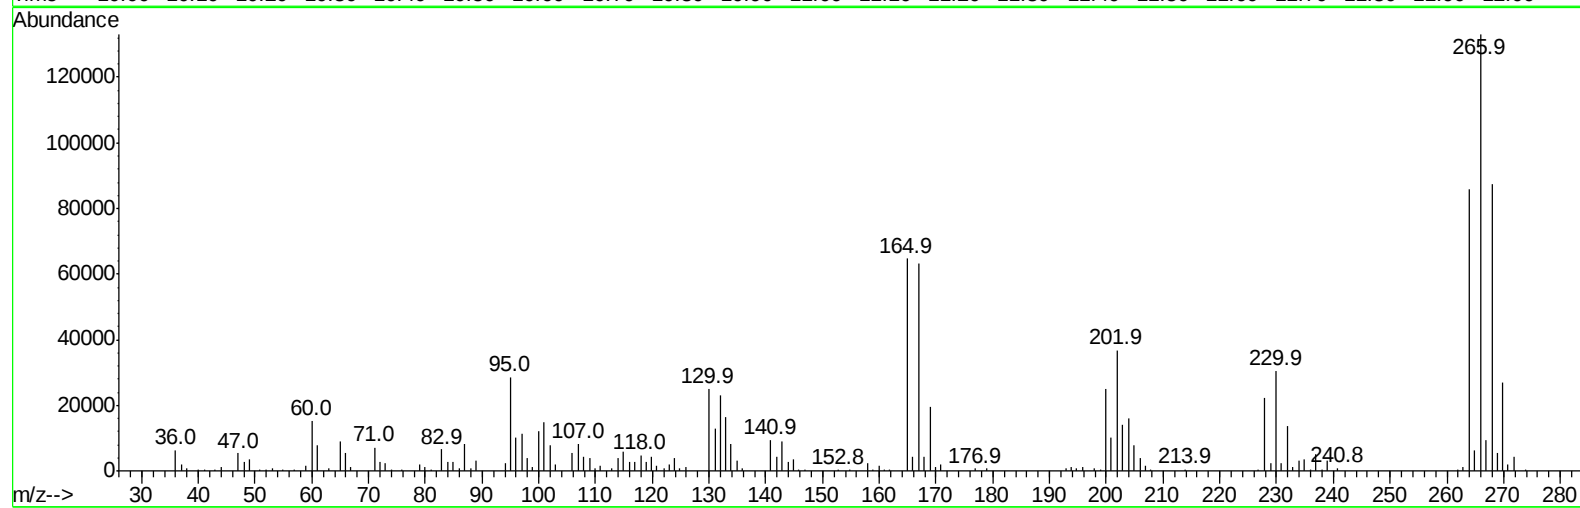


Data Path : U:\HPCHEM1\BNA F\DATA\BF011618\
Data File : BF102112.D
Acq On : 16 Jan 2018 16:30
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 17 07:03:10 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 11 12:53:54 2018
Response via : Initial Calibration

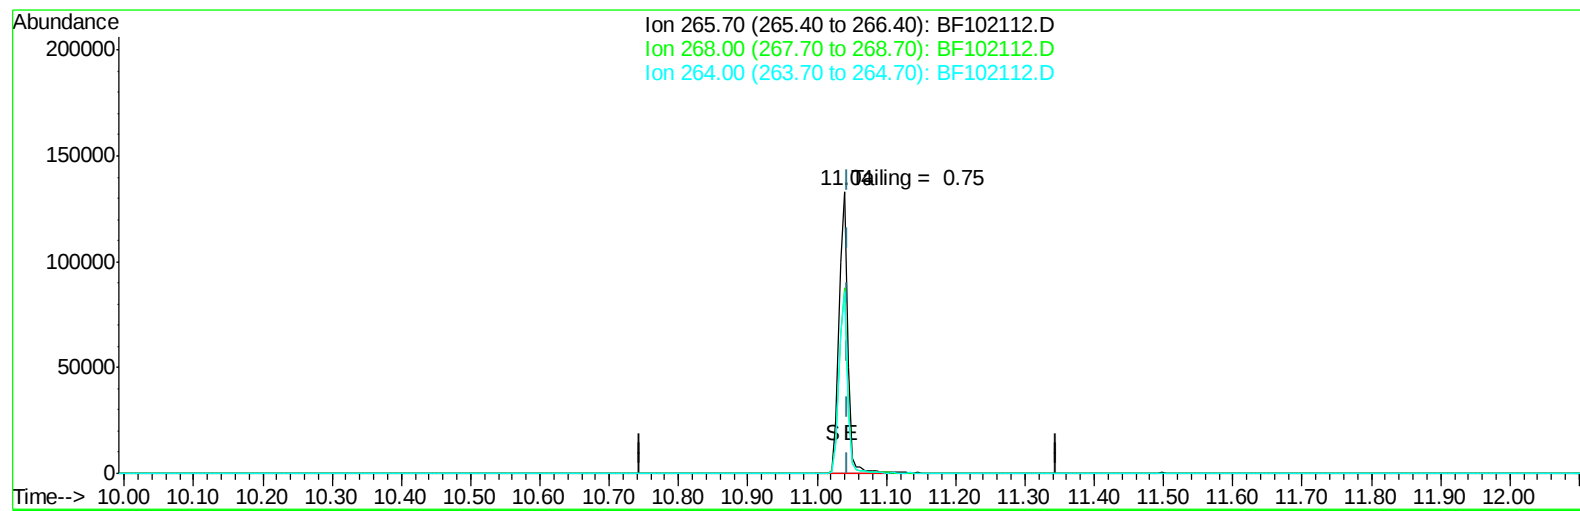

TIC: BF102112.D

(69) Pentachlorophenol (C)



11.039min (-0.006) 35613.99ng

response 115671

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.82
264.00	61.90	64.46
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA F\DATA\BF011618\
Data File : BF102112.D
Acq On : 16 Jan 2018 16:30
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 17 07:03:10 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 11 12:53:54 2018
Response via : Initial Calibration

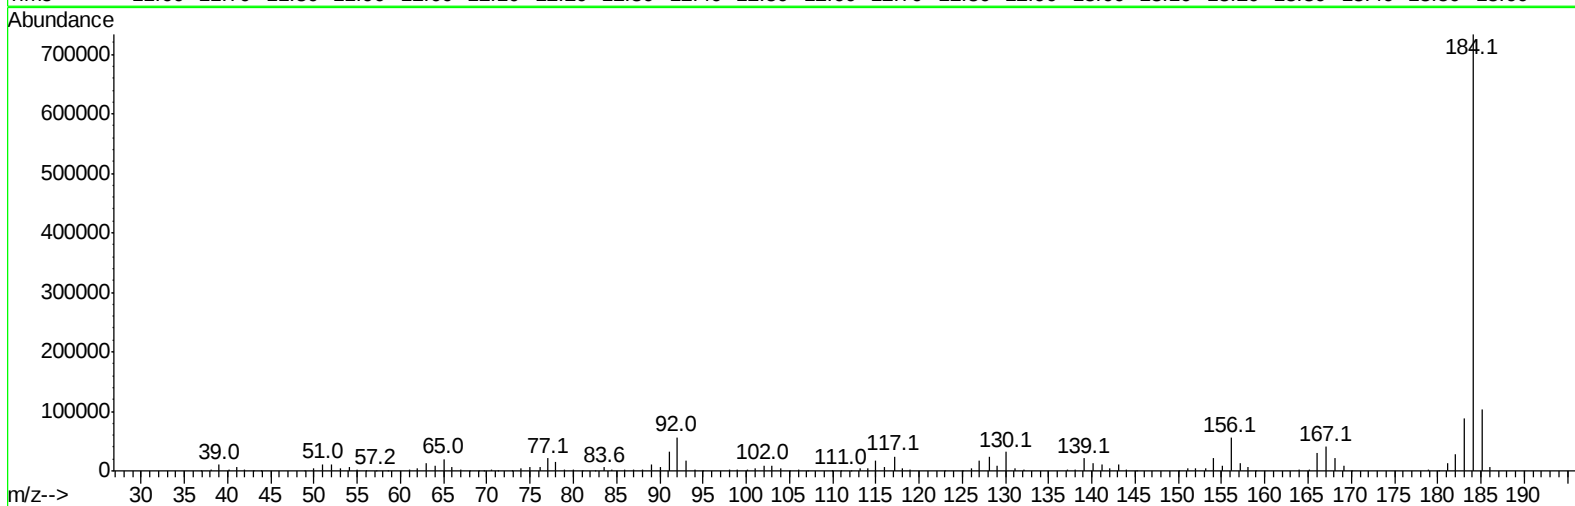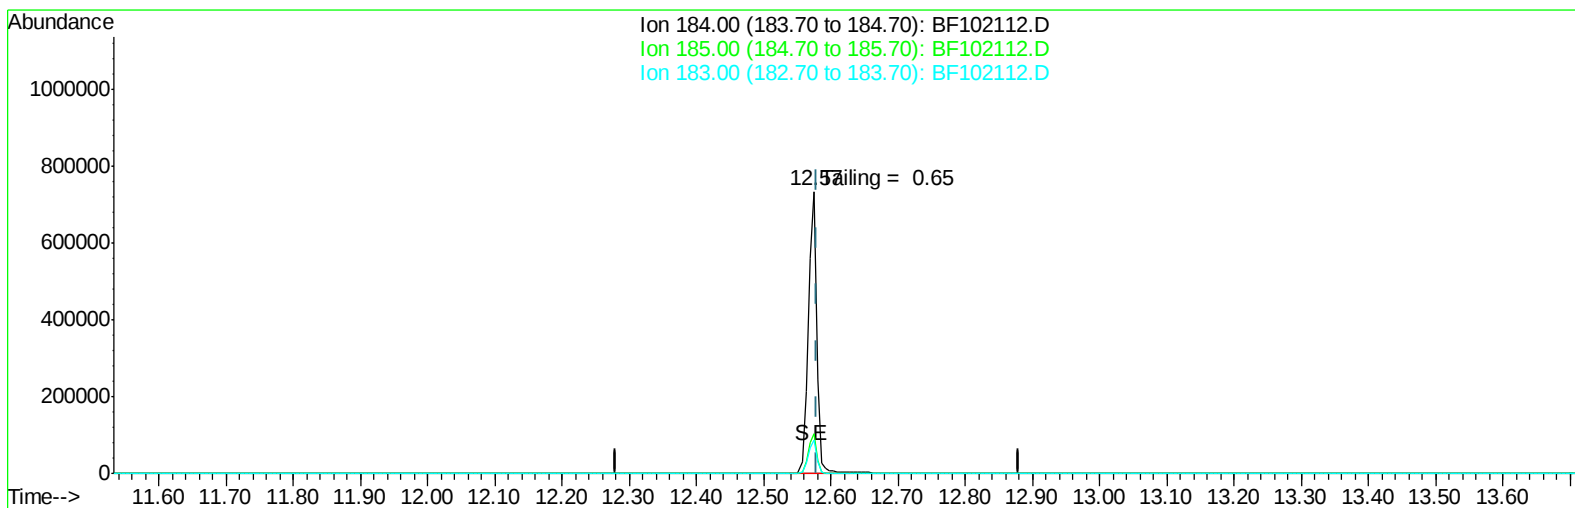

TIC: BF102112.D

(76) Benzidine

12.574min (-0.006) 0.00ng

response 659692

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.22
183.00	11.60	11.96
0.00	0.00	0.00