
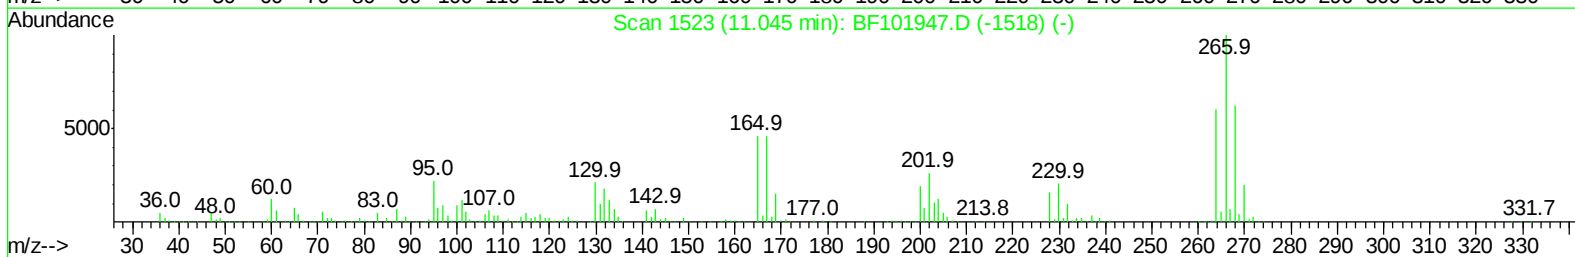
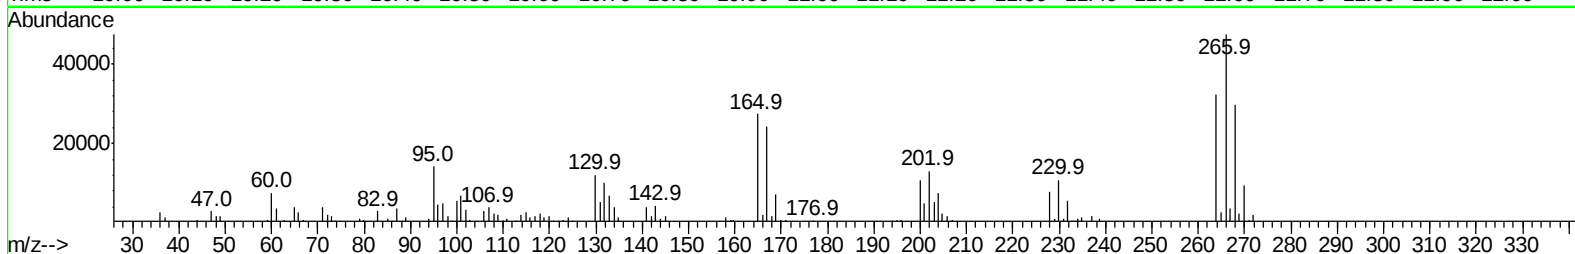


Data Path : U:\HPCHEM1\BNA F\DATA\BF011618\
Data File : BF102139.D
Acq On : 17 Jan 2018 5:03
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 17 07:04:19 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 11 12:53:54 2018
Response via : Initial Calibration

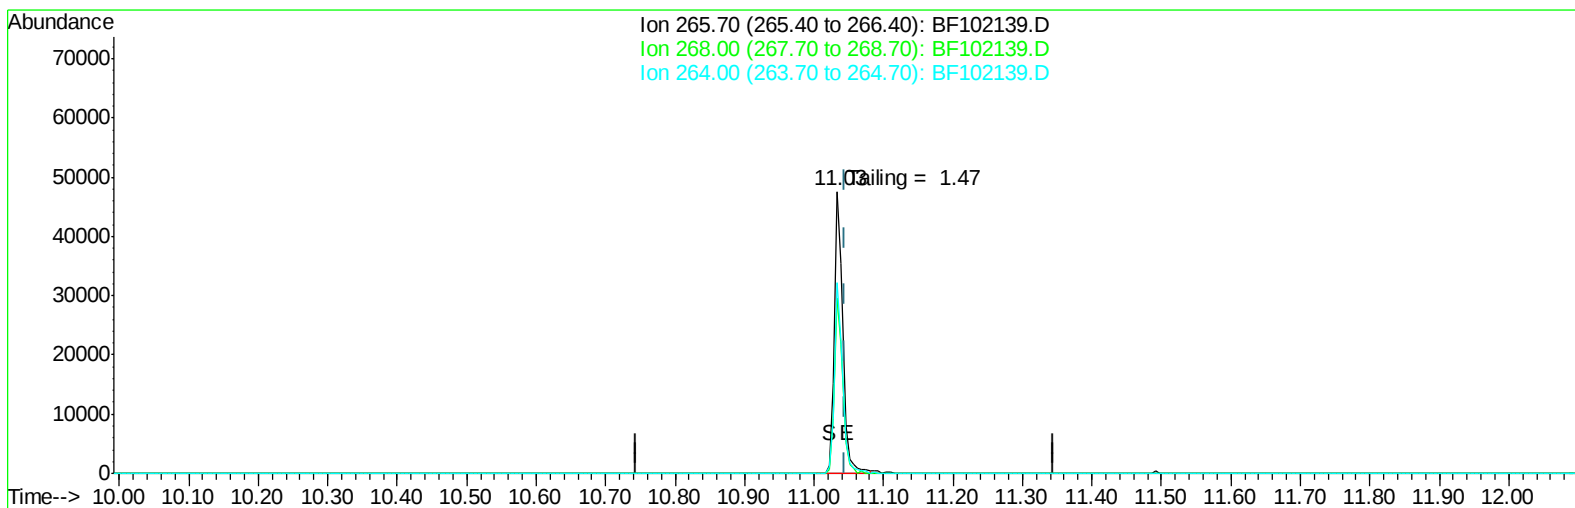

TIC: BF102139.D

(69) Pentachlorophenol (C)




11.033min (-0.012) 24012.09ng

response 40345

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.32
264.00	61.90	67.74
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA F\DATA\BF011618\
Data File : BF102139.D
Acq On : 17 Jan 2018 5:03
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 17 07:04:19 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 11 12:53:54 2018
Response via : Initial Calibration

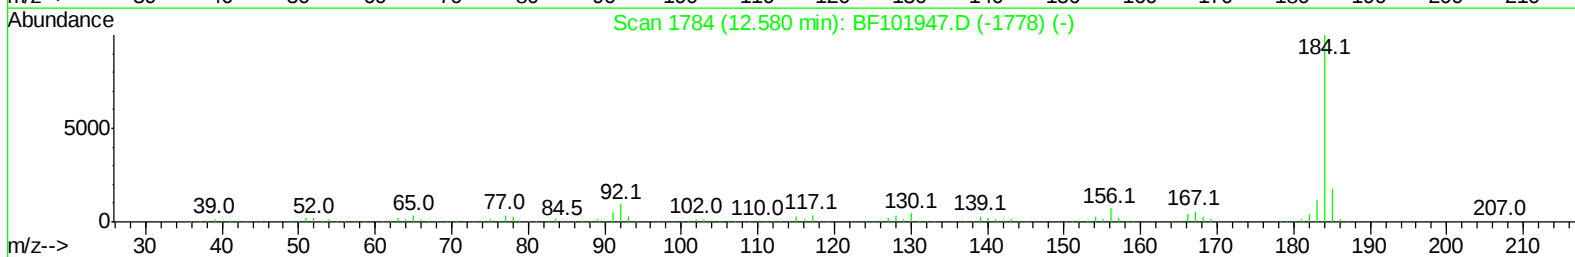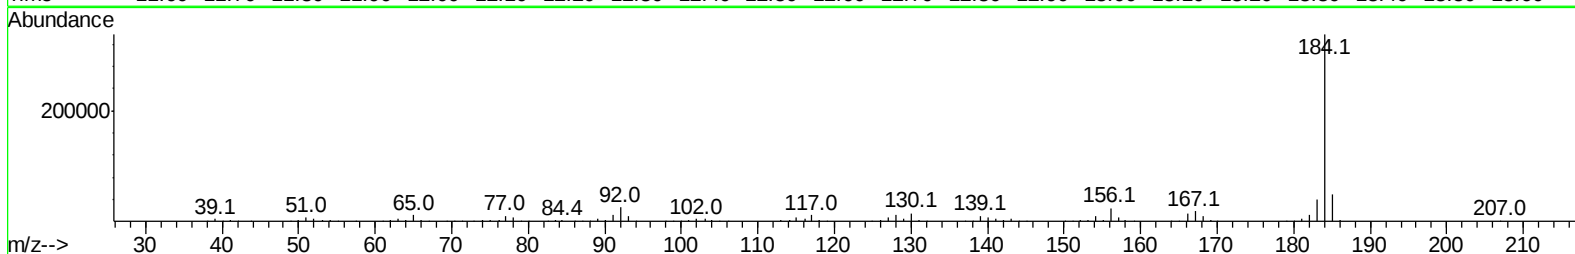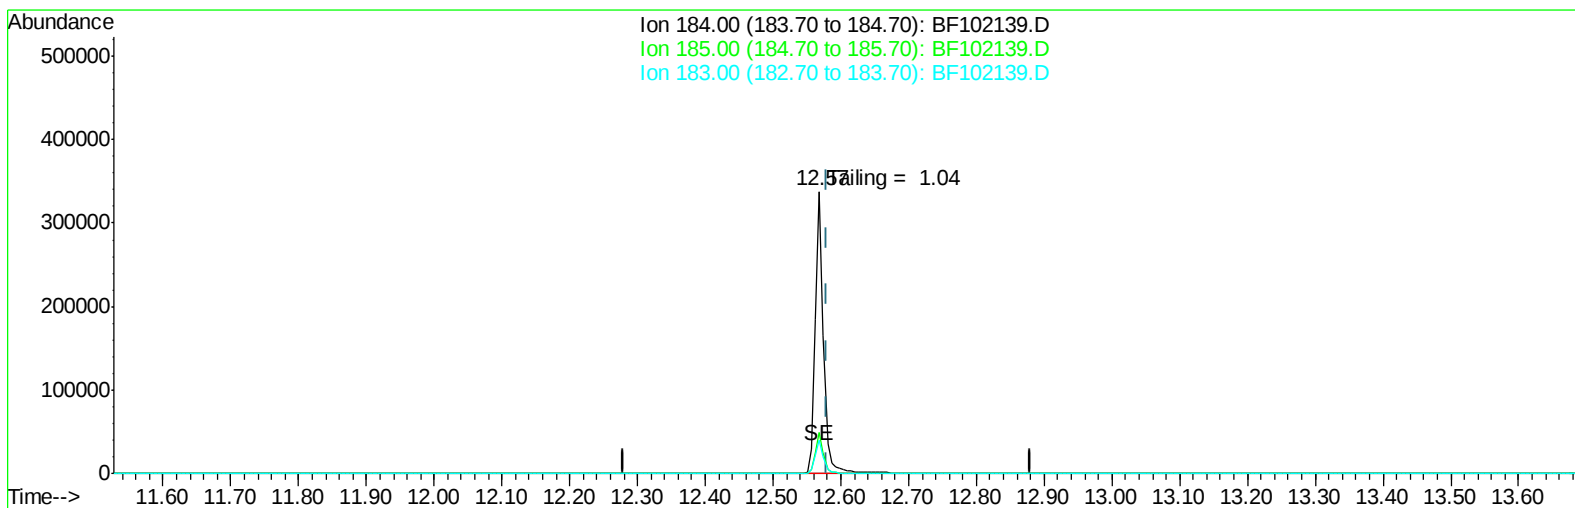

TIC: BF102139.D

(76) Benzidine

12.569min (-0.012) 0.00ng

response 283082

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.78
183.00	11.60	11.87
0.00	0.00	0.00