


Data Path : U:\HPCHEM1\BNA F\Data\BF011618\
 Data File : BF102096.D
 Acq On : 16 Jan 2018 9:16
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF010918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 11 12:53:54 2018

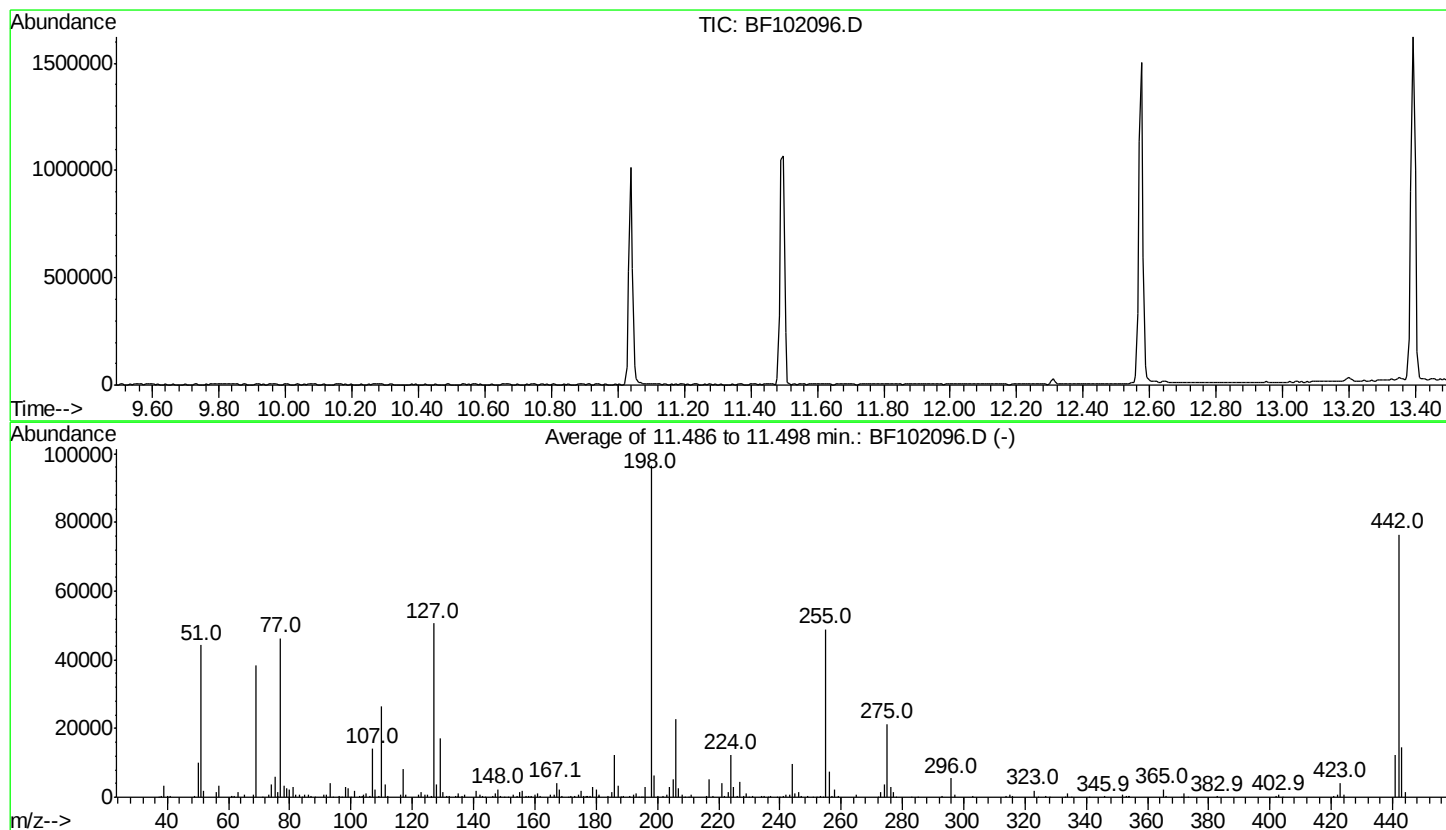

AutoFind: Scans 1598, 1599, 1600; Background Corrected with Scan 1594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.9	44354	PASS
68	69	0.00	2	1.7	646	PASS
69	198	0.00	100	39.9	38509	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.4	50586	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	96554	PASS
199	198	5	9	6.6	6407	PASS
275	198	10	60	22.1	21299	PASS
365	198	1	100	2.5	2385	PASS
441	443	0.01	100	83.3	12247	PASS
442	198	50	100	79.2	76464	PASS
443	442	15	24	19.2	14710	PASS