


Data Path : U:\HPCHEM1\BNA_F\Data\BF011618\
 Data File : BF102139.D
 Acq On : 17 Jan 2018 5:03
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF010918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 11 12:53:54 2018

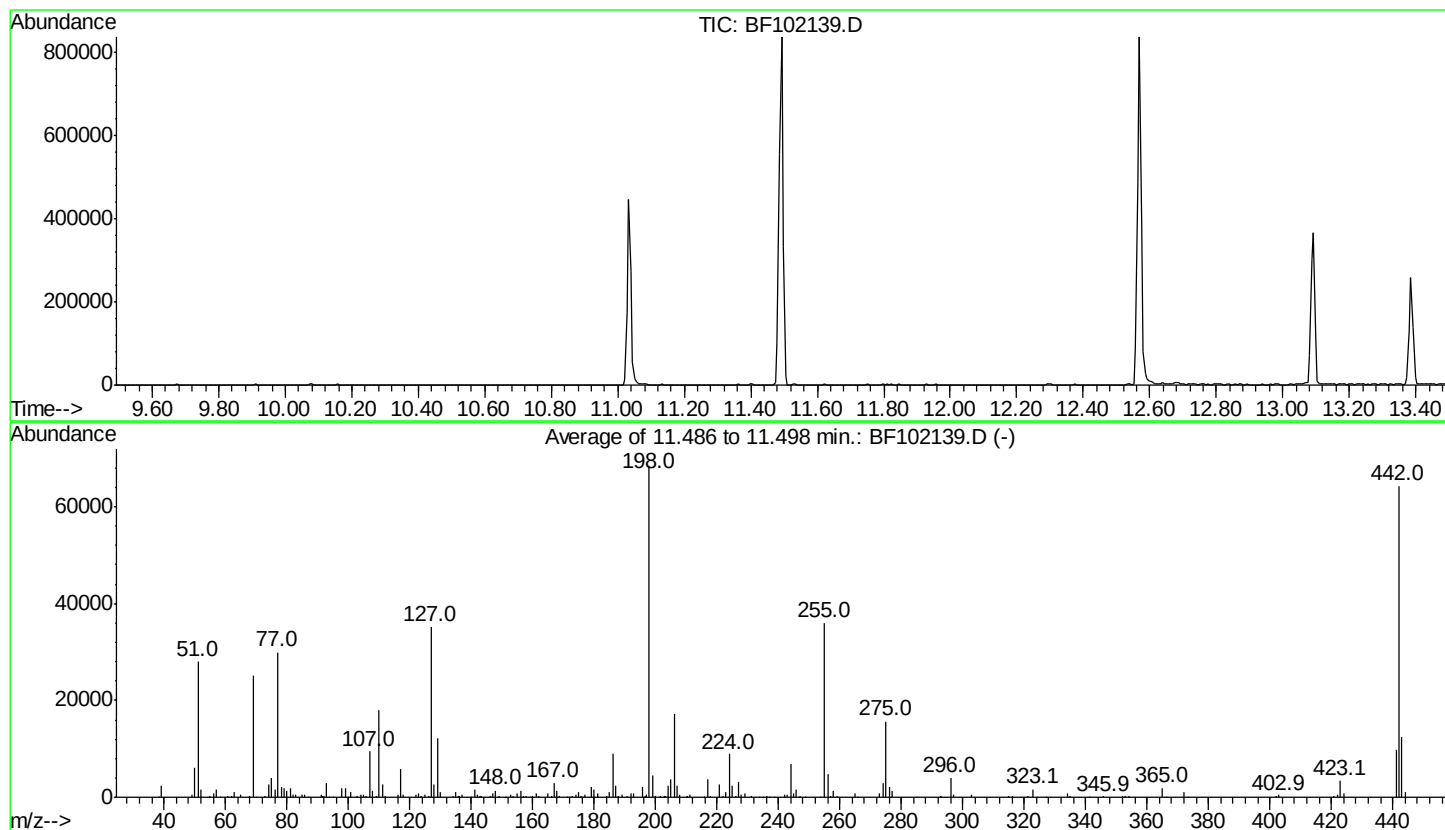

AutoFind: Scans 1598, 1599, 1600; Background Corrected with Scan 1593

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.8	27938	PASS
68	69	0.00	2	1.4	349	PASS
69	198	0.00	100	36.5	24996	PASS
70	69	0.00	2	0.4	106	PASS
127	198	10	80	51.5	35267	PASS
197	198	0.00	2	0.6	438	PASS
198	198	100	100	100.0	68488	PASS
199	198	5	9	6.5	4435	PASS
275	198	10	60	22.8	15616	PASS
365	198	1	100	2.8	1947	PASS
441	443	0.01	100	79.1	9746	PASS
442	198	50	100	93.8	64266	PASS
443	442	15	24	19.2	12318	PASS