
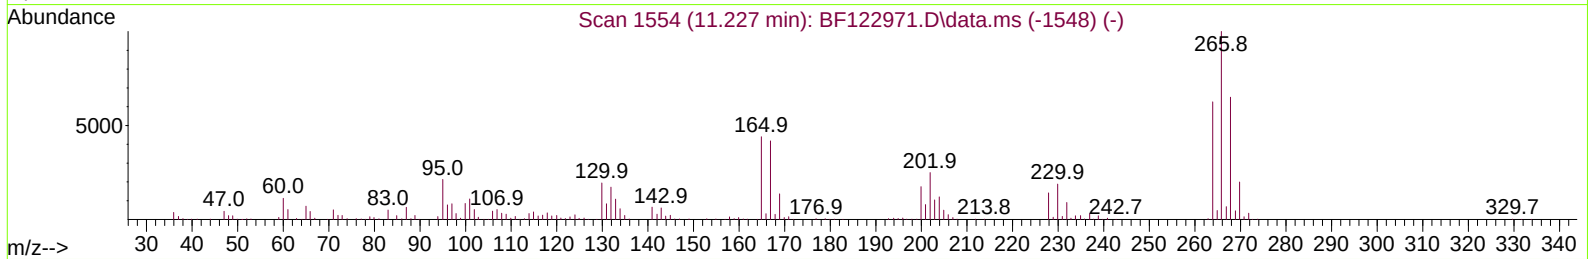
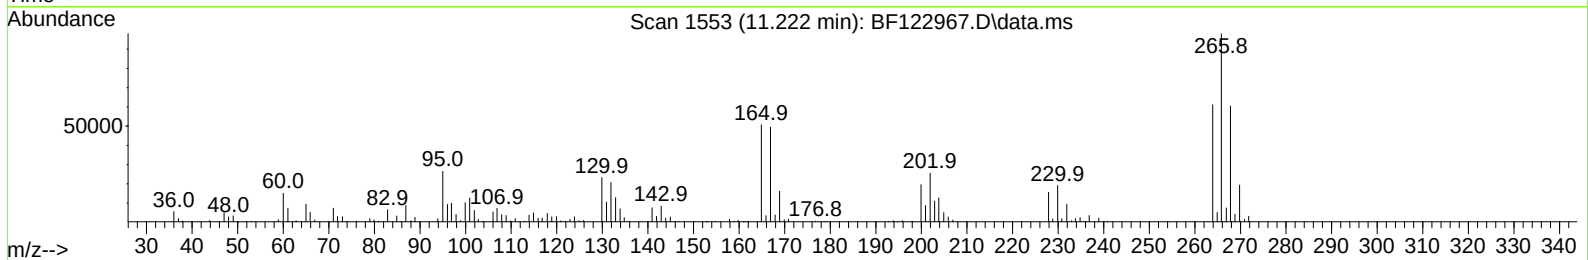


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011621\
 Data File : BF122967.D
 Acq On : 15 Jan 2021 17:18
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 19 07:47:17 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF011621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 18 13:14:08 2021
 Response via : Initial Calibration

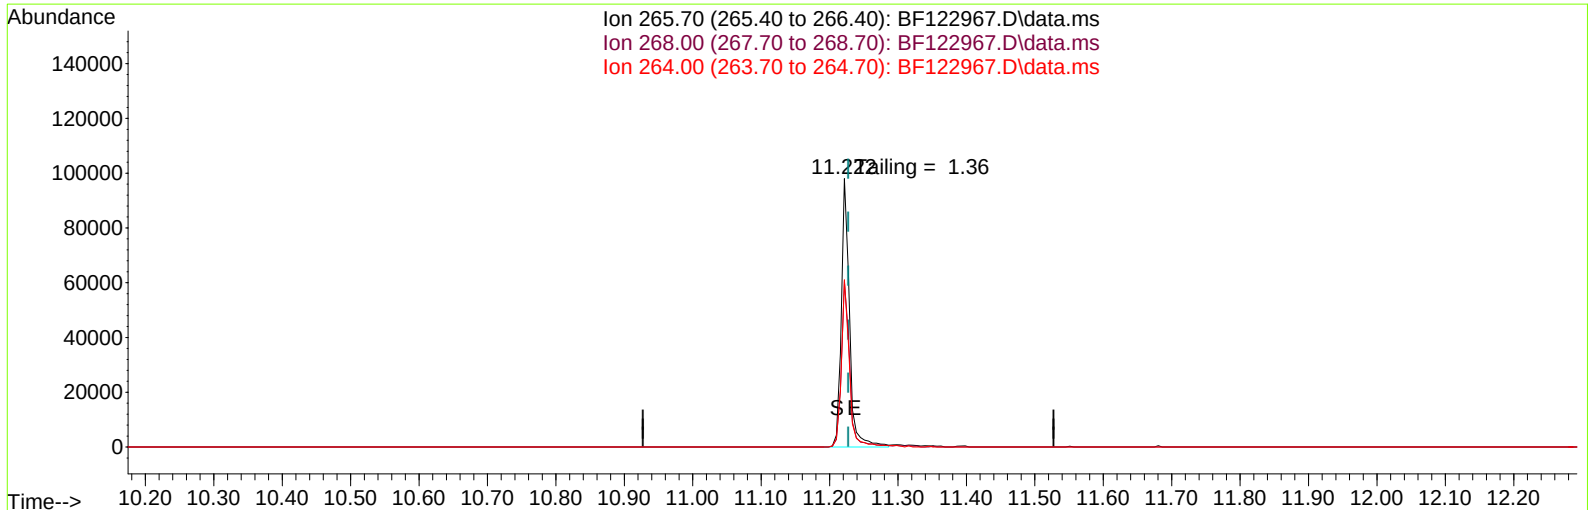

TIC: BF122967.D\data.ms

(70) Pentachlorophenol (C)




11.222min (-0.006) 31176.26 ng

response 82526

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	61.66
264.00	62.30	62.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011621\
Data File : BF122967.D
Acq On : 15 Jan 2021 17:18
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 19 07:47:17 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF011621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 18 13:14:08 2021
Response via : Initial Calibration

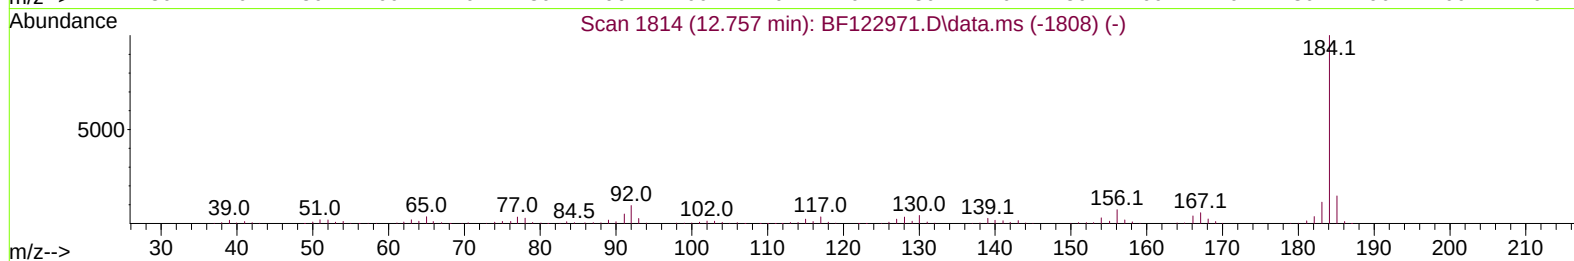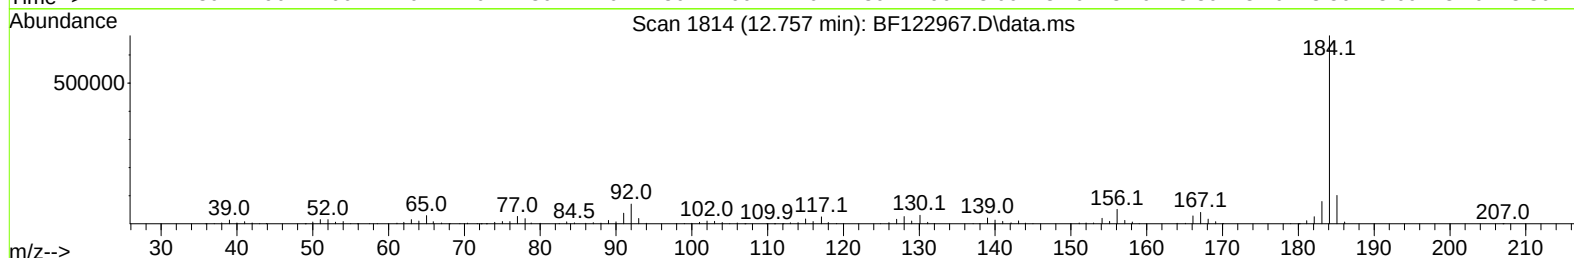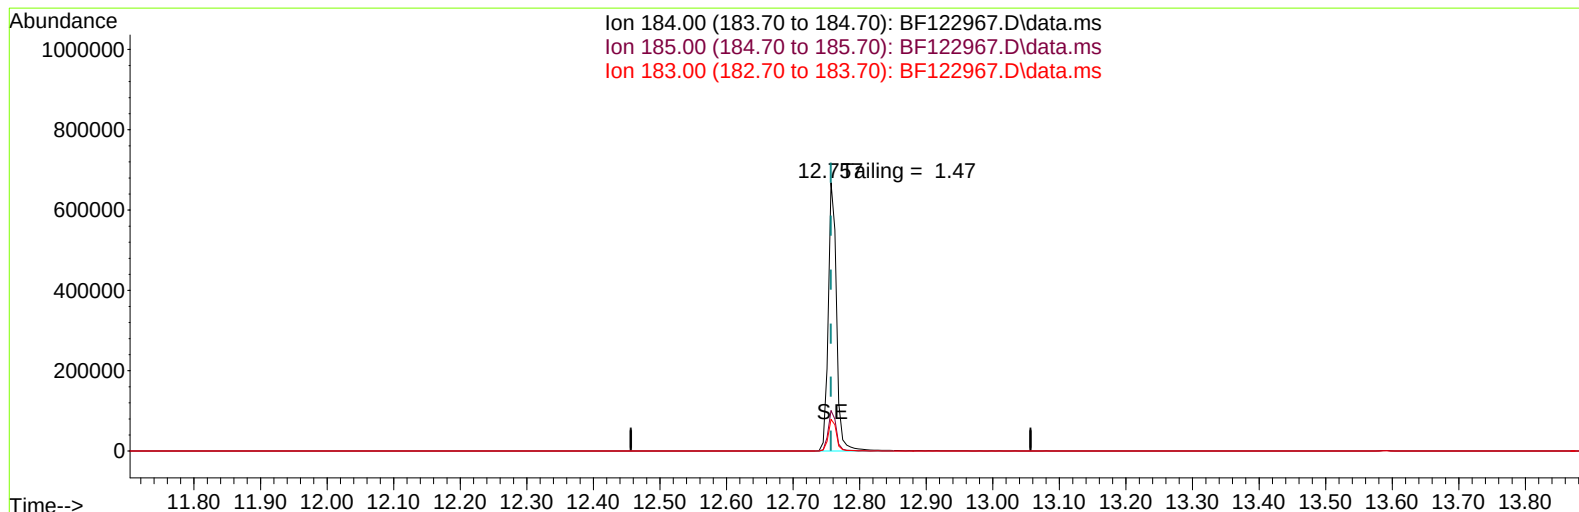

TIC: BF122967.D\data.ms

(77) Benzidine

12.757min (+ 0.000) 0.00 ng

response 584765

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	15.09
183.00	12.10	11.84
0.00	0.00	0.00