
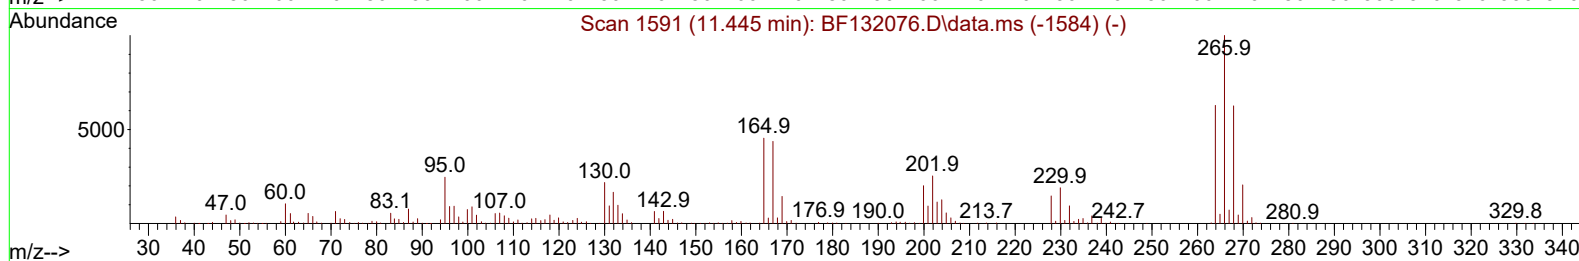
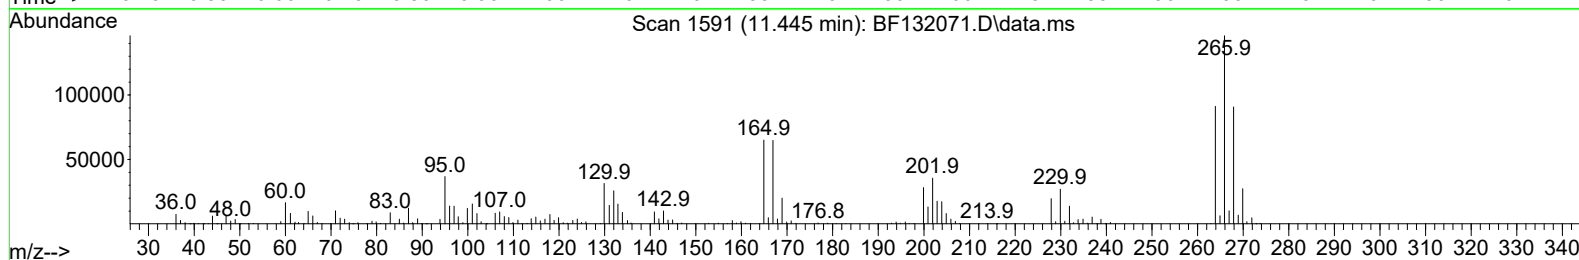


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011623\  
Data File : BF132071.D  
Acq On    : 16 Jan 2023   15:35  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Jan 17 08:06:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 17 01:48:42 2023
Response via : Initial Calibration

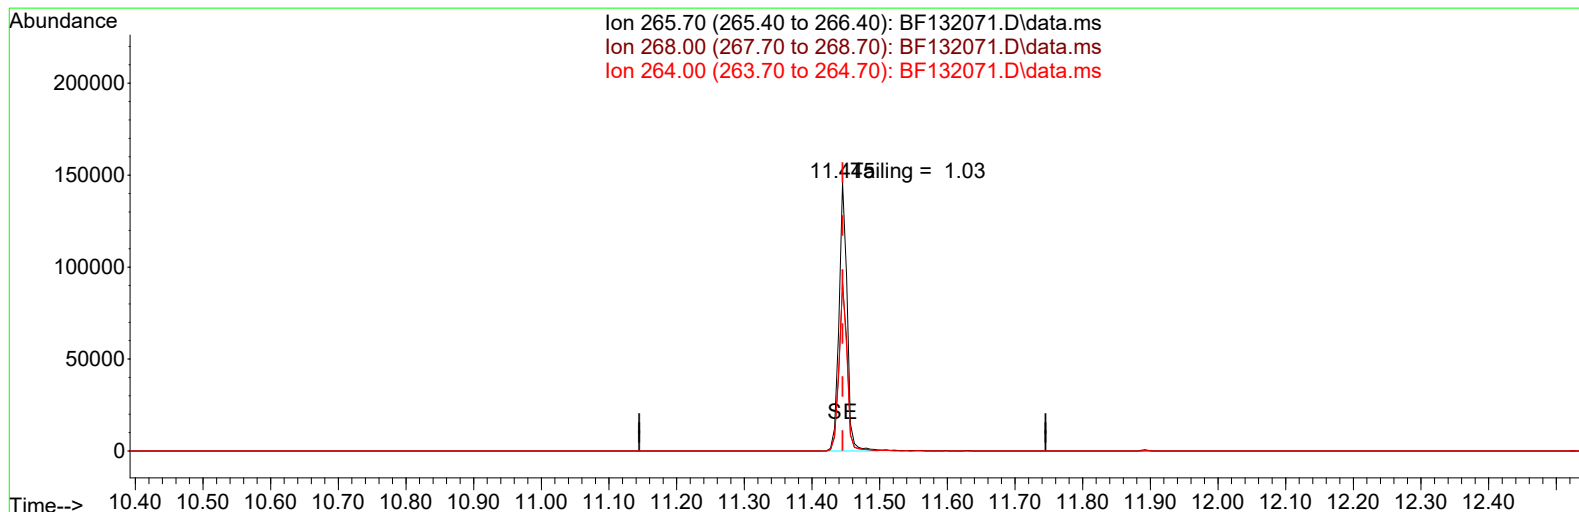

TIC: BF132071.D\data.ms

(70) Pentachlorophenol (C)




11.445min (+ 0.000) 26198.72 ng

response **122936**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.50	62.19
264.00	62.80	62.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011623\
Data File : BF132071.D
Acq On : 16 Jan 2023 15:35
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 17 08:06:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 17 01:48:42 2023
Response via : Initial Calibration

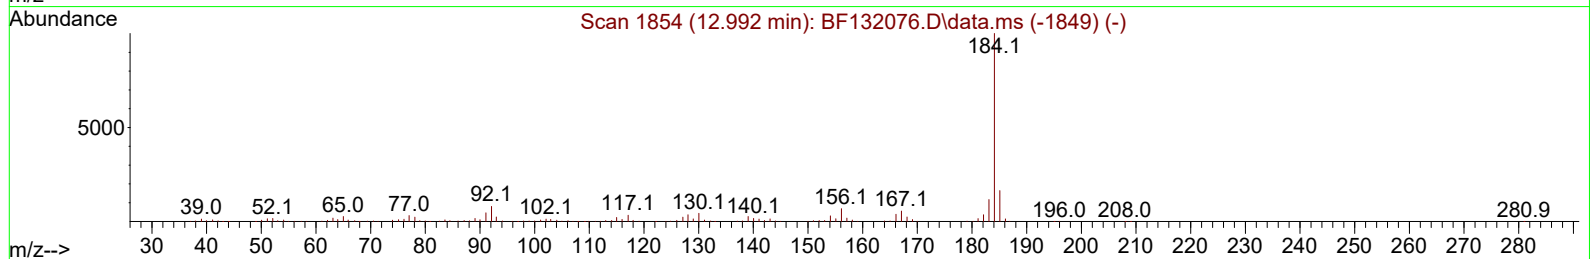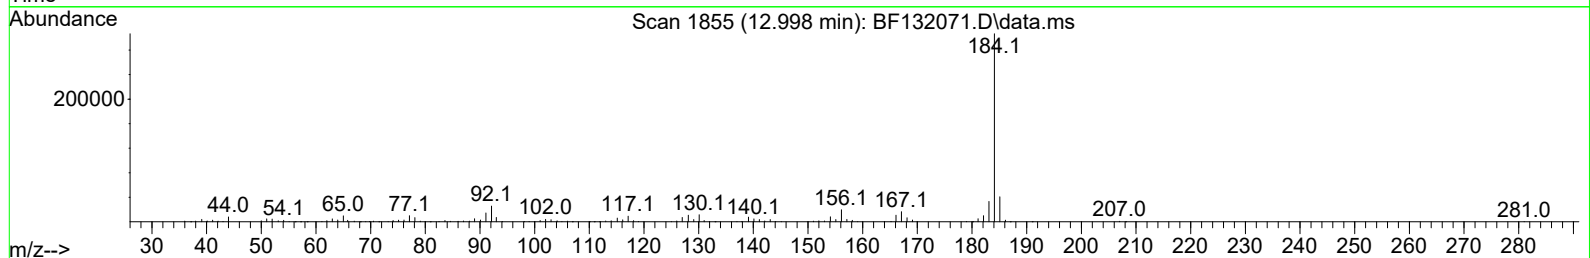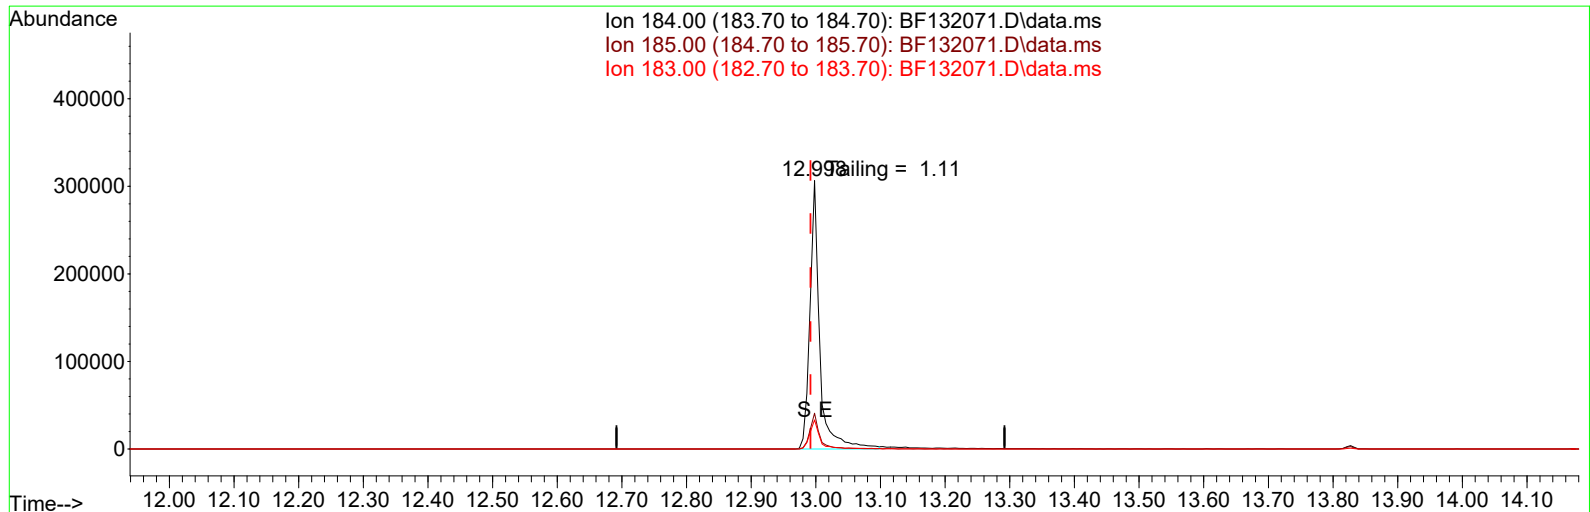

TIC: BF132071.D\data.ms

(77) Benzidine

12.998min (+ 0.006) 0.00 ng

response 333103

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.40	13.34
183.00	11.70	10.87
0.00	0.00	0.00