

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011623\
 Data File : BF132086.D
 Acq On : 17 Jan 2023 00:16
 Operator : CG\JU
 Sample : PB150154TB
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB150154TB

Quant Time: Jan 17 06:52:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 17 01:48:42 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	0.000	152	0	0.000	ng	-7.10
21) Naphthalene-d8	0.000	136	0	0.000	ng	-8.39
39) Acenaphthene-d10	0.000	164	0	0.000	ng	-10.16
64) Phenanthrene-d10	0.000	188	0	0.000	ng	-11.65
76) Chrysene-d12	0.000	240	0	0.000	ng	-14.32
86) Perylene-d12	0.000	264	0	0.000	ng	-15.92
System Monitoring Compounds						
5) 2-Fluorophenol	0.000	112	0	0.000	ng	
7) Phenol-d6	0.000	99	0	0.000	ng	
23) Nitrobenzene-d5	0.000	82	0	0.000	ng	
42) 2,4,6-Tribromophenol	0.000	330	0	0.000	ng	
45) 2-Fluorobiphenyl	0.000	172	0	0.000	ng	
79) Terphenyl-d14	0.000	244	0	0.000	ng	


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011623\
Data File : BF132086.D
Acq On : 17 Jan 2023 00:16
Operator : CG\JU
Sample : PB150154TB
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB150154TB

Quant Time: Jan 17 06:52:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 17 01:48:42 2023
Response via : Initial Calibration

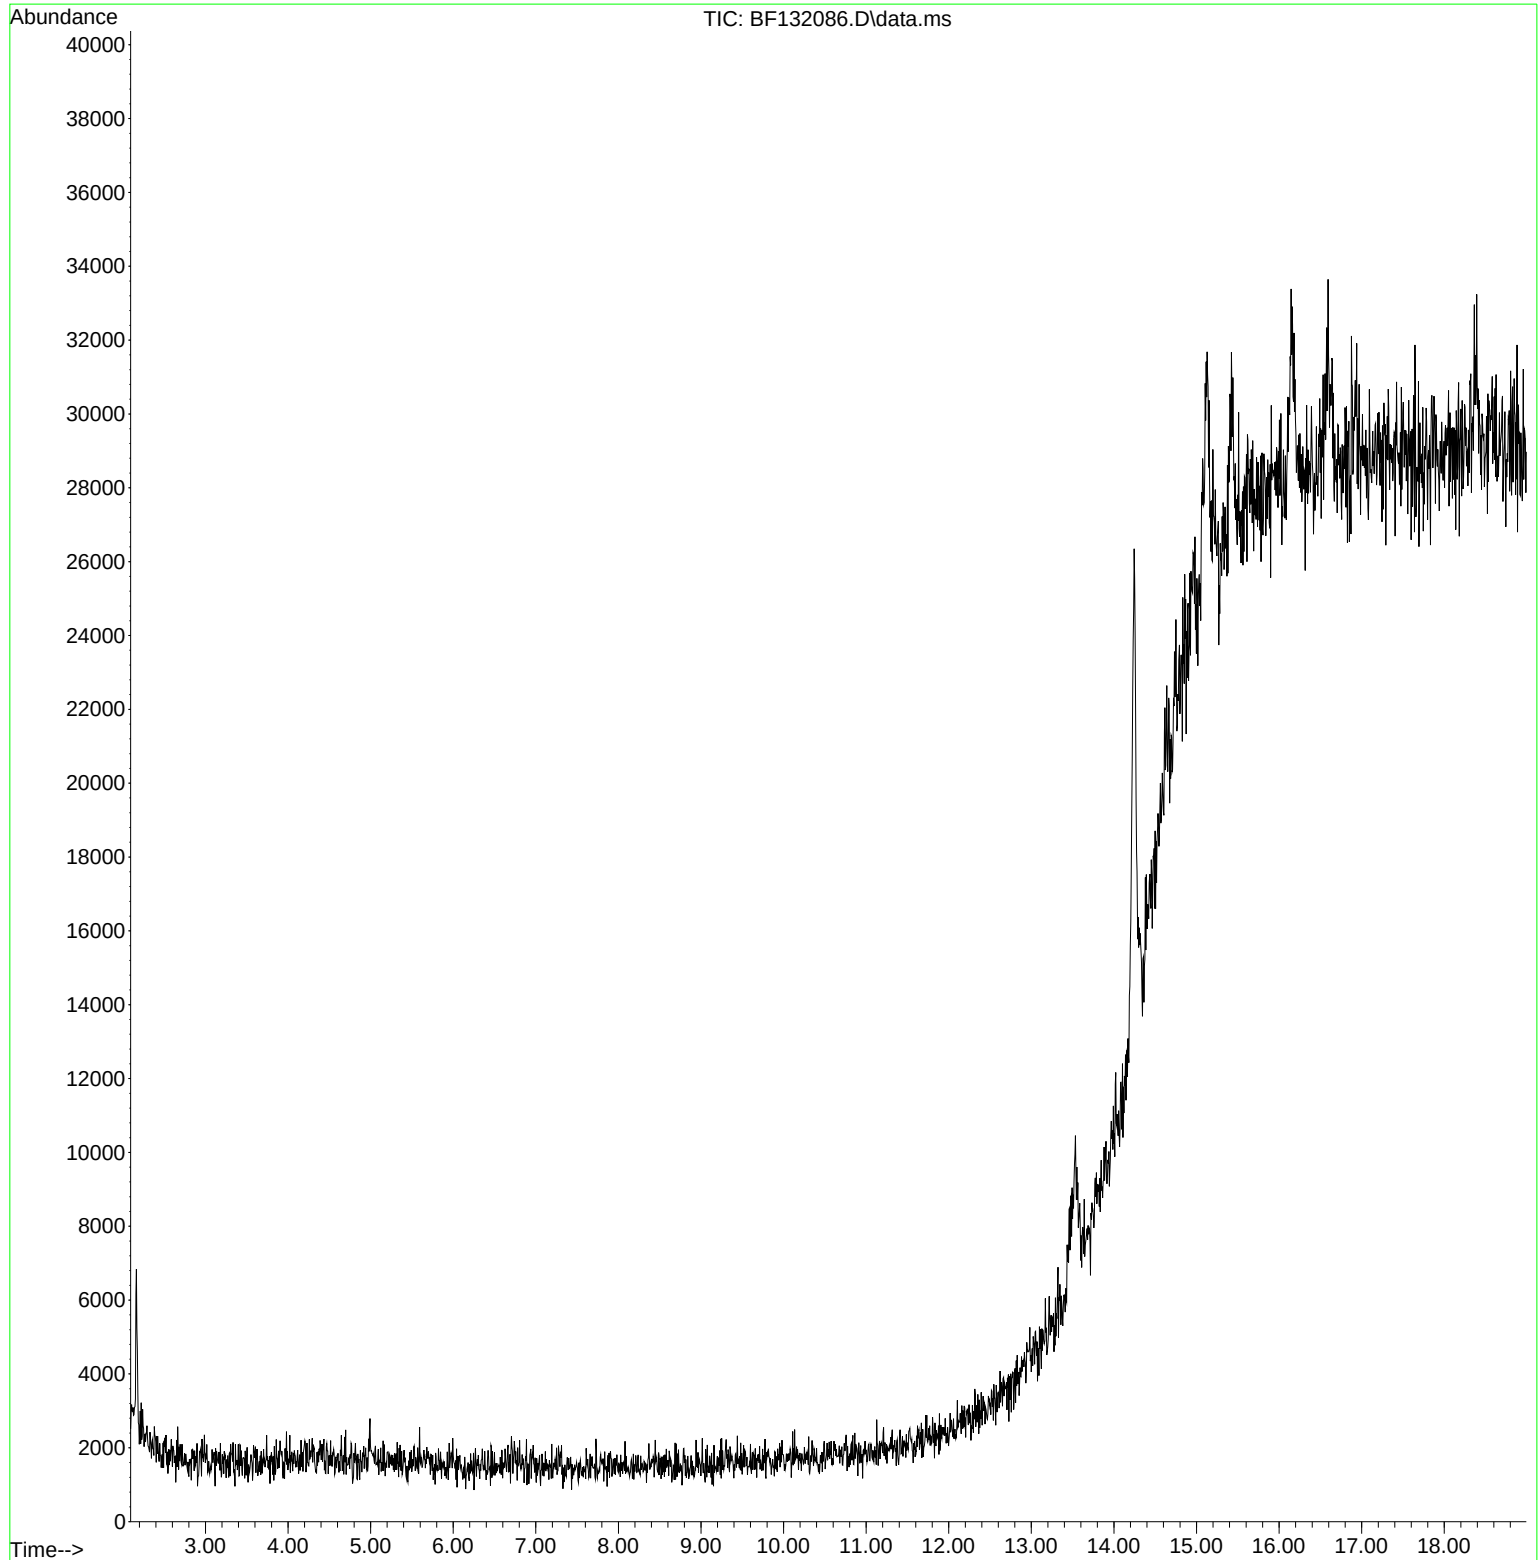


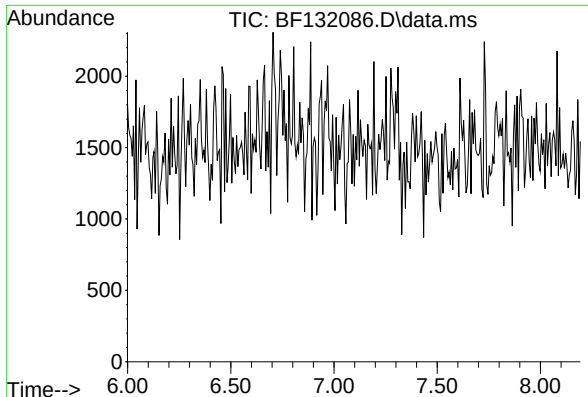


#1
 1,4-Dichlorobenzene-d4
 Concen: 0.000 ng
 Expected RT: 7.10 min
 Lab File: BF132086.D
 Acq: 17 Jan 2023 00:16

Instrument :
 BNA_F
 ClientSampleId :
 PB150154TB

Tgt Ion: 152


Sig	Exp Ratio
152	100
150	148.3
115	58.8

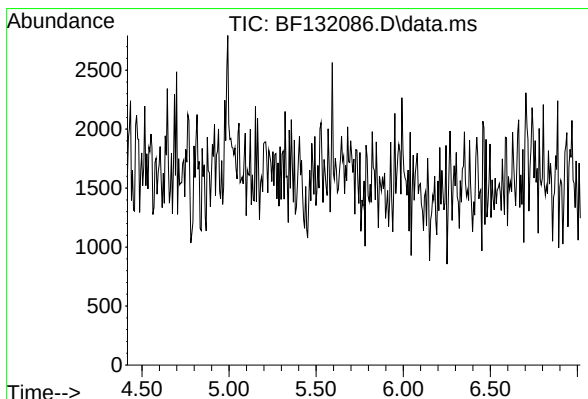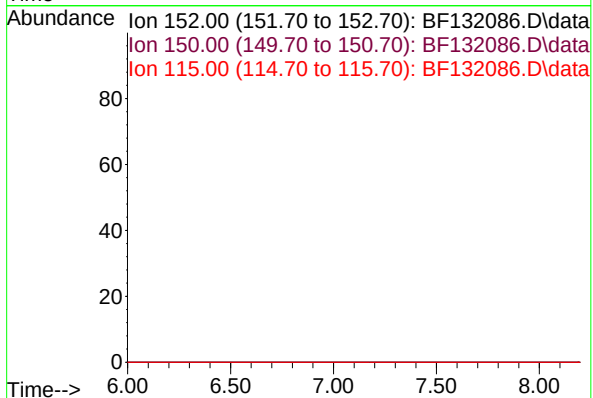


#5
 2-Fluorophenol
 Concen: 0.000 ng
 Expected RT: 5.72 min
 Lab File: BF132086.D
 Acq: 17 Jan 2023 00:16

Tgt Ion: 112

Sig	Exp Ratio
112	100
64	58.6
63	32.0

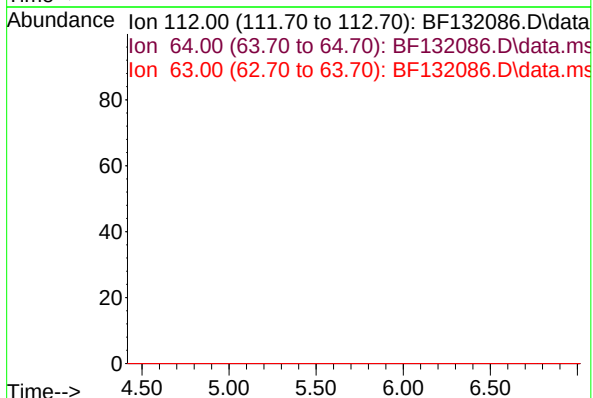


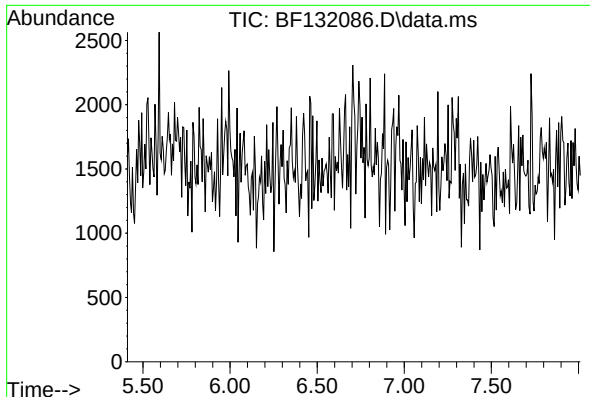


#7
 Phenol-d6
 Concen: 0.000 ng
 Expected RT: 6.71 min
 Lab File: BF132086.D
 Acq: 17 Jan 2023 00:16

Instrument :
 BNA_F
 ClientSampleId :
 PB150154TB

Tgt Ion: 99


Sig	Exp Ratio
99	100
42	17.5
71	35.3

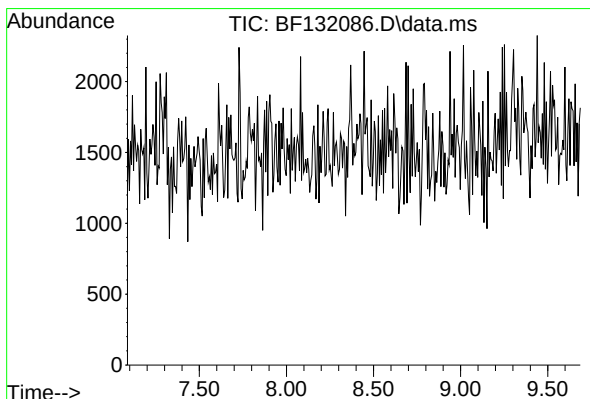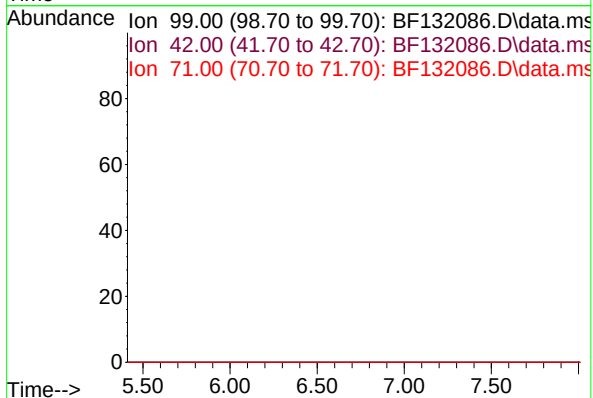


#21
 Naphthalene-d8
 Concen: 0.000 ng
 Expected RT: 8.39 min
 Lab File: BF132086.D
 Acq: 17 Jan 2023 00:16

Tgt Ion: 136

Sig	Exp Ratio
136	100
137	11.1
54	6.6
68	5.5


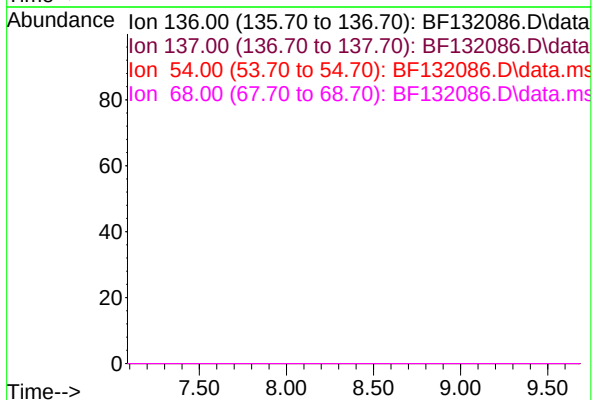


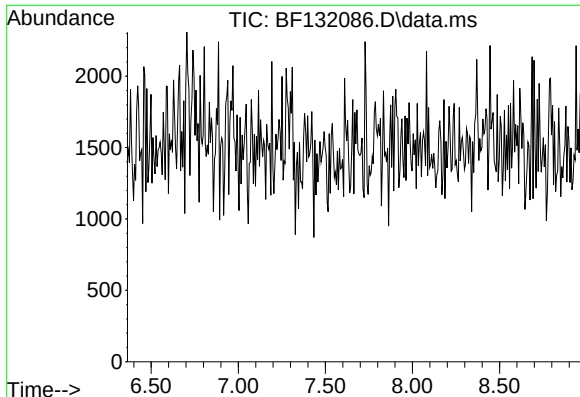

#23
 Nitrobenzene-d5
 Concen: 0.000 ng
 Expected RT: 7.66 min
 Lab File: BF132086.D
 Acq: 17 Jan 2023 00:16


Instrument :
 BNA_F
 ClientSampleId :
 PB150154TB


Tgt Ion: 82
 Sig Exp Ratio
 82 100
 128 40.7
 54 45.0

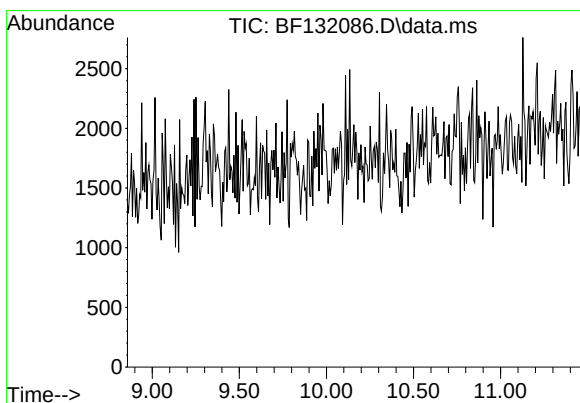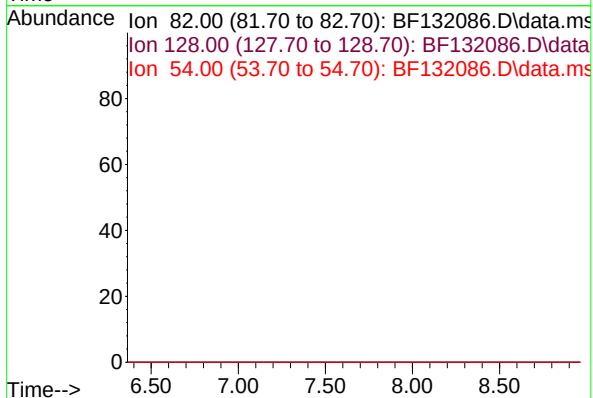

#39
 Acenaphthene-d10
 Concen: 0.000 ng
 Expected RT: 10.16 min
 Lab File: BF132086.D
 Acq: 17 Jan 2023 00:16

Tgt Ion: 164
 Sig Exp Ratio
 164 100
 162 101.9
 160 45.8

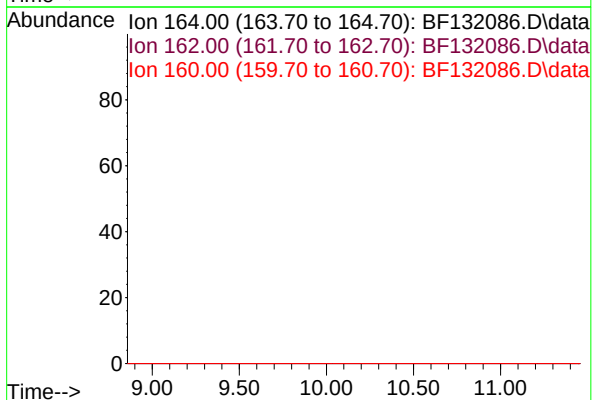


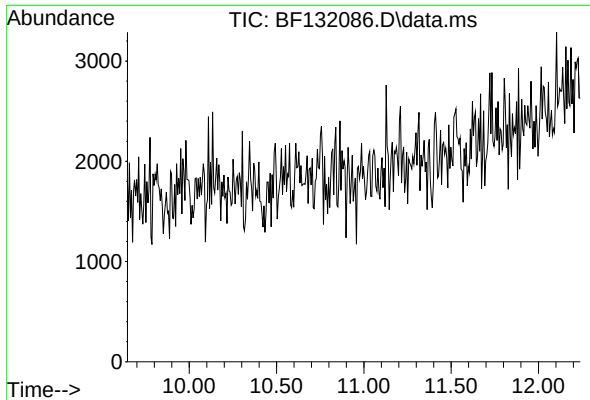


#42
2,4,6-Tribromophenol
Concen: 0.000 ng
Expected RT: 10.95 min

Lab File: BF132086.D
Acq: 17 Jan 2023 00:16

Instrument :
BNA_F
ClientSampleId :
PB150154TB


Tgt Ion: 330
Sig Exp Ratio
330 100
332 97.4
141 36.5

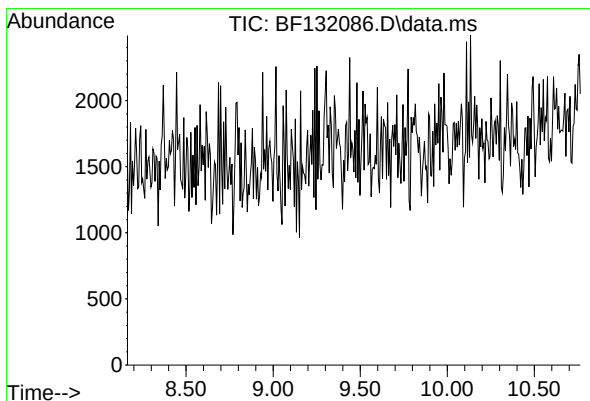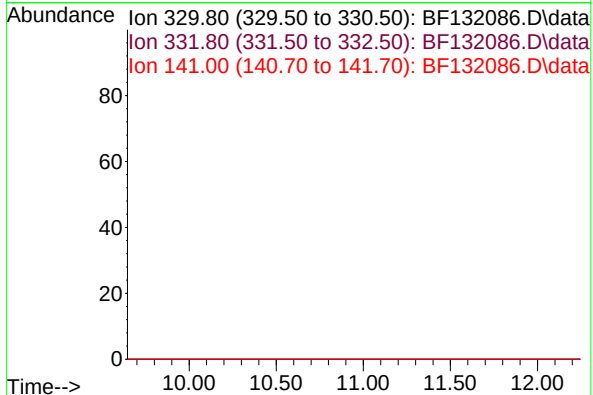


#45
2-Fluorobiphenyl
Concen: 0.000 ng
Expected RT: 9.46 min

Lab File: BF132086.D
Acq: 17 Jan 2023 00:16

Tgt Ion: 172
Sig Exp Ratio
172 100
171 35.9
170 24.4

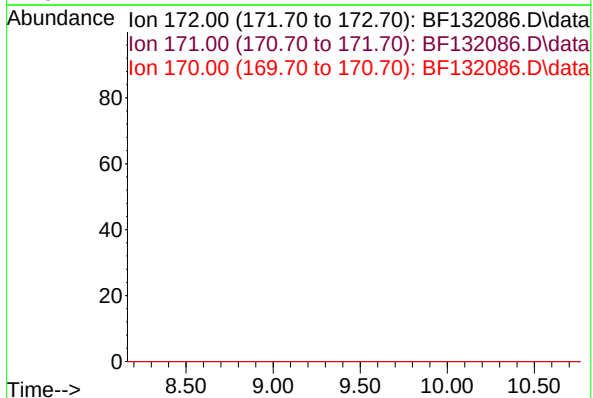


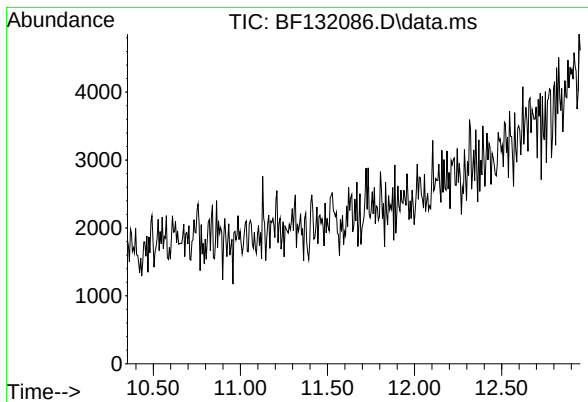


#64
 Phenanthrene-d10
 Concen: 0.000 ng
 Expected RT: 11.65 min
 Lab File: BF132086.D
 Acq: 17 Jan 2023 00:16

Instrument :
 BNA_F
 ClientSampleId :
 PB150154TB

Tgt Ion: 188


Sig	Exp Ratio
188	100
94	9.0
80	10.1

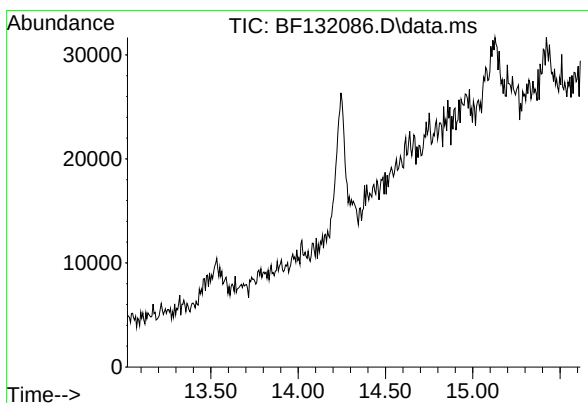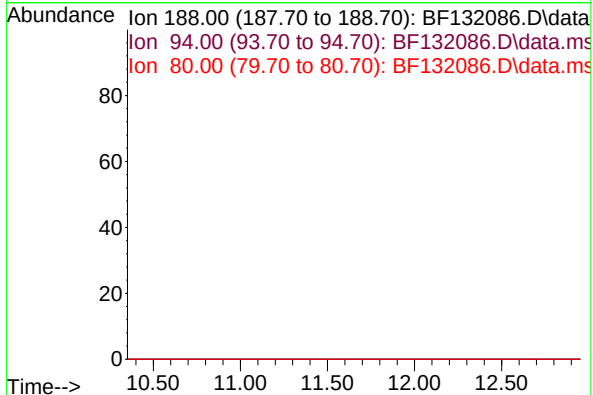


#76
 Chrysene-d12
 Concen: 0.000 ng
 Expected RT: 14.32 min
 Lab File: BF132086.D
 Acq: 17 Jan 2023 00:16

Tgt Ion: 240

Sig	Exp Ratio
240	100
120	10.1
236	26.2

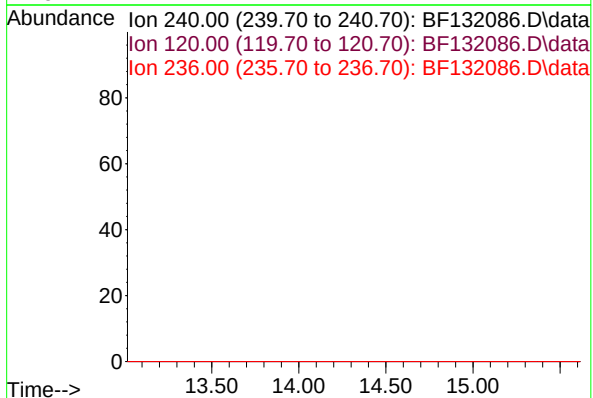

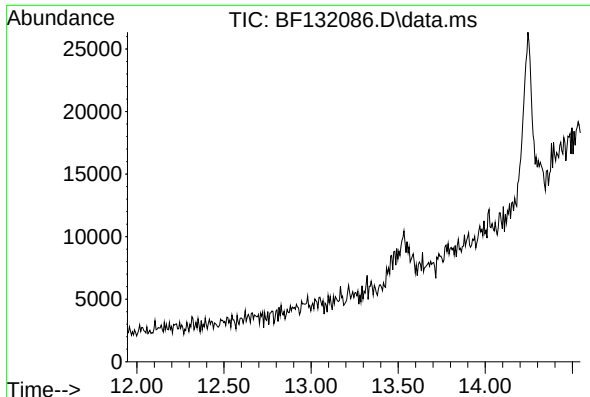

#79

Terphenyl-d14

Concen: 0.000 ng

Expected RT: 13.24 min

Lab File: BF132086.D

Acq: 17 Jan 2023 00:16

Instrument :

BNA_F

ClientSampleId :

PB150154TB



Tgt Ion: 244

Sig Exp Ratio

244 100

212 8.7

122 9.7

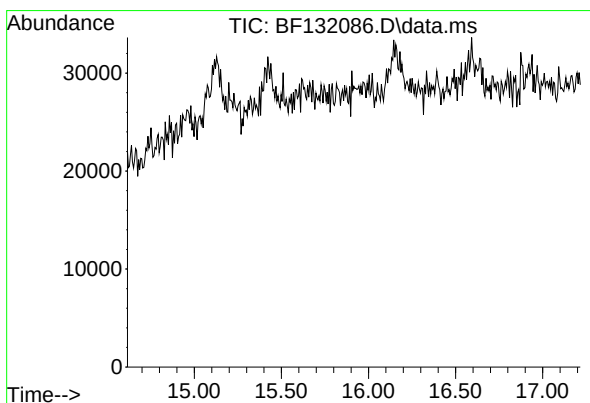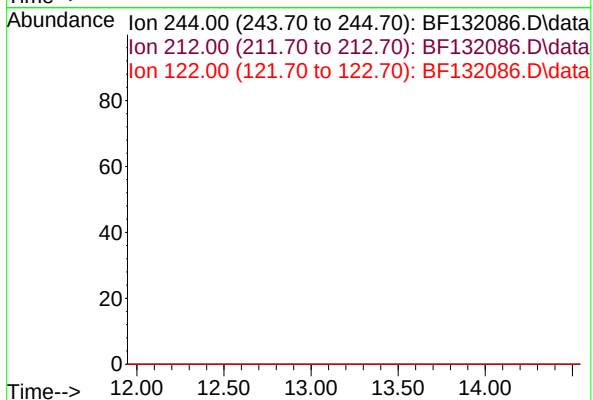

#86

Perylene-d12

Concen: 0.000 ng

Expected RT: 15.92 min

Lab File: BF132086.D

Acq: 17 Jan 2023 00:16

Tgt Ion: 264

Sig Exp Ratio

264 100

260 23.9

265 21.4

