


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011623\
Data File : BF132071.D
Acq On : 16 Jan 2023 15:35
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jan 17 01:48:42 2023

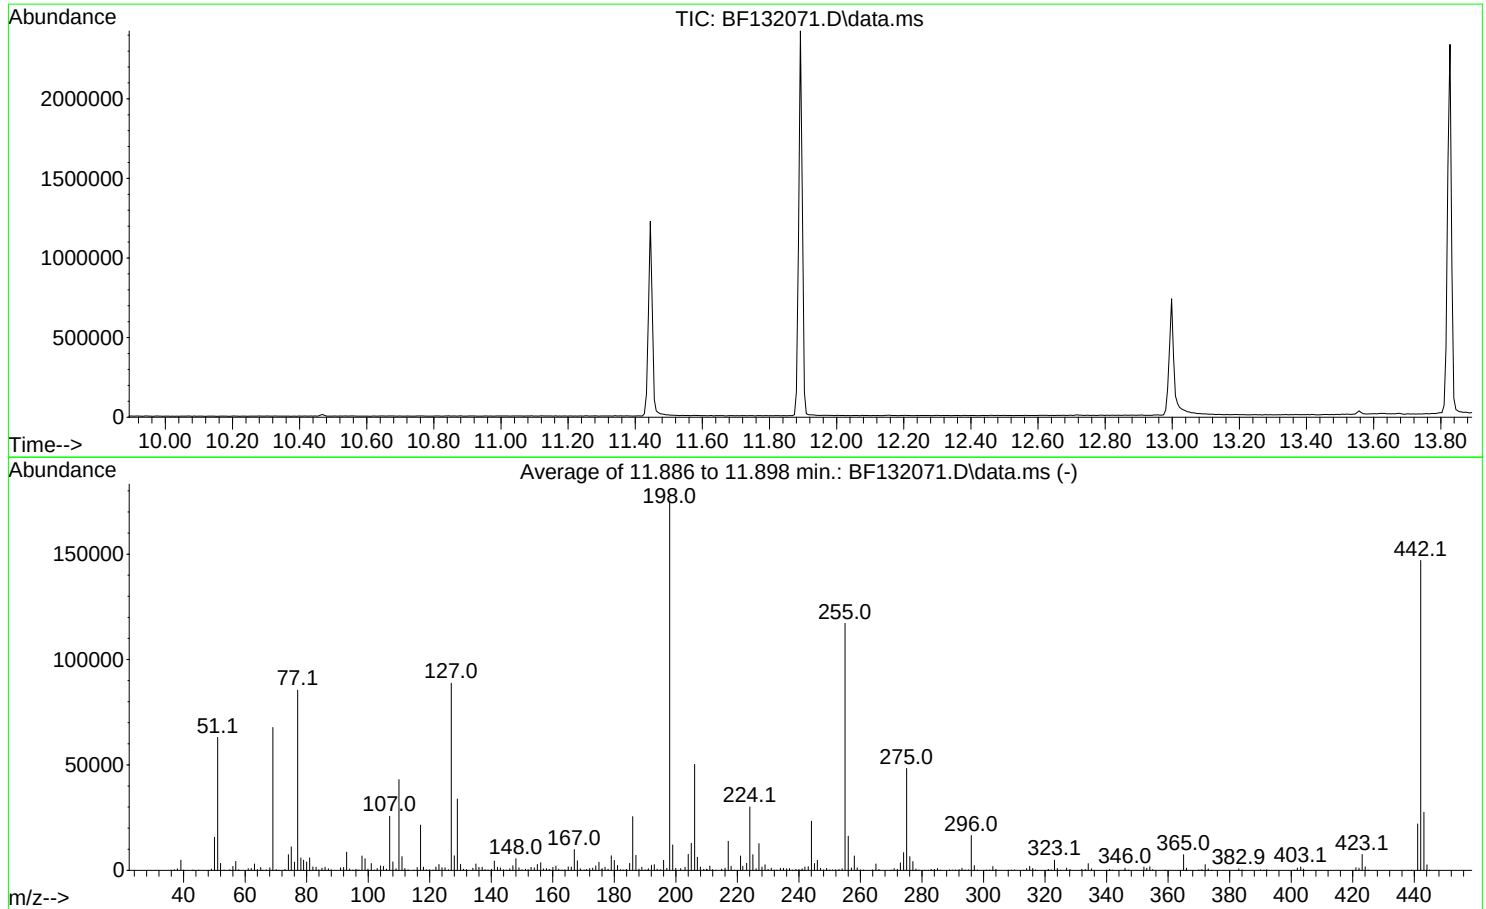




AutoFind: Scans 1666, 1667, 1668; Background Corrected with Scan 1661

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	63029	PASS
68	69	0.00	2	1.7	1145	PASS
69	198	0.00	100	38.8	67760	PASS
70	69	0.00	2	0.5	369	PASS
127	198	10	80	50.9	88789	PASS
197	198	0.00	2	0.5	953	PASS
198	198	100	100	100.0	174523	PASS
199	198	5	9	6.9	12000	PASS
275	198	10	60	27.7	48333	PASS
365	198	1	100	4.3	7421	PASS
441	198	0.01	100	12.6	21959	PASS
442	442	50	100	100.0	147000	PASS
443	442	15	24	18.7	27494	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011623\
Data File : BF132071.D
Acq On : 16 Jan 2023 15:35
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 17 08:06:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 17 01:48:42 2023
Response via : Initial Calibration

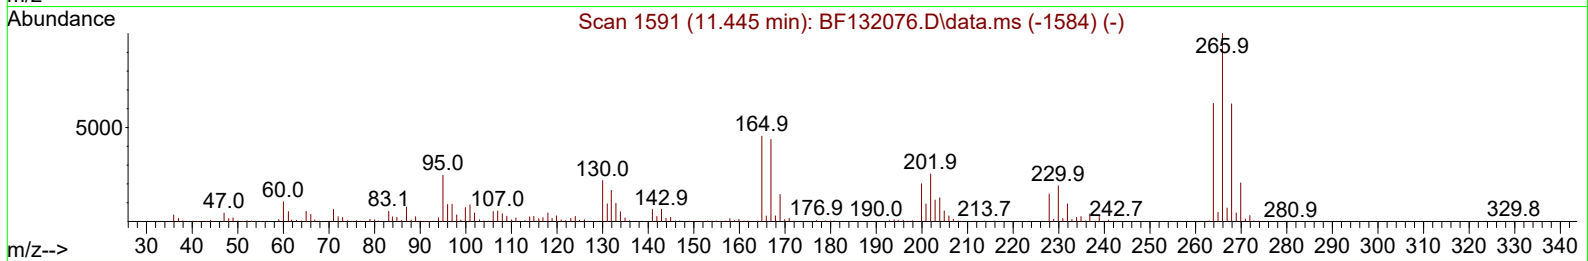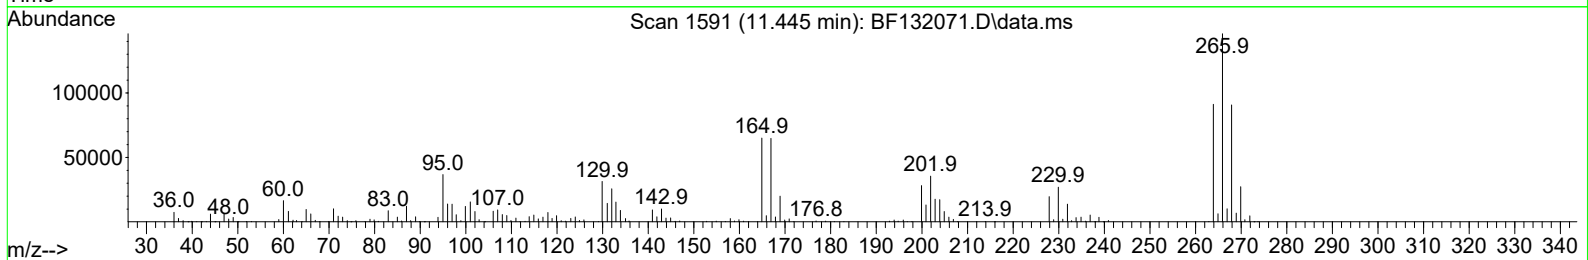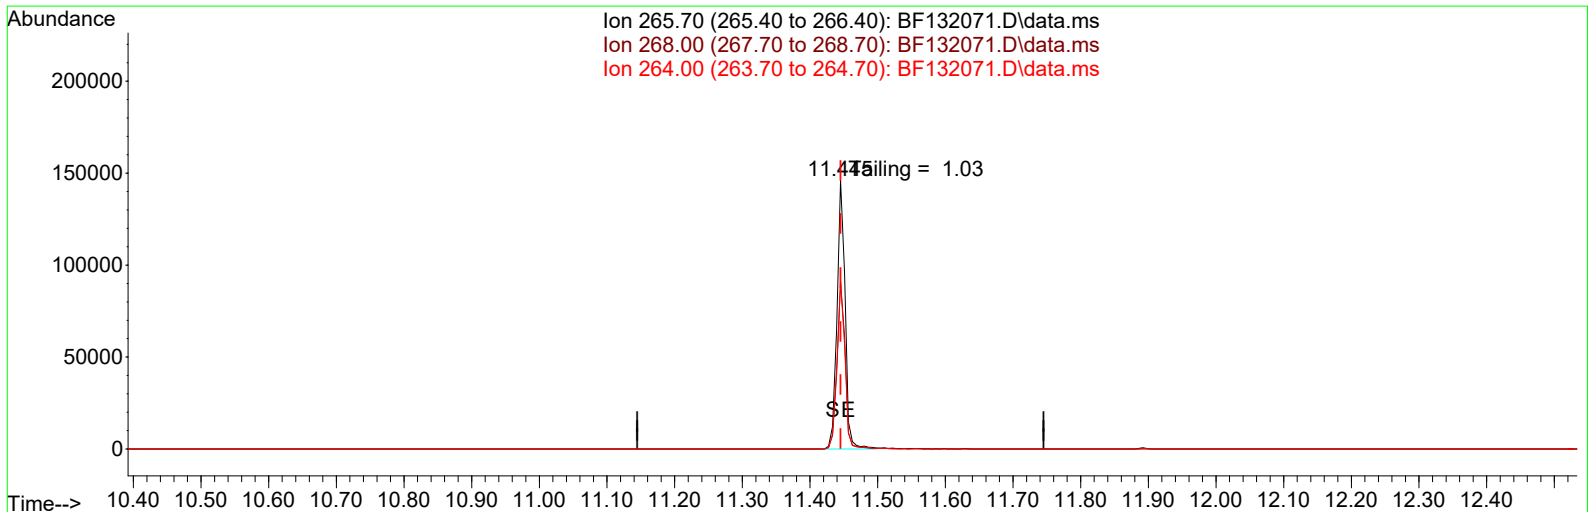

TIC: BF132071.D\data.ms

(70) Pentachlorophenol (C)

11.445min (+ 0.000) 26198.72 ng




response 122936

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.50	62.19
264.00	62.80	62.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011623\
Data File : BF132071.D
Acq On : 16 Jan 2023 15:35
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 17 08:06:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 17 01:48:42 2023
Response via : Initial Calibration

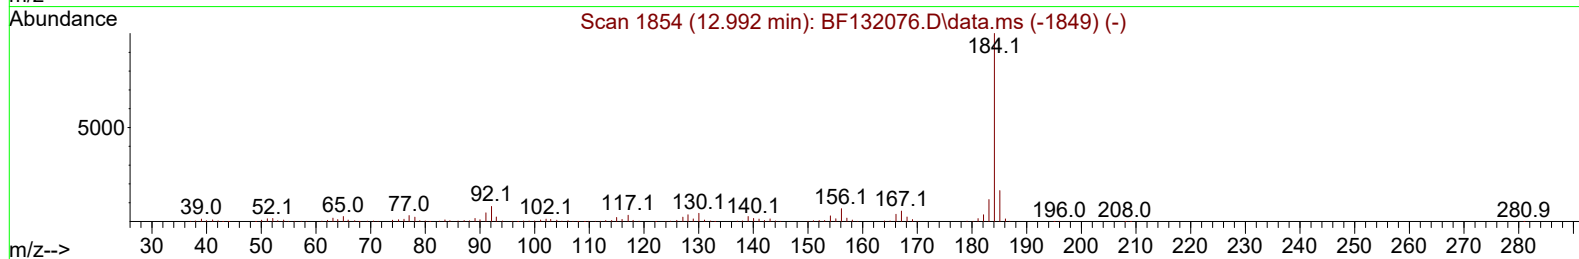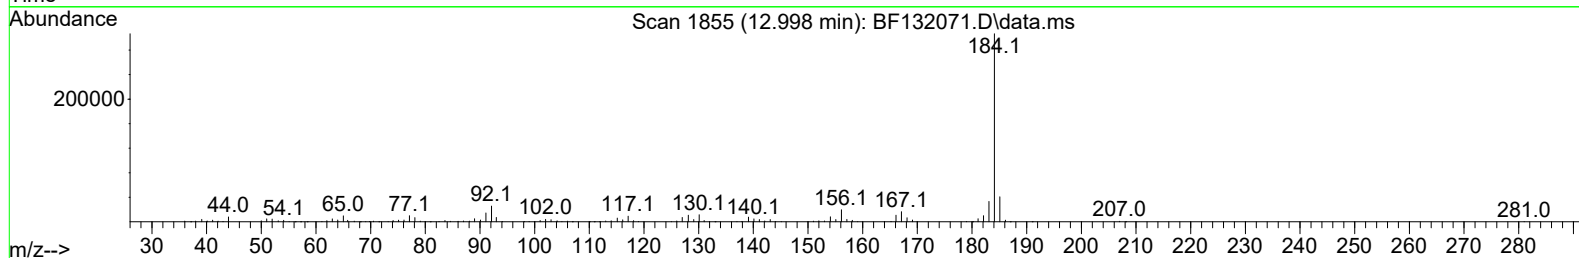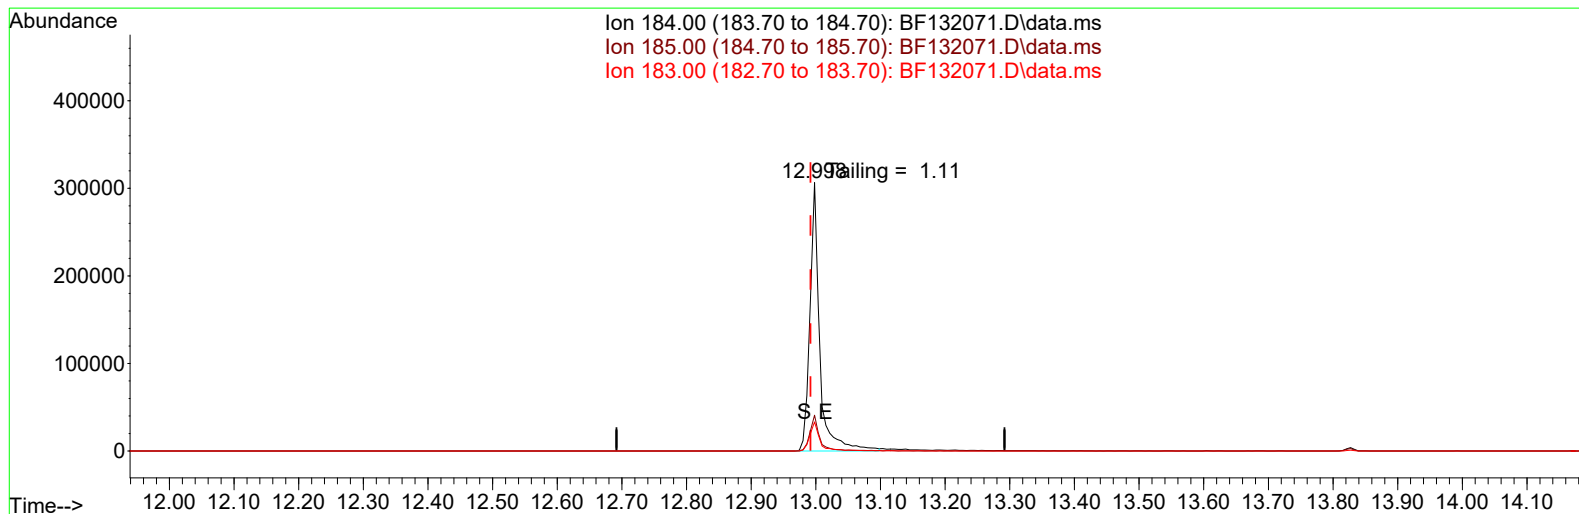

TIC: BF132071.D\data.ms

(77) Benzidine

12.998min (+ 0.006) 0.00 ng

response 333103

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.40	13.34
183.00	11.70	10.87
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/16/2023	BNA_F	<u>BF132071.D</u>
Compound Name	Response	Retention Time
DDT	166144	13.827
DDD	1665	13.557
DDE	0	12.845
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1665	167809	0.99

Instrument :
BNA_F
ClientSampleId :
DFTPP