
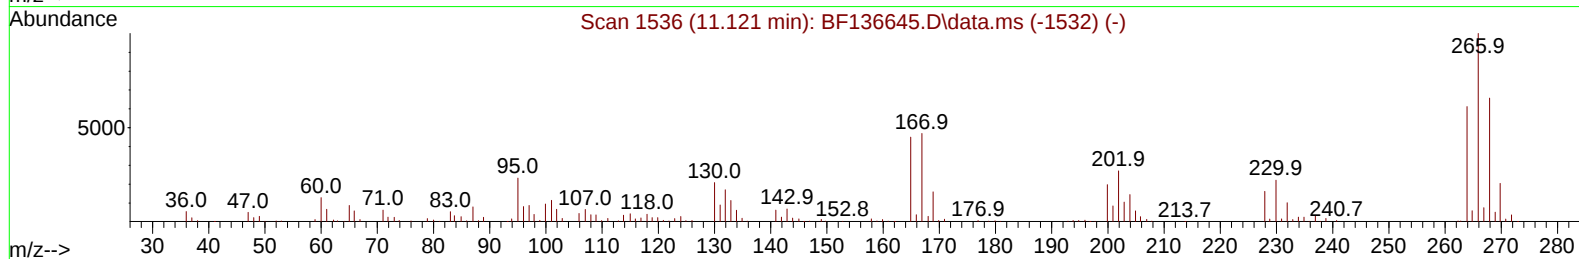
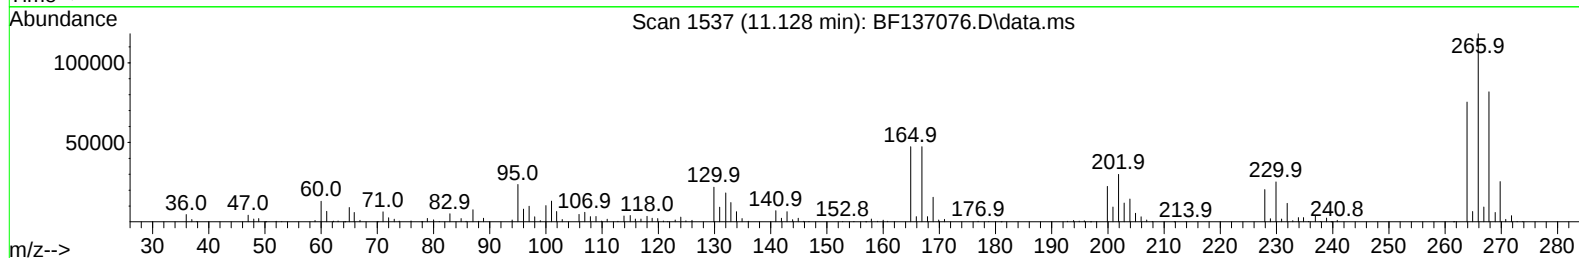


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011624\
Data File : BF137076.D
Acq On : 16 Jan 2024 13:39
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 16 14:08:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

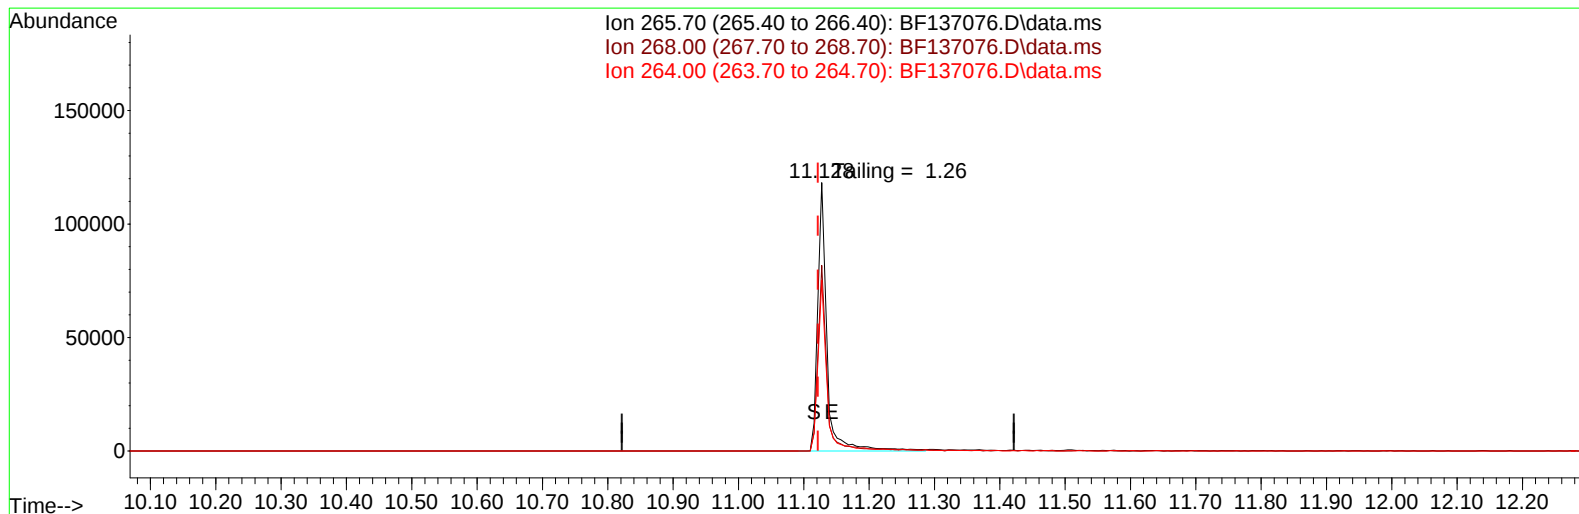




TIC: BF137076.D\data.ms

(70) Pentachlorophenol (C)**11.128min (+ 0.006) 134735.85 ng****response 116589**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	69.16
264.00	61.20	63.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011624\
Data File : BF137076.D
Acq On : 16 Jan 2024 13:39
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 16 14:08:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

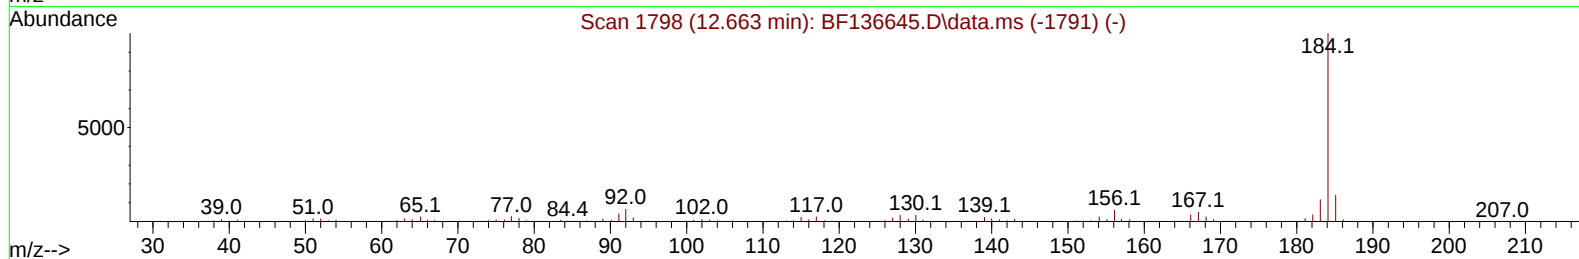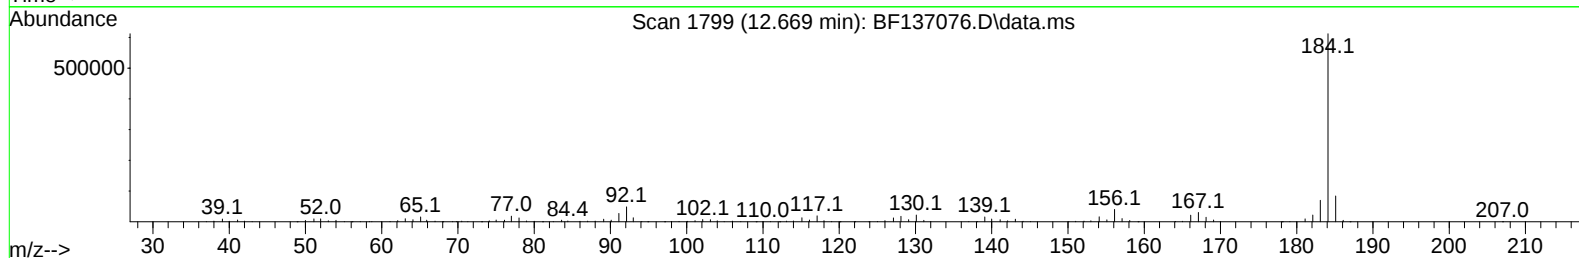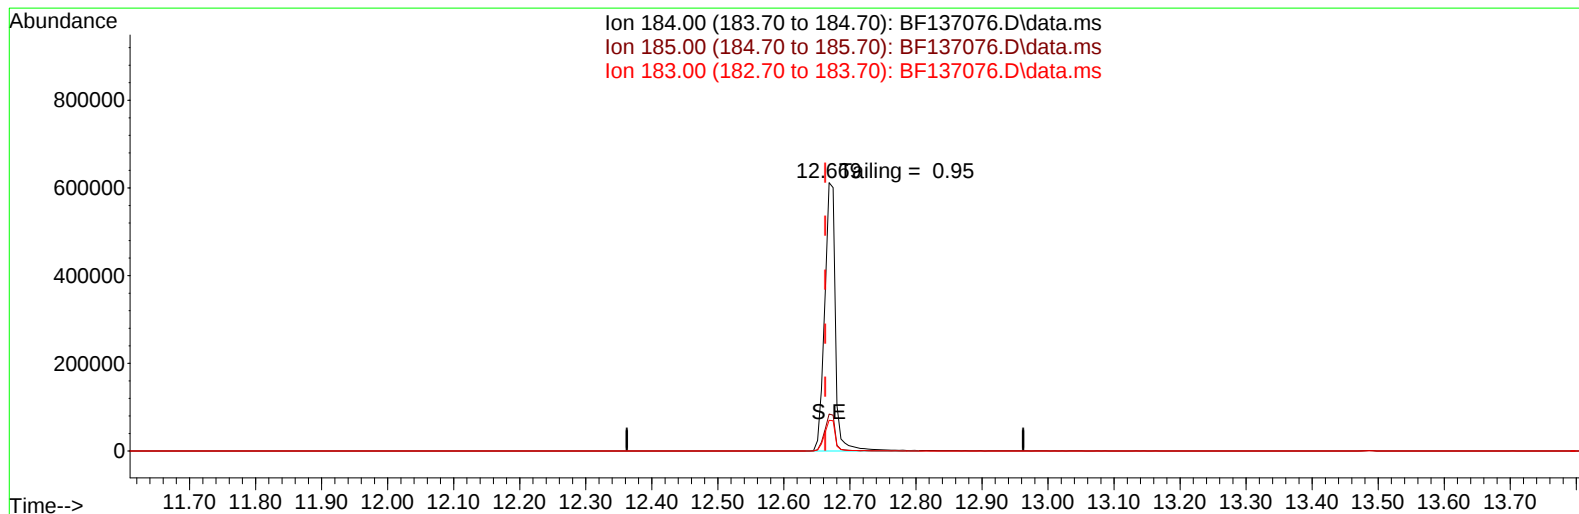

TIC: BF137076.D\data.ms

(77) Benzidine

12.669min (+ 0.006) 189668.64 ng

response 693472

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.77
183.00	11.60	11.47
0.00	0.00	0.00