
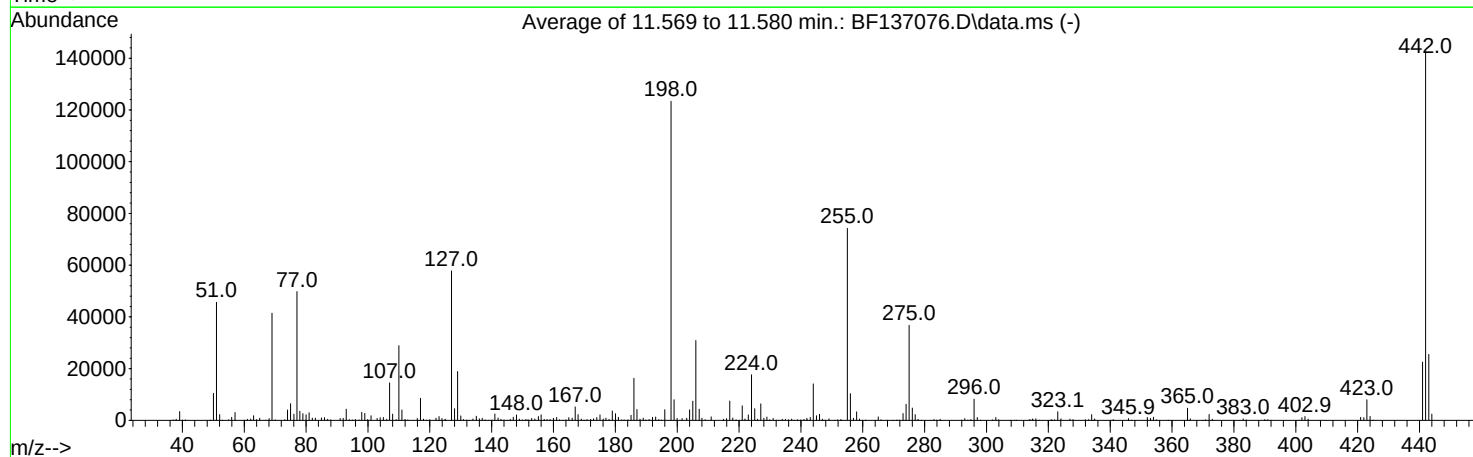


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011624\
Data File : BF137076.D
Acq On : 16 Jan 2024 13:39
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 21 01:54:25 2023

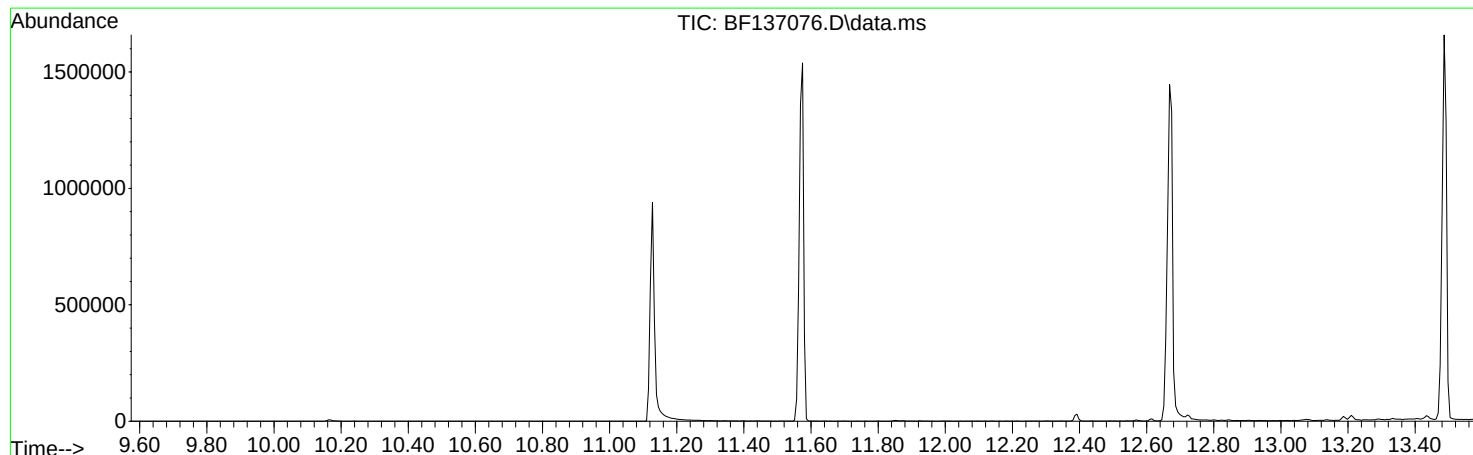




AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.0	45649	PASS
68	69	0.00	2	1.7	711	PASS
69	198	0.00	100	33.6	41449	PASS
70	69	0.00	2	0.5	209	PASS
127	198	10	80	46.8	57784	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	123355	PASS
199	198	5	9	6.5	7975	PASS
275	198	10	60	29.8	36751	PASS
365	198	1	100	3.8	4681	PASS
441	198	0.01	100	18.3	22532	PASS
442	442	50	100	100.0	142208	PASS
443	442	15	24	17.9	25496	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011624\
Data File : BF137076.D
Acq On : 16 Jan 2024 13:39
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 16 14:08:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

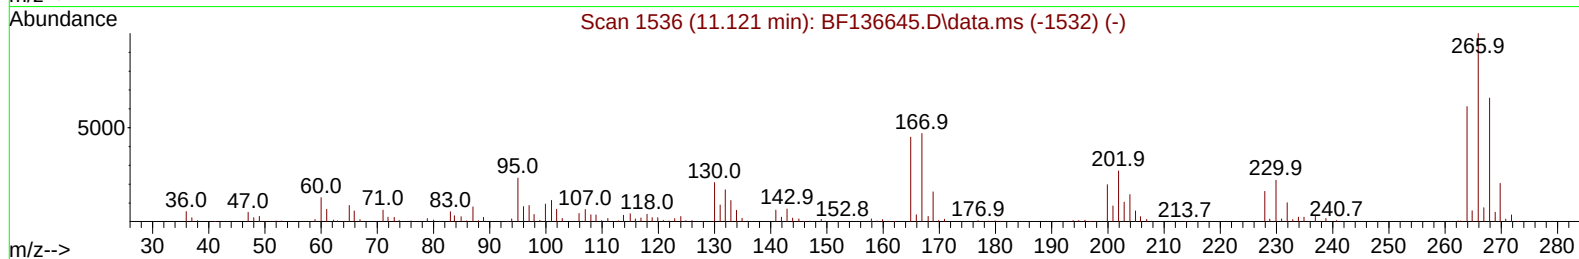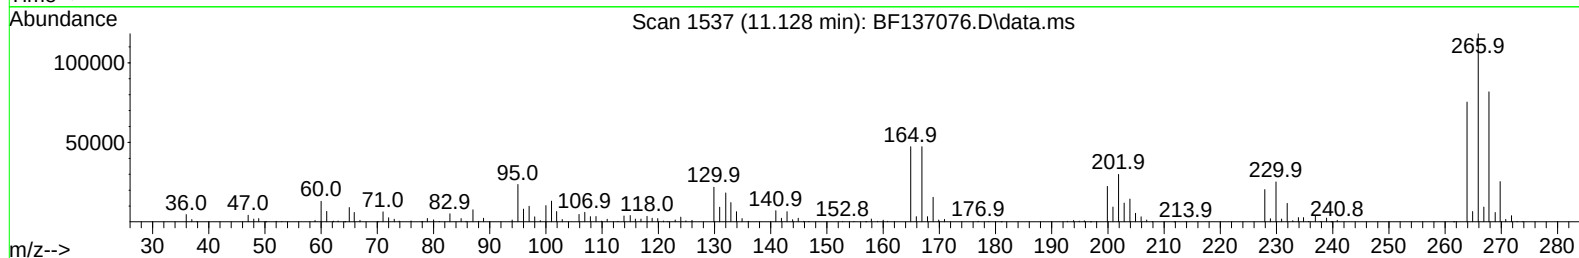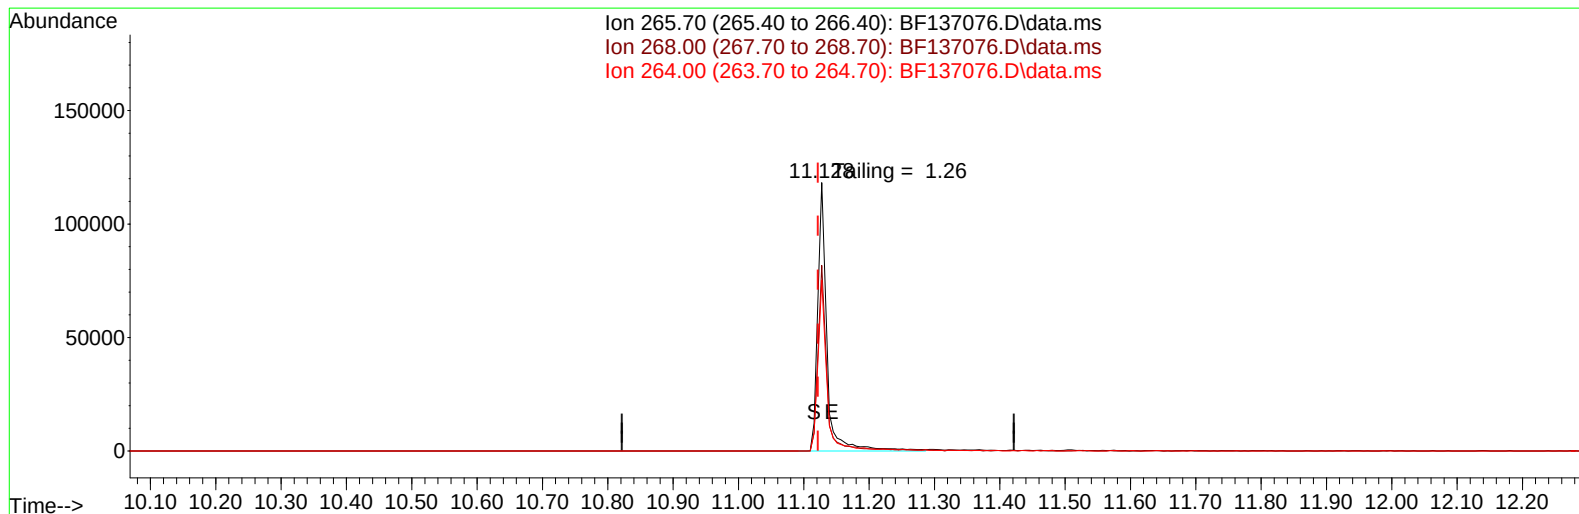

TIC: BF137076.D\data.ms

(70) Pentachlorophenol (C)

11.128min (+ 0.006) 134735.85 ng




response 116589

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	69.16
264.00	61.20	63.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011624\
Data File : BF137076.D
Acq On : 16 Jan 2024 13:39
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 16 14:08:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

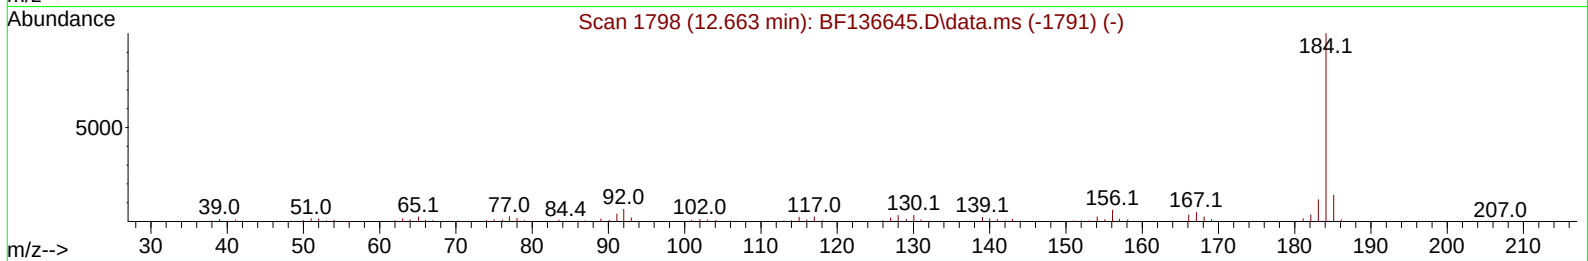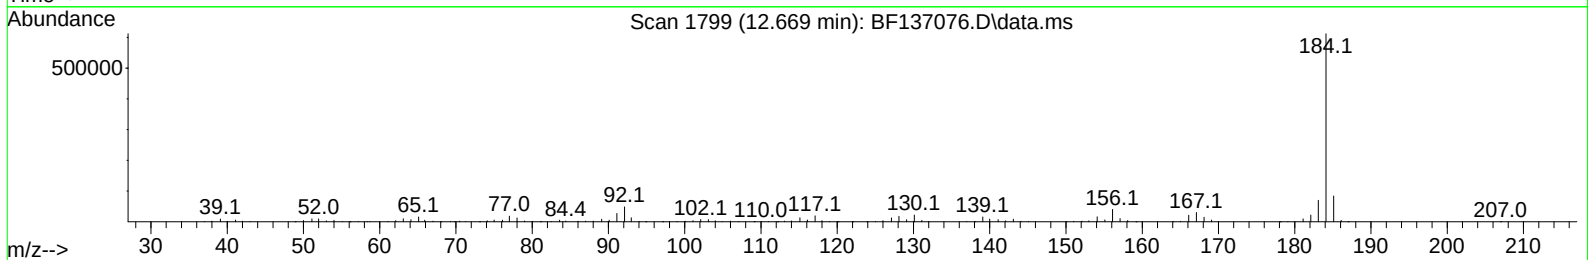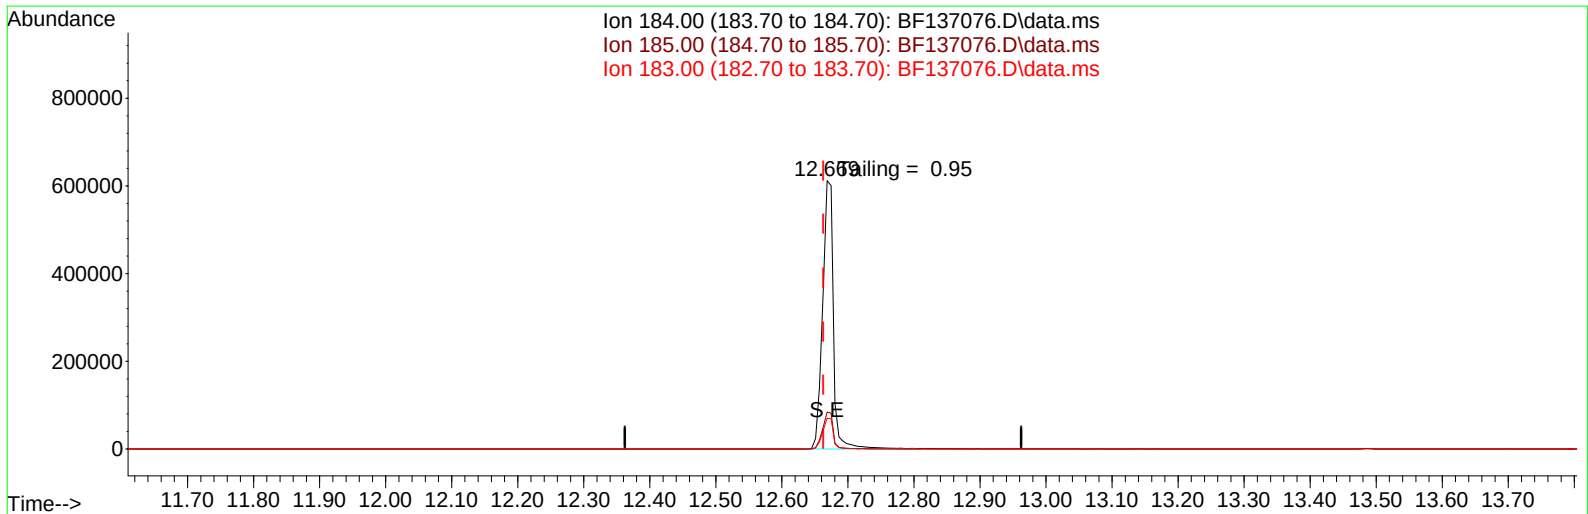

TIC: BF137076.D\data.ms

(77) Benzidine

12.669min (+ 0.006) 189668.64 ng

response 693472

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.77
183.00	11.60	11.47
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/16/2024	BNA_F	<u>BF137076.D</u>
Compound Name	Response	Retention Time
DDT	321109	13.486
DDD	7943	13.186
DDE	389	12.845
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8332	329441	2.53

Instrument :
BNA_F
ClientSampleId :
DFTPP