
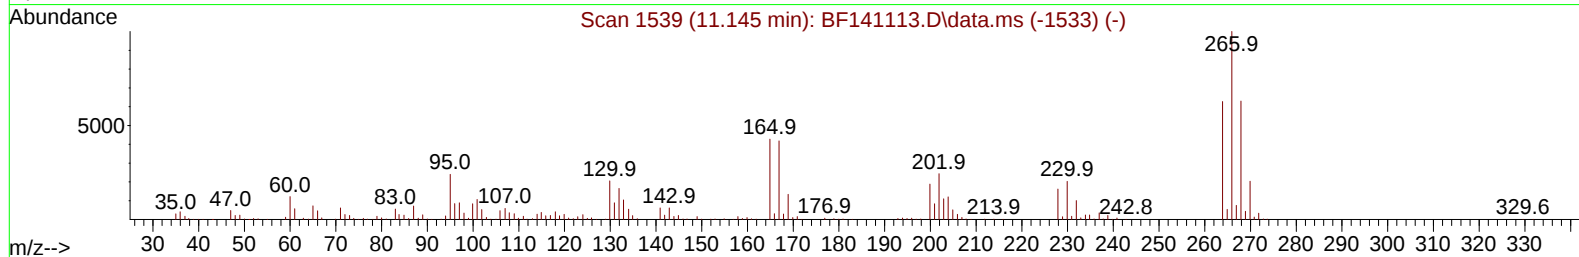
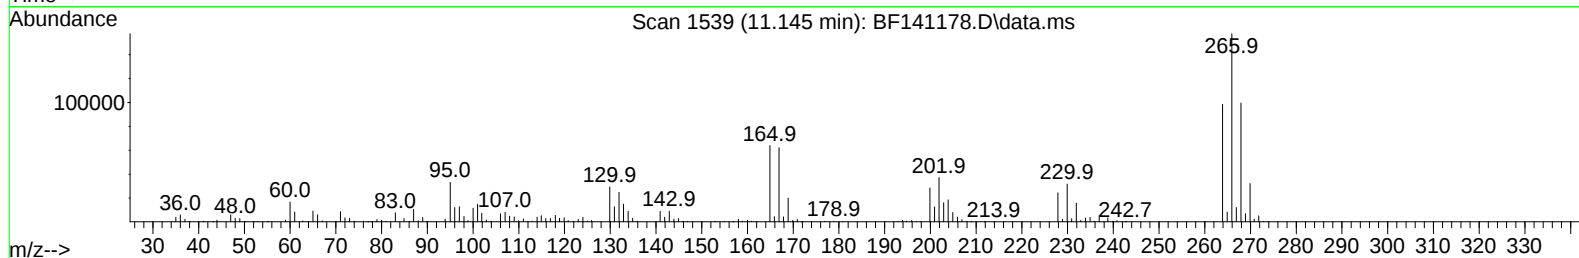


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF011625\  
Data File : BF141178.D  
Acq On : 16 Jan 2025 10:25  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 16 11:15:54 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF011025.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Jan 10 22:54:19 2025  
Response via : Initial Calibration

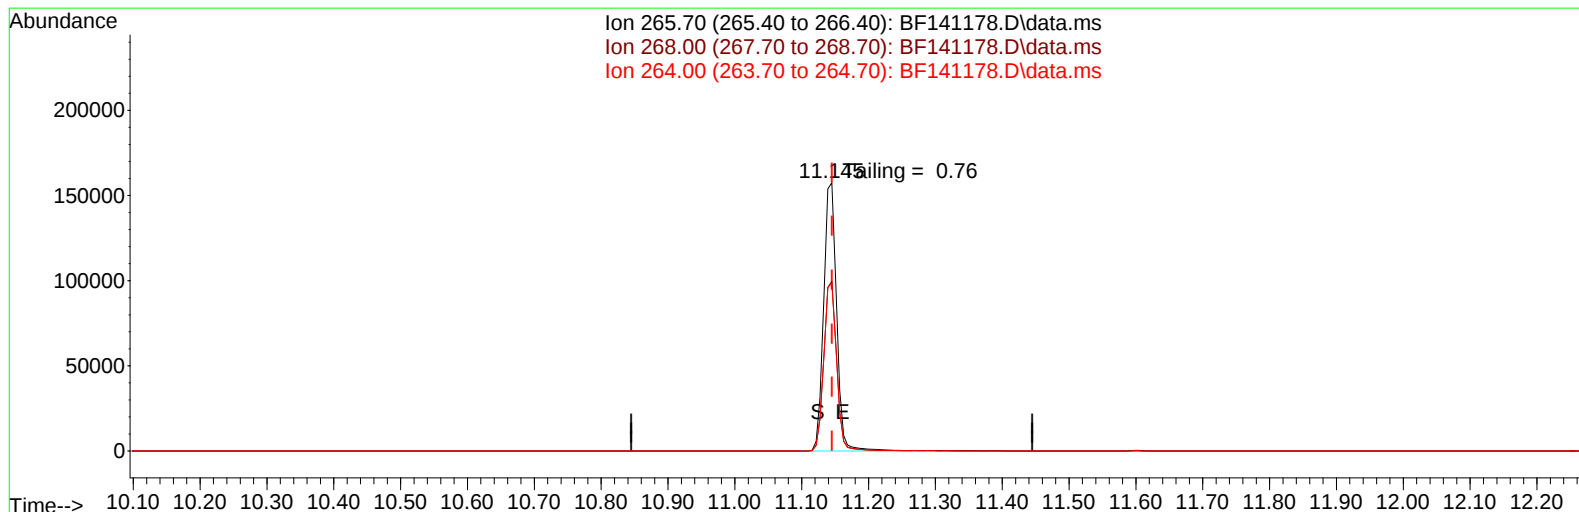

TIC: BF141178.D\data.ms

**(70) Pentachlorophenol (C)**




11.145min (-0.000) 19050.59 ng

response 212333

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.00  | 63.21  |
| 264.00 | 62.70  | 62.52  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF011625\  
Data File : BF141178.D  
Acq On : 16 Jan 2025 10:25  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 16 11:15:54 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF011025.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Jan 10 22:54:19 2025  
Response via : Initial Calibration

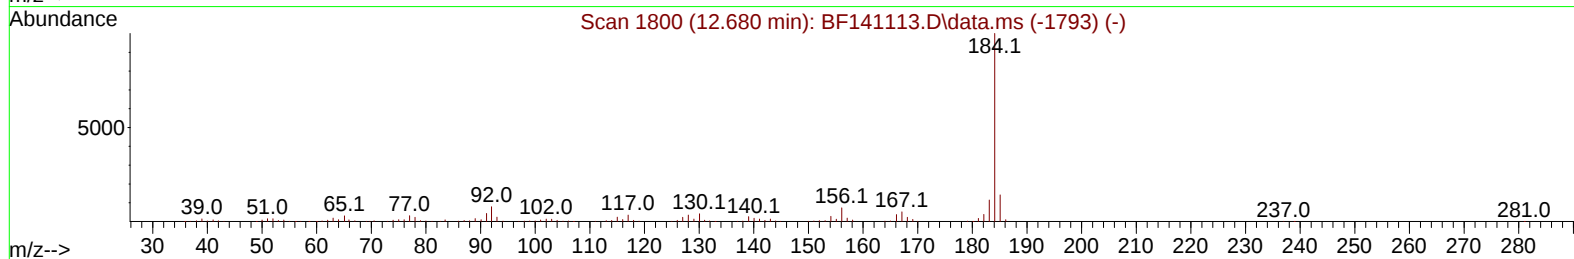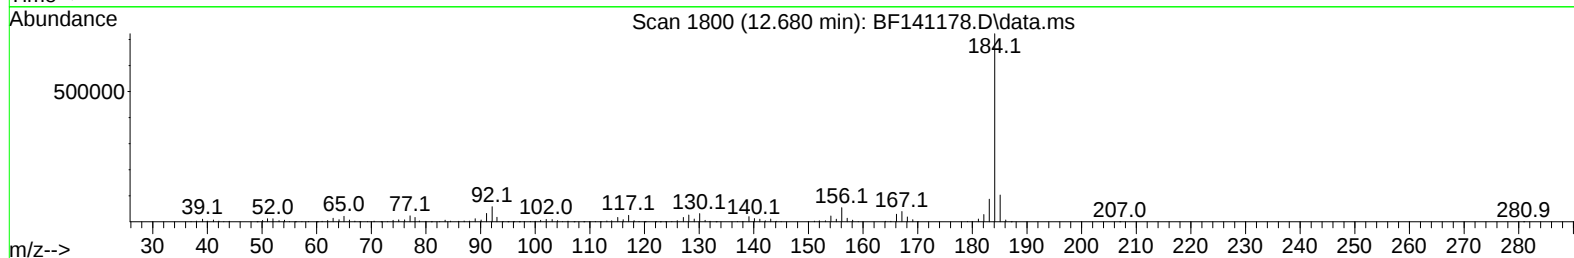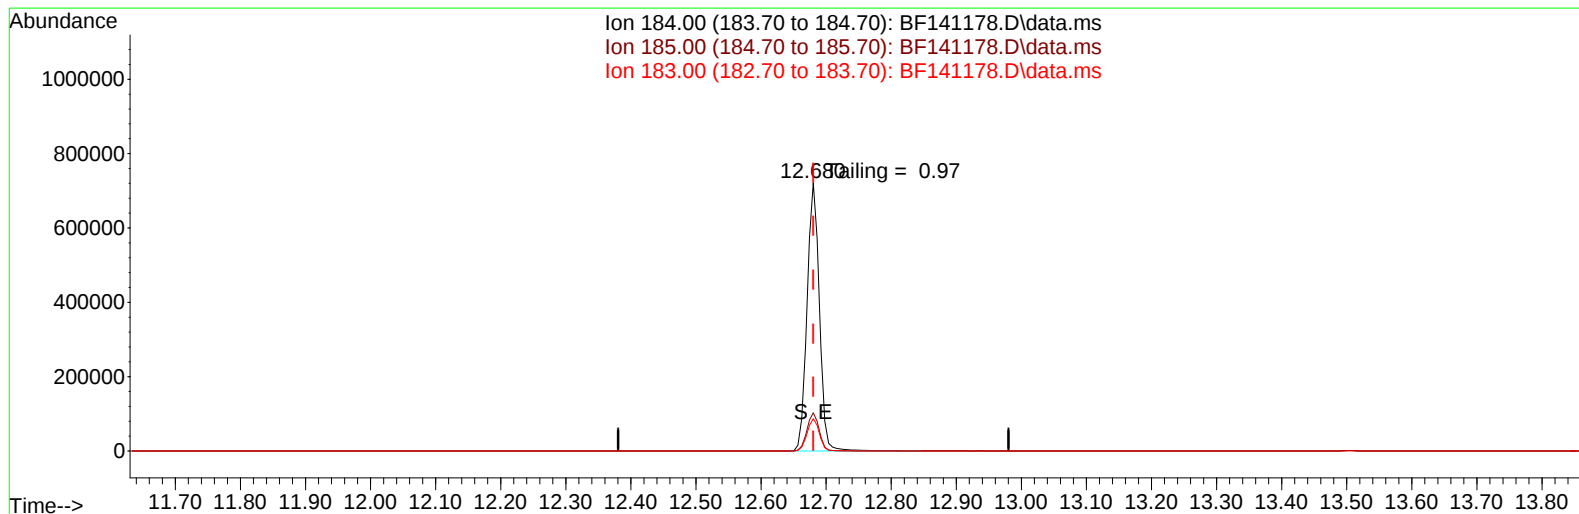

TIC: BF141178.D\data.ms

**(77) Benzidine****12.680min (-0.000) 33525.20 ng****response 949342**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.20  | 14.26  |
| 183.00 | 11.50  | 12.06  |
| 0.00   | 0.00   | 0.00   |