


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011625\
Data File : BF141178.D
Acq On : 16 Jan 2025 10:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jan 10 22:54:19 2025

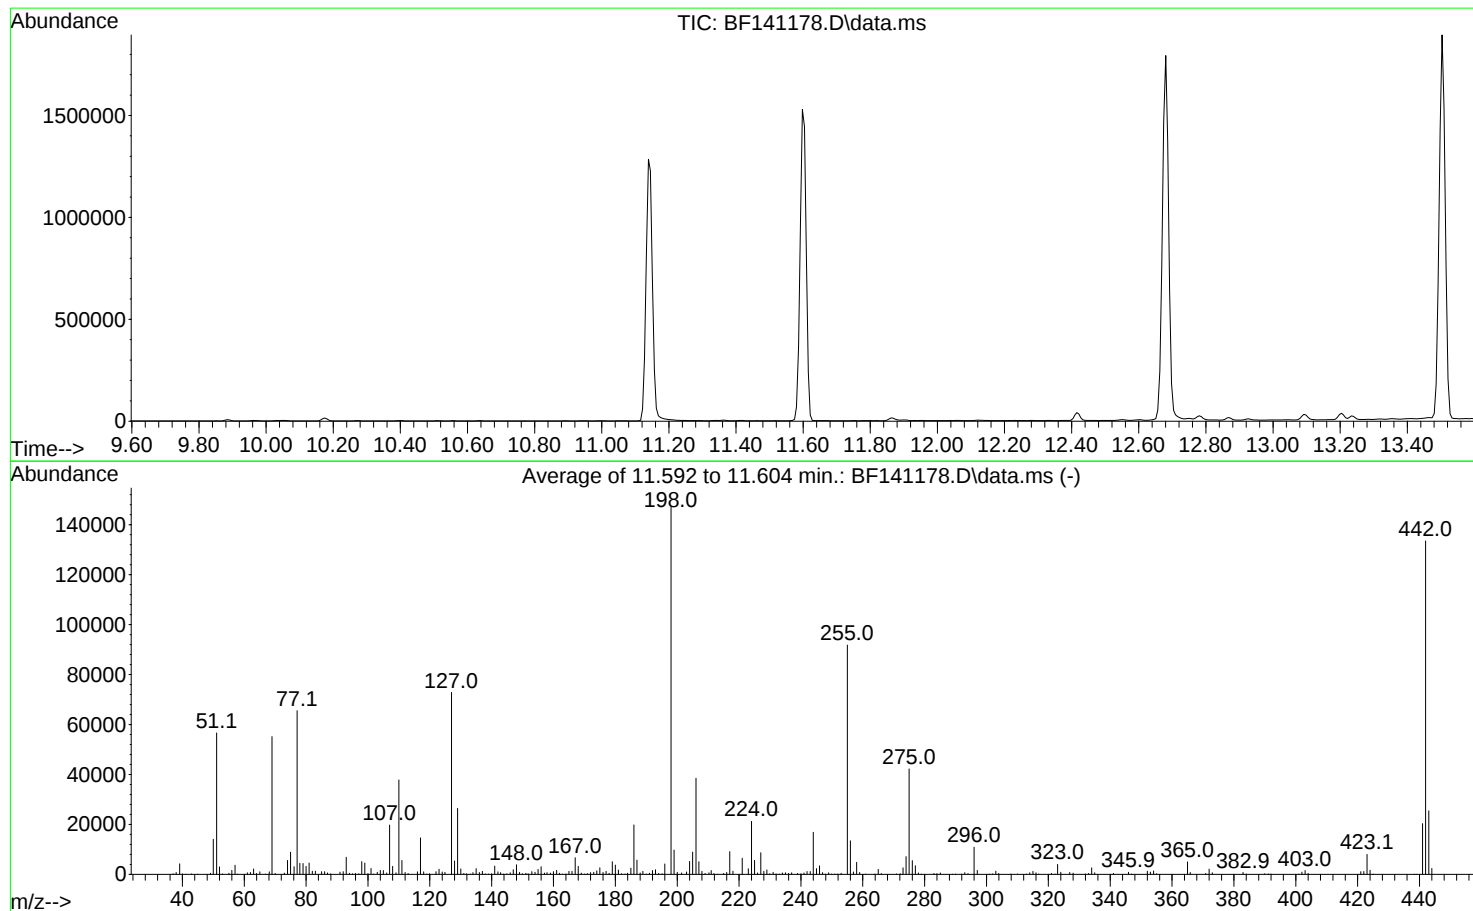

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.4	56629	PASS
68	69	0.00	2	1.9	1050	PASS
69	198	0.00	100	37.5	55181	PASS
70	69	0.00	2	0.7	398	PASS
127	198	10	80	49.5	72840	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	147293	PASS
199	198	5	9	6.6	9747	PASS
275	198	10	60	28.6	42197	PASS
365	198	1	100	3.4	4983	PASS
441	198	0.01	100	13.8	20308	PASS
442	442	50	100	100.0	133515	PASS
443	442	15	24	19.1	25469	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/16/2025	BNA_F	<u>BF141178.D</u>
Compound Name	Response	Retention Time
DDT	466469	13.504
DDD	12624	13.204
DDE	2391	12.868
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15015	481484	3.12

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011625\
Data File : BF141178.D
Acq On : 16 Jan 2025 10:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 16 11:15:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 10 22:54:19 2025
Response via : Initial Calibration

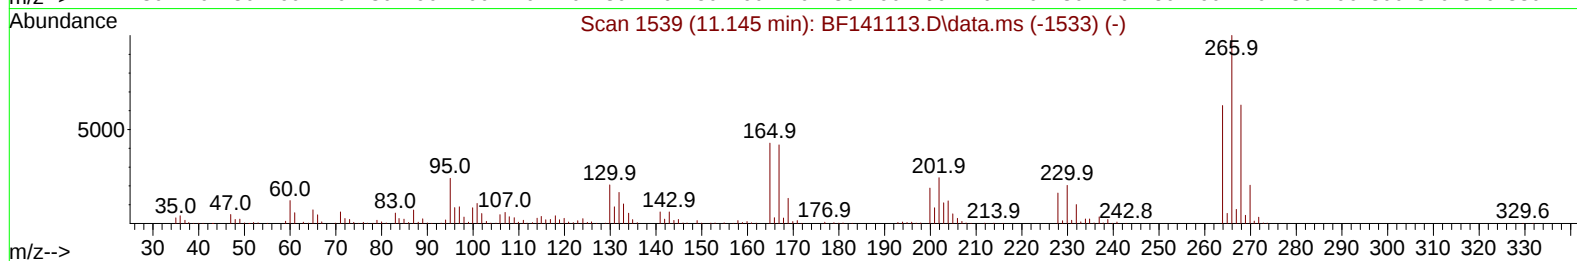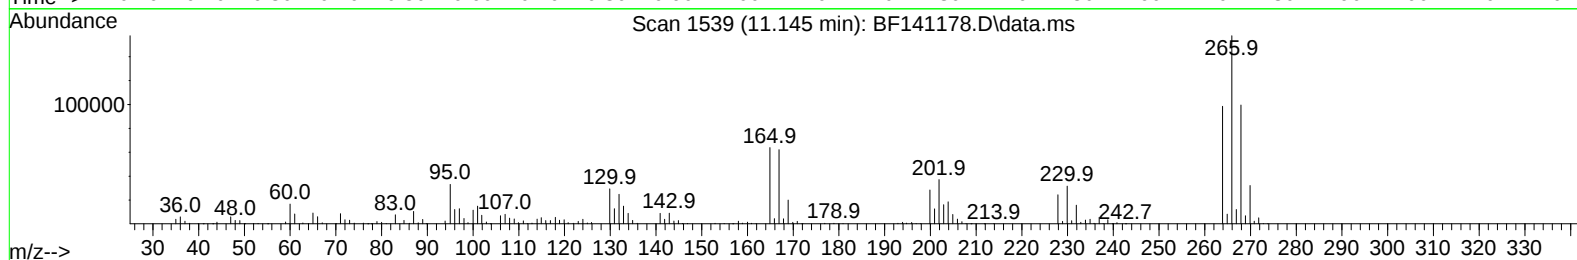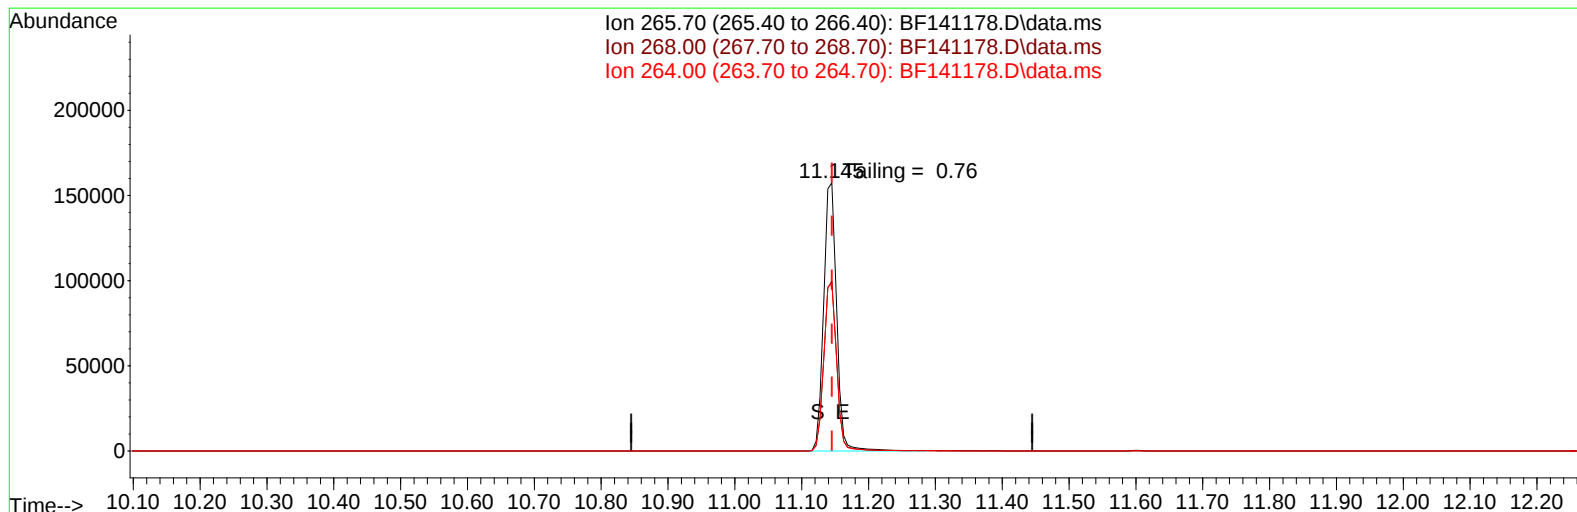

TIC: BF141178.D\data.ms

(70) Pentachlorophenol (C)

11.145min (-0.000) 19050.59 ng




response 212333

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.21
264.00	62.70	62.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011625\
Data File : BF141178.D
Acq On : 16 Jan 2025 10:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 16 11:15:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 10 22:54:19 2025
Response via : Initial Calibration

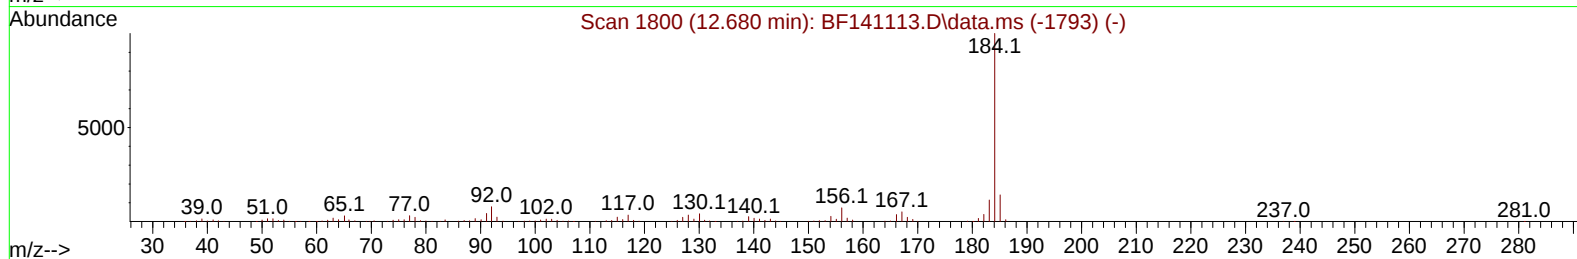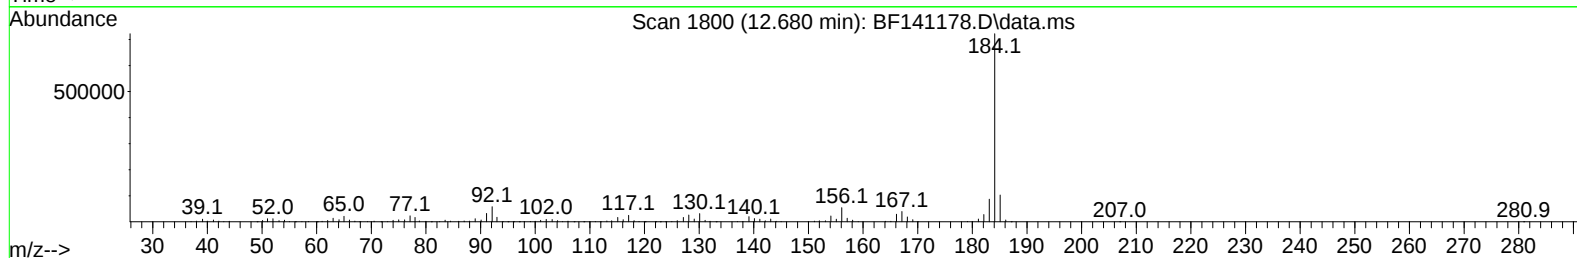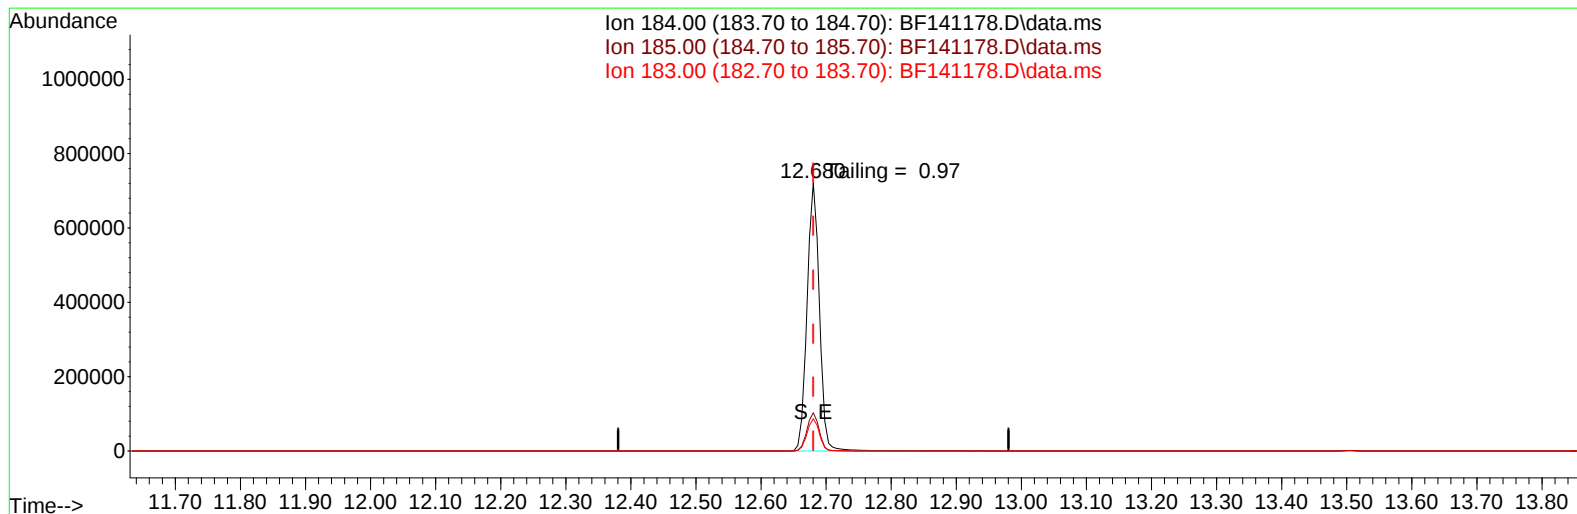

TIC: BF141178.D\data.ms

(77) Benzidine

12.680min (-0.000) 33525.20 ng

response 949342

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.26
183.00	11.50	12.06
0.00	0.00	0.00