
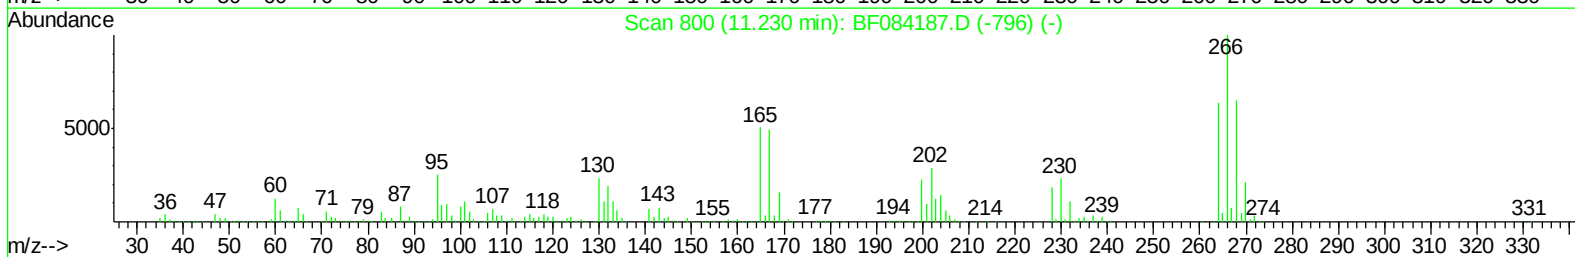
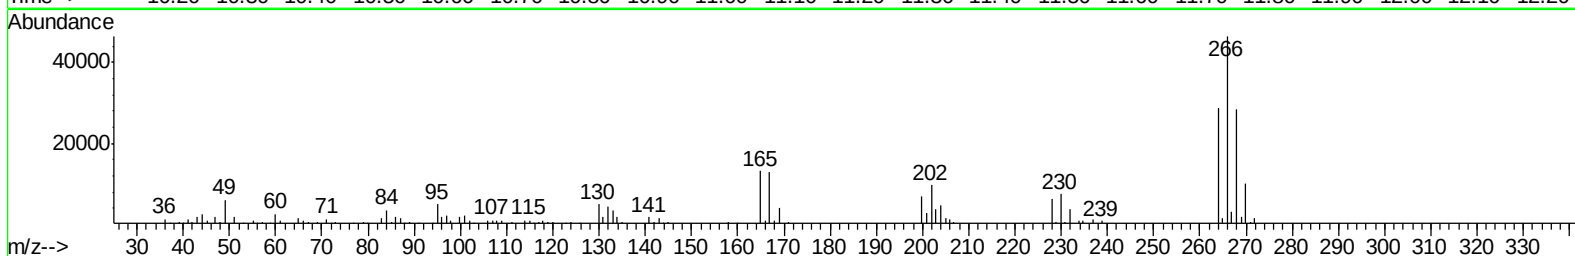


Data Path : Z:\HPCHEM1\BNA_F\Data\BF011716\
Data File : BF084528.D
Acq On : 17 Jan 2016 10:30
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BFB

Quant Time: Jan 18 08:08:35 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 14 14:15:52 2016
Response via : Initial Calibration

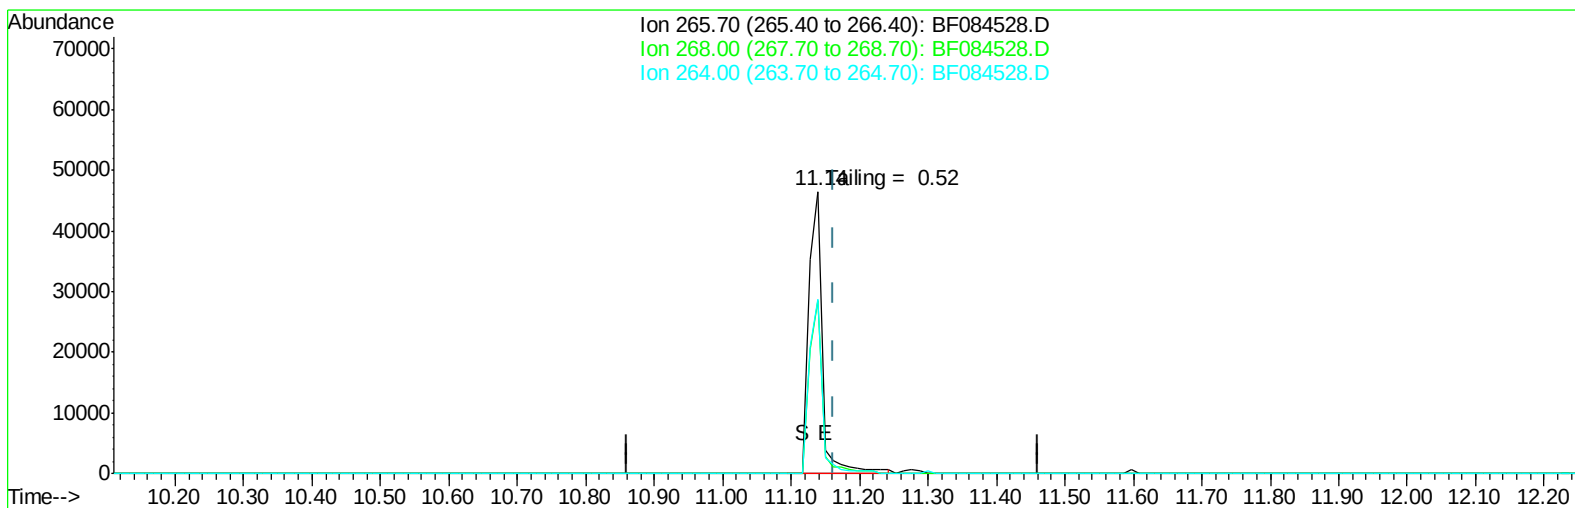

TIC: BF084528.D

(69) Pentachlorophenol (C)

11.139min (-0.023) 4268.67ng




response 64218

Ion	Exp%	Act%
265.70	100	100
268.00	65.50	61.47
264.00	62.70	61.63
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF011716\
Data File : BF084528.D
Acq On : 17 Jan 2016 10:30
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BFB

Quant Time: Jan 18 08:08:35 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 14 14:15:52 2016
Response via : Initial Calibration

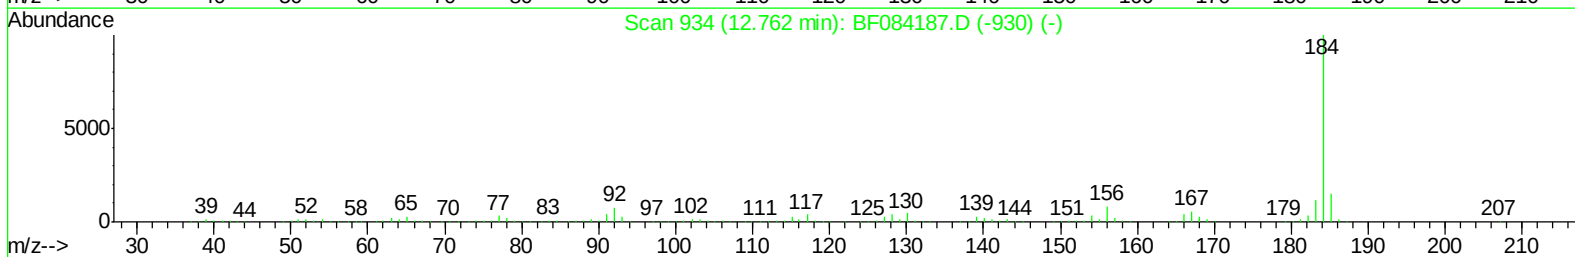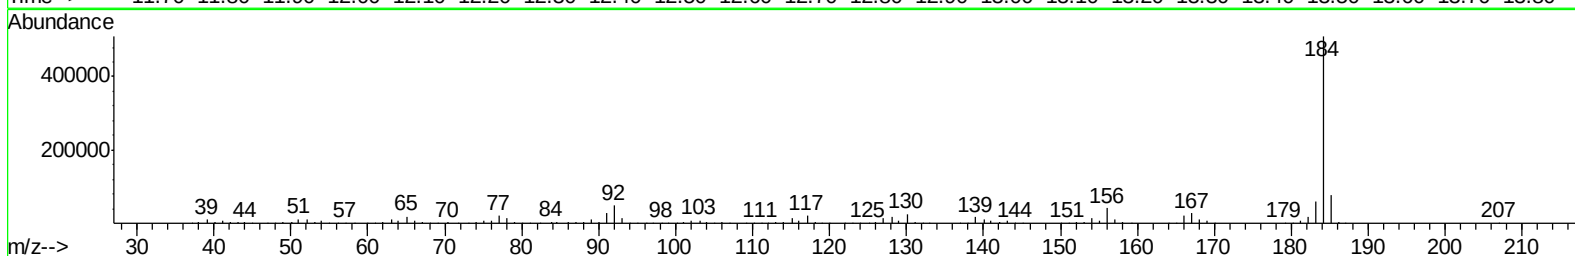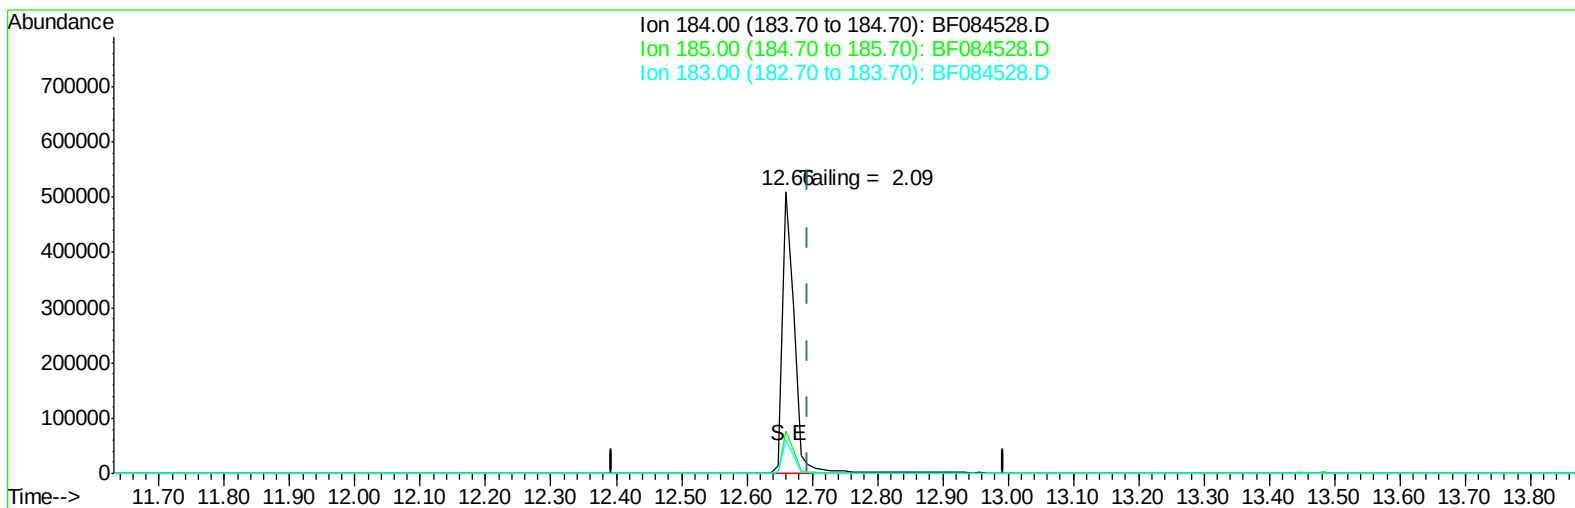

TIC: BF084528.D

(76) Benzidine

12.659min (-0.034) 2281.48ng




response 635362

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	15.13
183.00	12.30	11.79
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF011716\
Data File : BF084528.D
Acq On : 17 Jan 2016 10:30
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BFB

Quant Time: Jan 18 08:08:35 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 14 14:15:52 2016
Response via : Initial Calibration

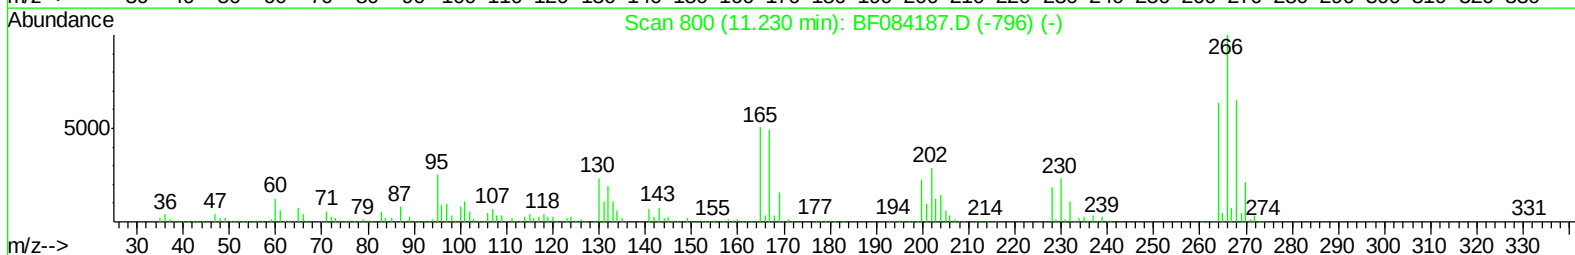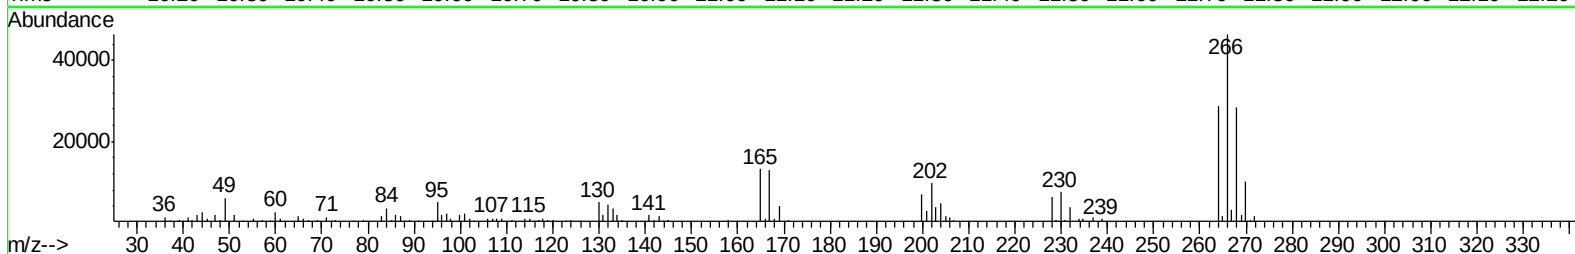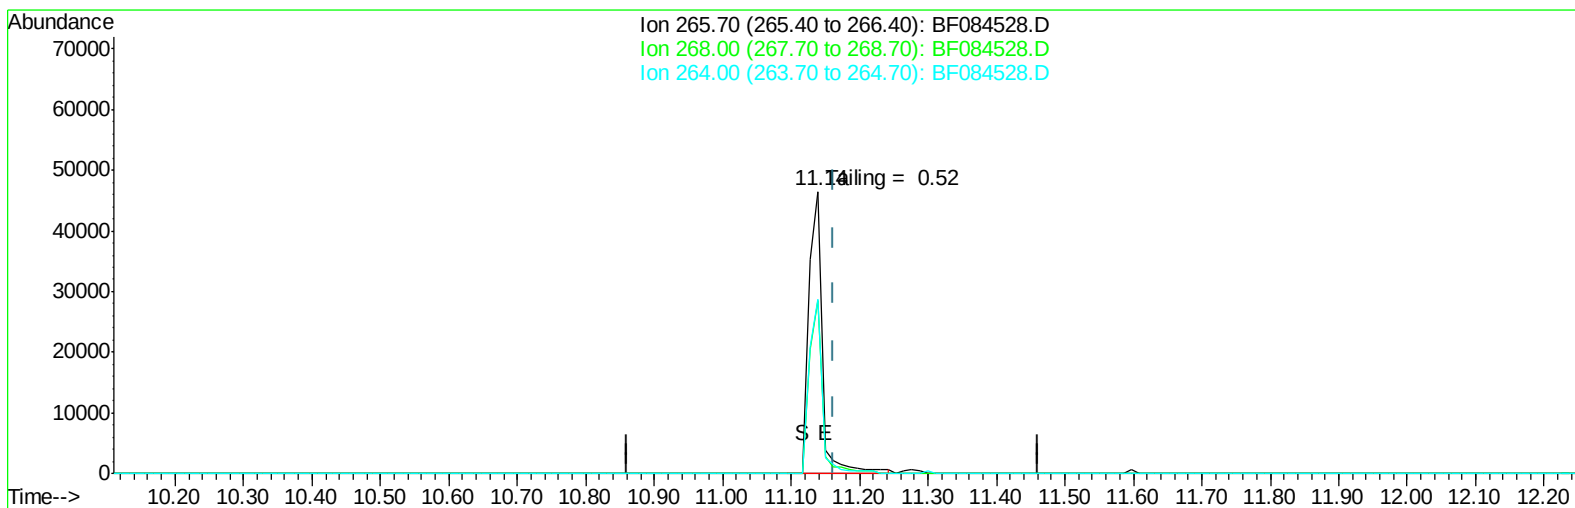

TIC: BF084528.D

(69) Pentachlorophenol (C)

11.139min (-0.023) 4268.67ng




response 64218

Ion	Exp%	Act%
265.70	100	100
268.00	65.50	61.47
264.00	62.70	61.63
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF011716\
Data File : BF084528.D
Acq On : 17 Jan 2016 10:30
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BFB

Quant Time: Jan 18 08:08:35 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 14 14:15:52 2016
Response via : Initial Calibration

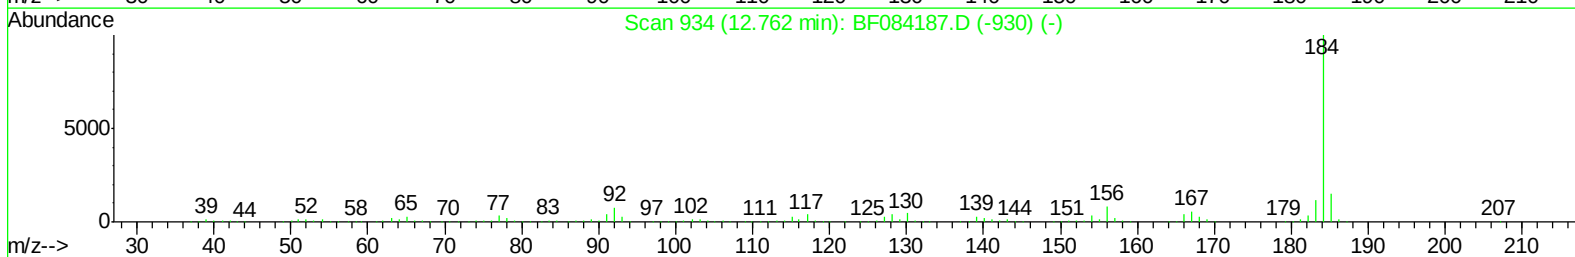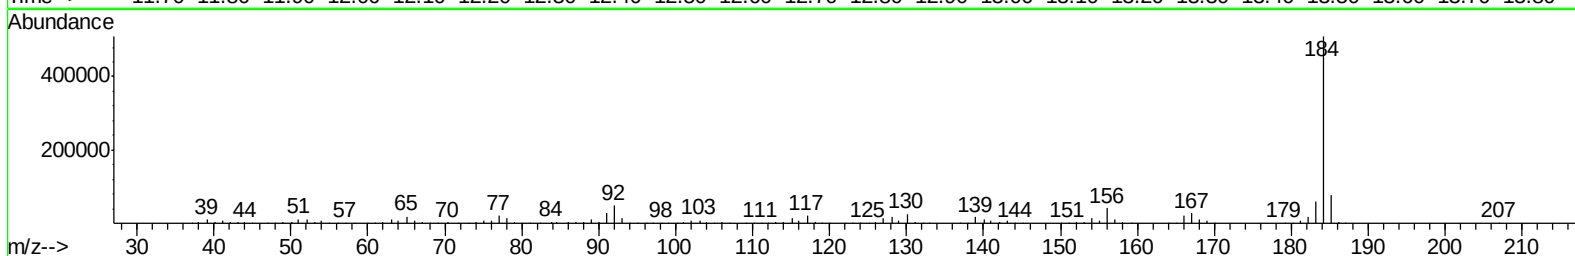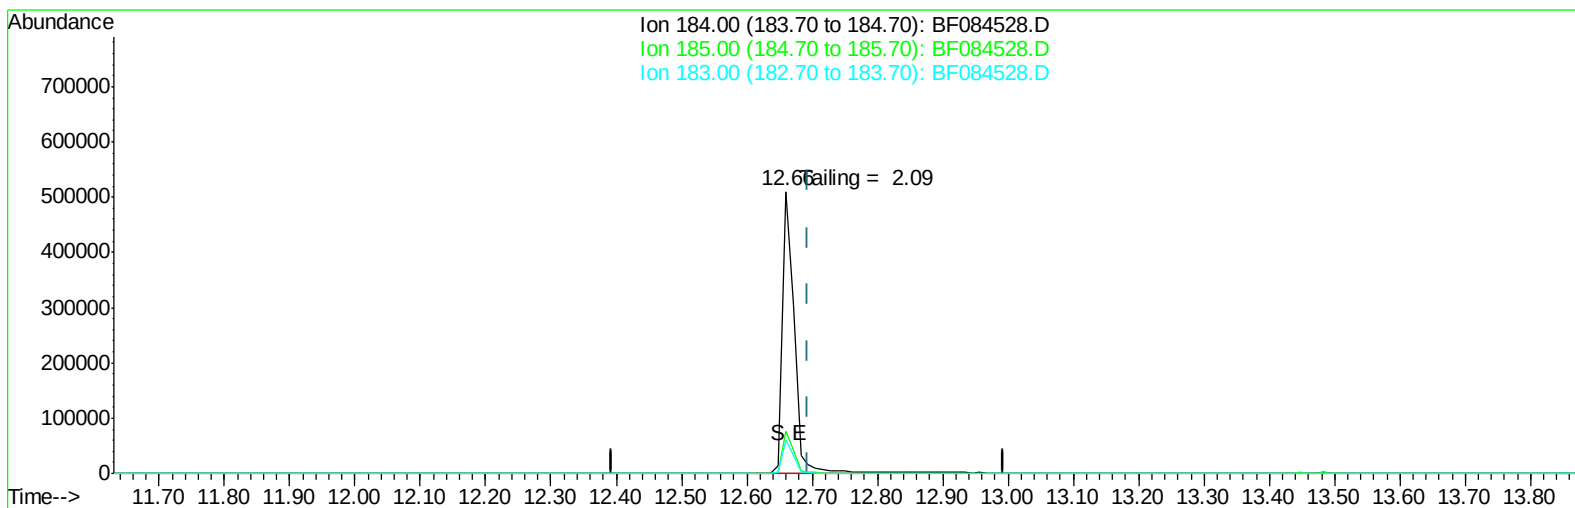

TIC: BF084528.D

(76) Benzidine

12.659min (-0.034) 2281.48ng

response 635362

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	15.13
183.00	12.30	11.79
0.00	0.00	0.00