


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011716\
 Data File : BF084528.D
 Acq On : 17 Jan 2016 10:30
 Operator : SJ/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 14 14:15:52 2016

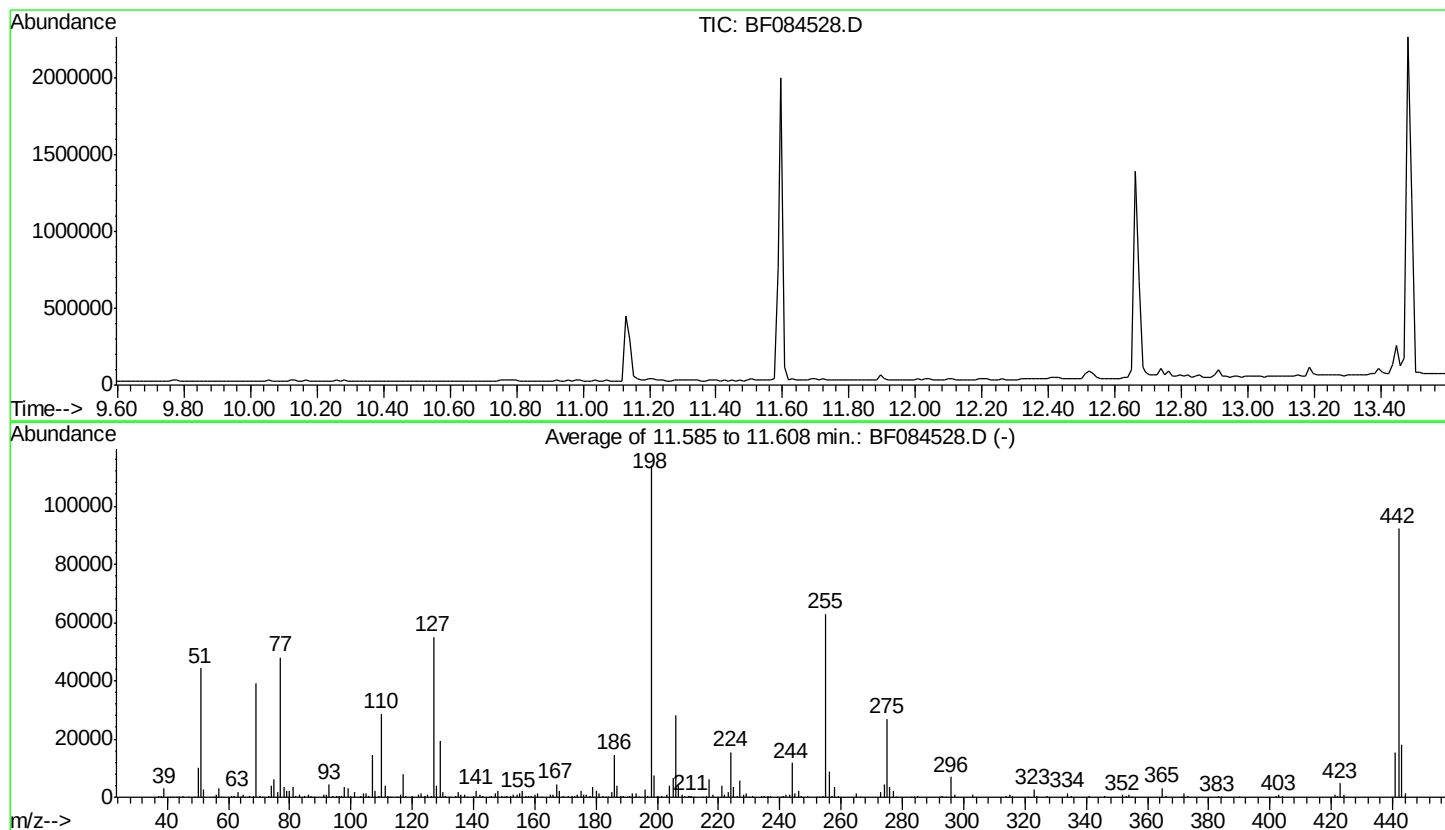

AutoFind: Scans 831, 832, 833; Background Corrected with Scan 827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.9	44328	PASS
68	69	0.00	2	1.7	675	PASS
69	198	0.00	100	34.2	38927	PASS
70	69	0.00	2	1.2	474	PASS
127	198	10	80	48.4	55100	PASS
197	198	0.00	2	0.4	456	PASS
198	198	100	100	100.0	113862	PASS
199	198	5	9	6.6	7519	PASS
275	198	10	60	23.7	26931	PASS
365	198	1	100	2.8	3144	PASS
441	442	0.01	24	16.6	15258	PASS
442	198	50	100	80.9	92159	PASS
443	442	15	24	19.4	17877	PASS