

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011717\
 Data File : BF092326.D
 Acq On : 17 Jan 2017 20:00
 Operator : UM/SJ
 Sample : I1230-03MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 B35MS

Quant Time: Jan 17 23:58:37 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 06 15:43:51 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.71	152	528863	20.00	ng	0.07
21) Naphthalene-d8	7.84	136	628164	20.00	ng	-0.09
38) Acenaphthene-d10	9.59	164	325803	20.00	ng	-0.09
63) Phenanthrene-d10	11.07	188	511562	20.00	ng	-0.09
75) Chrysene-d12	13.70	240	326392	20.00	ng	-0.09
86) Perylene-d12	15.05	264	281111	20.00	ng	-0.10

System Monitoring Compounds						
5) 2-Fluorophenol	5.15	112	1297127	40.95	ng	-0.09
7) Phenol-d6	6.22	99	1514978	39.18	ng	-0.09
23) Nitrobenzene-d5	7.14	82	1031457	91.31	ng	-0.08
41) 2,4,6-Tribromophenol	10.38	330	344463	127.76	ng	-0.09
44) 2-Fluorobiphenyl	8.93	172	1690893	110.16	ng	-0.08
78) Terphenyl-d14	12.64	244	1414666	105.12	ng	-0.10


Target Compounds						Qvalue
2) 1,4-Dioxane	1.99	88	143621	9.21	ng	# 93
3) Pyridine	2.61	79	453274	8.33	ng	100
4) n-Nitrosodimethylamine	2.56	42	202077	9.84	ng	93
6) Aniline	6.30	93	429508	8.55	ng	# 22
8) 2-Chlorophenol	6.35	128	415310	11.53	ng	89
10) Phenol	6.23	94	541323	12.28	ng	87
11) bis(2-Chloroethyl)ether	6.30	93	429508	12.25	ng	98
12) 1,3-Dichlorobenzene	6.58	146	432856	11.25	ng	99
13) 1,4-Dichlorobenzene	6.72	146	413580	10.56	ng	98
14) 1,2-Dichlorobenzene	6.72	146	413580	12.18	ng	99
15) Benzyl Alcohol	6.71	79	357944	11.91	ng	94
16) 2,2'-oxybis(1-Chloropropan	6.85	45	609725	11.68	ng	53
17) 2-Methylphenol	7.00	107	505782	17.46	ng	# 71
18) Hexachloroethane	7.07	117	162361	11.19	ng	89
19) n-Nitroso-di-n-propylamine	6.99	70	318345	12.37	ng	98
20) 3+4-Methylphenols	7.00	107	505782	14.63	ng	# 69
22) Acetophenone	6.98	105	626253	40.42	ng	# 93
24) Nitrobenzene	7.15	77	464370	38.60	ng	99
25) Isophorone	7.39	82	851685	40.86	ng	94
26) 2-Nitrophenol	7.47	139	238160	40.14	ng	96
27) 2,4-Dimethylphenol	7.52	122	391772	39.81	ng	99
28) bis(2-Chloroethoxy)methane	7.60	93	521465	41.26	ng	97
29) 2,4-Dichlorophenol	7.72	162	380190	45.62	ng	90
30) 1,2,4-Trichlorobenzene	7.79	180	359132	39.33	ng	96
31) Naphthalene	7.87	128	1244965	43.30	ng	99
32) Benzoic acid	7.65	122	62354	8.54	ng	98
33) 4-Chloroaniline	7.92	127	232925	17.97	ng	98
34) Hexachlorobutadiene	7.98	225	189200	39.25	ng	99
35) Caprolactam	8.30	113	61726	22.54	ng	# 71
36) 4-Chloro-3-methylphenol	8.44	107	399147	41.63	ng	88
37) 2-Methylnaphthalene	8.55	142	754099	42.39	ng	100
39) 1,2,4						

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011717\
 Data File : BF092326.D
 Acq On : 17 Jan 2017 20:00
 Operator : UM/SJ
 Sample : I1230-03MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 B35MS

Quant Time: Jan 17 23:58:37 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 06 15:43:51 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
43) 2,4,5-Trichlorophenol	8.90	196	242056	40.86	ng	99
45) 1,1'-Biphenyl	9.02	154	1014851	45.49	ng	99
46) 2-Chloronaphthalene	9.04	162	777845	44.03	ng	99
47) 2-Nitroaniline	9.15	65	230180	36.59	ng	98
48) Acenaphthylene	9.46	152	1157165	42.59	ng	97
49) Dimethylphthalate	9.33	163	962652	46.20	ng	98
50) 2,6-Dinitrotoluene	9.40	165	213673	46.85	ng	95
51) Acenaphthene	9.63	154	731252	39.70	ng	98
52) 3-Nitroaniline	9.56	138	133275	23.61	ng	95
53) 2,4-Dinitrophenol	9.68	184	95524	37.64	ng	# 85
54) Dibenzofuran	9.80	168	1039327	41.78	ng	95
55) 4-Nitrophenol	9.80	139	660387	172.32	ng	# 10
56) 2,4-Dinitrotoluene	9.80	165	226697	39.60	ng	# 72
57) Fluorene	10.14	166	798089	44.10	ng	100
58) 2,3,4,6-Tetrachlorophenol	9.92	232	183734	39.21	ng	98
59) Diethylphthalate	10.03	149	806212	39.84	ng	99
60) 4-Chlorophenyl-phenylether	10.13	204	323545	40.83	ng	99
61) 4-Nitroaniline	10.18	138	202466	34.61	ng	96
62) Azobenzene	10.29	77	970268	43.55	ng	99
64) 4,6-Dinitro-2-methylphenol	10.21	198	121161	39.17	ng	# 56
65) n-Nitrosodiphenylamine	10.26	169	679171	44.74	ng	99
66) 4-Bromophenyl-phenylether	10.62	248	246215	46.27	ng	# 84
67) Hexachlorobenzene	10.68	284	236487	41.58	ng	# 78
68) Atrazine	10.79	200	233184	47.62	ng	98
69) Pentachlorophenol	10.88	266	171658	61.50	ng	98
70) Phenanthrene	11.09					






#1
 1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 6.71 min Scan# 431
 Delta R.T. 0.07 min
 Lab File: BF092326.D
 Acq: 17 Jan 2017 20:00

Instrument :
 BNA_F
 ClientSampleID :
 B35MS

Tgt Ion:152 Resp: 528863
 Ion Ratio Lower Upper
 152 100
 150 153.8 124.9 187.3
 115 61.5 46.0 69.0




Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E






#2
 1,4-Dioxane
 Concen: 9.21 ng
 RT: 1.99 min Scan# 18
 Delta R.T. -0.09 min
 Lab File: BF092326.D
 Acq: 17 Jan 2017 20:00

Tgt Ion: 88 Resp: 143621
 Ion Ratio Lower Upper
 88 100
 58 75.9 57.8 86.8
 43 35.1 22.3 33.5#



Abundance Ion 88.00 (87.70 to 88.70): BF0
 Ion 58.00 (57.70 to 58.70): BF0
 Ion 43.00 (42.70 to 43.70): BF0



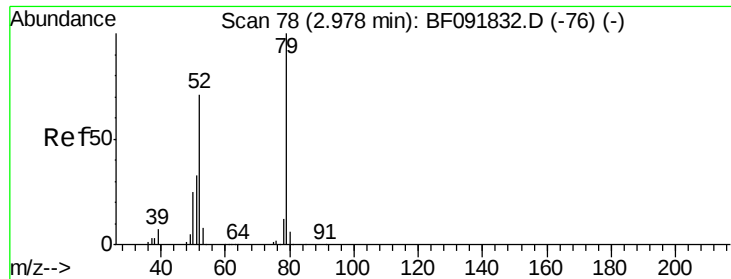

#3

Pyridine

Concen: 8.33 ng

RT: 2.61 min Scan# 72

Delta R.T. -0.12 min

Lab File: BF092326.D

Acq: 17 Jan 2017 20:00

Instrument :

BNA_F

ClientSampleId :

B35MS


Tgt Ion: 79 Resp: 453274

Ion Ratio Lower Upper

79 100

52 71.3 57.1 85.7



51 34.6 27.3 40.9



Abundance Ion 79.00 (78.70 to 79.70): BF0

Ion 52.00 (51.70 to 52.70): BF0

Ion 51.00 (50.70 to 51.70): BF0



#4

n-Nitrosodimethylamine

Concen: 9.84 ng

RT: 2.56 min Scan# 68

Delta R.T. -0.12 min

Lab File: BF092326.D

Acq: 17 Jan 2017 20:00


Tgt Ion: 42 Resp: 202077

Ion Ratio Lower Upper

42 100

74 137.0 117.0 175.4



44 7.6 5.5 8.3




Abundance Ion 42.00 (41.70 to 42.70): BF0

Ion 74.00 (73.70 to 74.70): BF0

Ion 44.00 (43.70 to 44.70): BF0





#5

2-Fluorophenol

Concen: 40.95 ng

RT: 5.15 min Scan# 294

Delta R.T. -0.09 min

Lab File: BF092326.D

Acq: 17 Jan 2017 20:00

Instrument :

BNA_F

ClientSampleId :

B35MS


Tgt Ion: 112 Resp: 1297127

Ion Ratio Lower Upper

112 100

64 54.5 46.1 69.1




63 27.6 23.8 35.6



Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0



#6

Aniline

Concen: 8.55 ng

RT: 6.30 min Scan# 395

Delta R.T. -0.01 min

Lab File: BF092326.D

Acq: 17 Jan 2017 20:00


Tgt Ion: 93 Resp: 429508

Ion Ratio Lower Upper

93 100

66 0.8 76.2 114.2#



65 25.2 49.3 73.9#



Abundance Ion 93.00 (92.70 to 93.70): BF0

Ion 66.00 (65.70 to 66.70): BF0

Ion 65.00 (64.70 to 65.70): BF0





#7

Phenol-d6

Concen: 39.18 ng

RT: 6.22 min Scan# 388

Delta R.T. -0.09 min

Lab File: BF092326.D

Acq: 17 Jan 2017 20:00

Instrument :

BNA_F

ClientSampleId :

B35MS


Tgt Ion: 99 Resp: 1514978

Ion Ratio Lower Upper

99 100

42 19.9 15.6 23.4




71 34.3 27.5 41.3



Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0



#8

2-Chlorophenol

Concen: 11.53 ng

RT: 6.35 min Scan# 399

Delta R.T. -0.09 min

Lab File: BF092326.D

Acq: 17 Jan 2017 20:00


Tgt Ion: 128 Resp: 415310

Ion Ratio Lower Upper

128 100

130 34.0 12.3 52.3



64 40.7 32.2 72.2




Abundance Ion 128.00 (127.70 to 128.70): E

Ion 130.00 (129.70 to 130.70): E

Ion 64.00 (63.70 to 64.70): BF0





#10

Phenol

Concen: 12.28 ng

RT: 6.23 min Scan# 389

Delta R.T. -0.09 min

Lab File: BF092326.D

Acq: 17 Jan 2017 20:00

Instrument :

BNA_F

ClientSampleId :

B35MS


Tgt Ion: 94 Resp: 541323

Ion Ratio Lower Upper

94 100

65 35.2 21.4 61.4




66 51.8 44.0 84.0



Abundance Ion 94.00 (93.70 to 94.70): BF0

Ion 65.00 (64.70 to 65.70): BF0

Ion 66.00 (65.70 to 66.70): BF0



#11

bis(2-Chloroethyl)ether

Concen: 12.25 ng

RT: 6.30 min Scan# 395

Delta R.T. -0.09 min

Lab File: BF092326.D

Acq: 17 Jan 2017 20:00


Tgt Ion: 93 Resp: 429508

Ion Ratio Lower Upper

93 100

63 78.6 60.4 100.4



95 33.0 12.8 52.8




Abundance Ion 93.00 (92.70 to 93.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

Ion 95.00 (94.70 to 95.70): BF0





#12

1,3-Dichlorobenzene

Concen: 11.25 ng

RT: 6.58 min Scan# 419

Delta R.T. -0.01 min

Lab File: BF092326.D

Acq: 17 Jan 2017 20:00

Instrument :

BNA_F

ClientSampleId :

B35MS


Tgt Ion:146 Resp: 432856

Ion Ratio Lower Upper




146 100

148 65.6 53.4 80.0

75 23.6 18.5 27.7



Abundance Ion 146.00 (145.70 to 146.70): E
Ion 148.00 (147.70 to 148.70): E
Ion 75.00 (74.70 to 75.70): BF0



#13

1,4-Dichlorobenzene

Concen: 10.56 ng

RT: 6.72 min Scan# 432

Delta R.T. 0.06 min

Lab File: BF092326.D

Acq: 17 Jan 2017 20:00


Tgt Ion:146 Resp: 413580

Ion Ratio Lower Upper



146 100


148 64.8 50.6 76.0

111 44.2 36.2 54.4



Abundance Ion 146.00 (145.70 to 146.70): E
Ion 148.00 (147.70 to 148.70): E
Ion 111.00 (110.70 to 111.70): E









#14
 1,2-Dichlorobenzene
 Concen: 12.18 ng
 RT: 6.72 min Scan# 432
 Delta R.T. -0.09 min
 Lab File: BF092326.D
 Acq: 17 Jan 2017 20:00




Instrument :
 BNA_F
 ClientSampleId :
 B35MS


Tgt Ion: 146 Resp: 413580
 Ion Ratio Lower Upper
 146 100
 148 64.8 52.2 78.2
 111 44.2 36.2 54.2



#15
 Benzyl Alcohol
 Concen: 11.91 ng
 RT: 6.71 min Scan# 431
 Delta R.T. -0.09 min
 Lab File: BF092326.D
 Acq: 17 Jan 2017 20:00

Tgt Ion: 79 Resp: 357944
 Ion Ratio Lower Upper
 79 100
 108 69.5 61.4 92.0
 77 66.2 50.9 76.3









#16
2,2'-oxybis(1-Chloropropane)
Concen: 11.68 ng
RT: 6.85 min Scan# 443
Delta R.T. -0.09 min
Lab File: BF092326.D
Acq: 17 Jan 2017 20:00




Instrument :
BNA_F
ClientSampleId :
B35MS


Tgt Ion: 45 Resp: 609725
Ion Ratio Lower Upper
45 100
77 33.3 0.0 34.6
79 29.5 0.0 31.2



#17
2-Methylphenol
Concen: 17.46 ng
RT: 7.00 min Scan# 456
Delta R.T. 0.07 min
Lab File: BF092326.D
Acq: 17 Jan 2017 20:00

Tgt Ion: 107 Resp: 505782
Ion Ratio Lower Upper
107 100
108 83.8 93.0 139.6#
77 34.4 39.8 59.8#
79 24.7 38.0 57.0#





#18

Hexachloroethane

Concen: 11.19 ng

RT: 7.07 min Scan# 462

Delta R.T. -0.09 min

Lab File: BF092326.D

Acq: 17 Jan 2017 20:00

Instrument :

BNA_F

ClientSampleId :

B35MS


Tgt Ion: 117 Resp: 162361

Ion Ratio Lower Upper

117 100

119 100.3 78.1 117.1




201 116.6 78.6 117.8



Abundance Ion 117.00 (116.70 to 117.70): E

Ion 119.00 (118.70 to 119.70): E

Ion 201.00 (200.70 to 201.70): E



#19

n-Nitroso-di-n-propylamine

Concen: 12.37 ng

RT: 6.99 min Scan# 455

Delta R.T. -0.09 min


Lab File: BF092326.D

Acq: 17 Jan 2017 20:00

Tgt Ion: 70 Resp: 318345

Ion Ratio Lower Upper

70 100



#20

3+4-Methylphenols

Concen: 14.63 ng

RT: 7.00 min Scan# 456

Delta R.T. -0.09 min

Lab File: BF092326.D

Acq: 17 Jan 2017 20:00

Instrument :

BNA_F

ClientSampleId :

B35MS

Tgt Ion:107 Resp: 505782


Ion Ratio Lower Upper

107 100

108 83.8 73.0 113.0

77 34.4 71.3 111.3#

79 24.7 11.1 51.1






Abundance Ion 107.00 (106.70 to 107.70): E

Ion 108.00 (107.70 to 108.70): E

Ion 77.00 (76.70 to 77.70): BF0

Ion 79.00 (78.70 to 79.70): BF0



#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.84 min Scan# 530

Delta R.T. -0.09 min


Lab File: BF092326.D

Acq: 17 Jan 2017 20:00

Tgt Ion:136 Resp: 628164

Ion Ratio Lower Upper


136 1






#22
Acetophenone
Concen: 40.42 ng
RT: 6.98 min Scan# 454
Delta R.T. -0.09 min
Lab File: BF092326.D
Acq: 17 Jan 2017 20:00

Instrument :
BNA_F
ClientSampleId :
B35MS

Tgt Ion: 105 Resp: 626253
Ion Ratio Lower Upper
105 100
71 2.5 3.2 4.8#
51 26.7 26.2 39.4
120 20.5 16.6 24.8




Abundance Ion 105.00 (104.70 to 105.70): E
Ion 71.00 (70.70 to 71.70): BF0
Ion 51.00 (50.70 to 51.70): BF0
Ion 120.00 (119.70 to 120.70): E






#23
Nitrobenzene-d5
Concen: 91.31 ng
RT: 7.14 min Scan# 468
Delta R.T. -0.08 min
Lab File: BF092326.D
Acq: 17 Jan 2017 20:00

Tgt Ion: 82 Resp: 1031457
Ion Ratio Lower Upper
82 100
128 47.8 34.6 52.0
54 44.6 39.5 59.3



Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0





#24

Nitrobenzene

Concen: 38.60 ng

RT: 7.15 min Scan# 469

Delta R.T. -0.09 min

Lab File: BF092326.D

Acq: 17 Jan 2017 20:00

Instrument :

BNA_F

ClientSampleId :

B35MS


Tgt Ion: 77 Resp: 464370

Ion Ratio Lower Upper

77 100

123 42.0 33.0 49.4




65 13.6 11.2 16.8



Abundance Ion 77.00 (76.70 to 77.70): BF0

Ion 123.00 (122.70 to 123.70): BF0

Ion 65.00 (64.70 to 65.70): BF0



#25

Isophorone

Concen: 40.86 ng

RT: 7.39 min Scan# 490

Delta R.T. -0.09 min

Lab File: BF092326.D

Acq: 17 Jan 2017 20:00


Tgt Ion: 82 Resp: 851685

Ion Ratio Lower Upper

82 100

95 6.3 5.6 8.4


138 14.7 14.6 22.0



Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 95.00 (94.70 to 95.70): BF0





Ion 138.00 (137.70



#26
2-Nitrophenol
Concen: 40.14 ng
RT: 7.47 min Scan# 497
Delta R.T. -0.09 min
Lab File: BF092326.D
Acq: 17 Jan 2017 20:00




Instrument :
BNA_F
ClientSampleId :
B35MS


Tgt Ion:139 Resp: 238160
Ion Ratio Lower Upper
139 100
109 26.5 23.3 34.9
65 50.7 42.7 64.1



#27
2,4-Dimethylphenol
Concen: 39.81 ng
RT: 7.52 min Scan# 502
Delta R.T. -0.09 min
Lab File: BF092326.D
Acq: 17 Jan 2017 20:00

Tgt Ion:122 Resp: 391772
Ion Ratio Lower Upper
122 100
107 116.4 94.1 141.1
121 57.1 46.0 69.0





#28

bis(2-Chloroethoxy)methane

Concen: 41.26 ng

RT: 7.60 min Scan# 509

Delta R.T. -0.09 min

Lab File: BF092326.D

Acq: 17 Jan 2017 20:00

Instrument :

BNA_F

ClientSampleId :

B35MS





Tgt Ion: 93 Resp: 521465

Ion Ratio Lower Upper

93 100

95 31.8 26.5 39.7

123 9.1 8.6 13.0



#29

2,4-Dichlorophenol

Concen: 45.62 ng

RT: 7.72 min Scan# 519

Delta R.T. -0.09 min

Lab File: BF092326.D

Acq: 17 Jan 2017 20:00



Tgt Ion: 162 Resp: 380190


Ion Ratio Lower Upper

162 100

164 63.1 46.8 86.8

98 40.7 9.1 49.1









#30
 1,2,4-Trichlorobenzene
 Concen: 39.33 ng
 RT: 7.79 min Scan# 525
 Delta R.T. -0.09 min
 Lab File: BF092326.D
 Acq: 17 Jan 2017 20:00

Instrument :
 BNA_F
 ClientSampleId :
 B35MS

Tgt Ion:180 Resp: 359132
 Ion Ratio Lower Upper
 180 100
 182 95.3 78.2 117.4
 145 31.9 21.6 32.4




Abundance Ion 180.00 (179.70 to 180.70): E
 Ion 182.00 (181.70 to 182.70): E
 Ion 145.00 (144.70 to 145.70): E






#31
 Naphthalene
 Concen: 43.30 ng
 RT: 7.87 min Scan# 532
 Delta R.T. -0.09 min
 Lab File: BF092326.D
 Acq: 17 Jan 2017 20:00

Tgt Ion:128 Resp: 1244965
 Ion Ratio Lower Upper
 128 100
 129 11.1 9.5 14.3
 127 13.1 10.8 16.2



Abundance Ion 128.00 (127.70 to 128.70): E
 Ion 129.00 (128.70 to 129.70): E
 Ion 127.00 (126.70 to 127.70): E





#32

Benzoic acid

Concen: 8.54 ng

RT: 7.65 min Scan# 513

Delta R.T. -0.10 min

Lab File: BF092326.D

Acq: 17 Jan 2017 20:00

Instrument :

BNA_F

ClientSampled :

B35MS


Tgt Ion:122 Resp: 62354

Ion Ratio Lower Upper

122 100

105 125.2 107.2 147.2




77 96.7 74.5 114.5



Abundance Ion 122.00 (121.70 to 122.70): E

Ion 105.00 (104.70 to 105.70): E

Ion 77.00 (76.70 to 77.70): BF0



#33

4-Chloroaniline

Concen: 17.97 ng

RT: 7.92 min Scan# 537

Delta R.T. -0.09 min

Lab File: BF092326.D

Acq: 17 Jan 2017 20:00

Tgt Ion:127 Resp: 232925


Ion Ratio Lower Upper

127 100

129 32.2 26.3 39.5


65 34.0 25.8 38.8

92 20.4 16.1 24.1



Abundance Ion 127.00 (126.70 to 127.70): E


Ion 129.00 (






#34
Hexachlorobutadiene
Concen: 39.25 ng
RT: 7.98 min Scan# 542
Delta R.T. -0.10 min
Lab File: BF092326.D
Acq: 17 Jan 2017 20:00

Instrument :
BNA_F
ClientSampleId :
B35MS

Tgt Ion: 225 Resp: 189200
Ion Ratio Lower Upper
225 100
223 64.6 51.0 76.6
227 63.0 50.6 76.0




Abundance Ion 225.00 (224.70 to 225.70): E
Ion 223.00 (222.70 to 223.70): E
Ion 227.00 (226.70 to 227.70): E






#35
Caprolactam
Concen: 22.54 ng
RT: 8.30 min Scan# 570
Delta R.T. -0.09 min
Lab File: BF092326.D
Acq: 17 Jan 2017 20:00

Tgt Ion: 113 Resp: 61726
Ion Ratio Lower Upper
113 100
55 174.4 119.2 159.2#
56 132.5 83.8 123.8#



Abundance Ion 113.00 (112.70 to 113.70): E
Ion 55.00 (54.70 to 55.70): BF0
Ion 56.00 (55.70 to 56.70): BF0









#36
 4-Chloro-3-methylphenol
 Concen: 41.63 ng
 RT: 8.44 min Scan# 582
 Delta R.T. -0.07 min
 Lab File: BF092326.D
 Acq: 17 Jan 2017 20:00

Instrument :
 BNA_F
 ClientSampleId :
 B35MS

Tgt Ion:107 Resp: 399147
 Ion Ratio Lower Upper
 107 100
 144 27.8 19.3 28.9
 142 84.8 59.0 88.6




Abundance Ion 107.00 (106.70 to 107.70): E
 Ion 144.00 (143.70 to 144.70): E
 Ion 142.00 (141.70 to 142.70): E






#37
 2-Methylnaphthalene
 Concen: 42.39 ng
 RT: 8.55 min Scan# 592
 Delta R.T. -0.09 min
 Lab File: BF092326.D
 Acq: 17 Jan 2017 20:00

Tgt Ion:142 Resp: 754099
 Ion Ratio Lower Upper
 142 100
 141 88.9 71.0 106.6
 115 35.3 28.3 42.5



Abundance Ion 142.00 (141.70 to 142.70): E
 Ion 141.00 (140.70 to 141.70): E
 Ion 115.00 (114.70 to 115.70): E





#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.59 min Scan# 683

Delta R.T. -0.09 min

Lab File: BF092326.D

Acq: 17 Jan 2017 20:00

Instrument :

BNA_F

ClientSampleId :

B35MS


Tgt Ion:164 Resp: 325803

Ion Ratio Lower Upper

164 100

162 99.9 80.2 120.2




160 44.0 36.9 55.3



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E



#39

1,2,4,5-Tetrachlorobenzene

Concen: 42.36 ng

RT: 8.72 min Scan# 607

Delta R.T. -0.09 min


Lab File: BF092326.D

Acq: 17 Jan 2017 20:00

Tgt Ion:216 Resp: 348710

Ion Ratio Lower Upper





216 100



#40
Hexachlorocyclopentadiene
Concen: 63.85 ng
RT: 8.71 min Scan# 606
Delta R.T. -0.09 min
Lab File: BF092326.D
Acq: 17 Jan 2017 20:00




Instrument :
BNA_F
ClientSampleId :
B35MS


Tgt Ion:237 Resp: 230960
Ion Ratio Lower Upper
237 100
235 63.7 41.2 81.2
272 14.0 0.0 35.4



#41
2,4,6-Tribromophenol
Concen: 127.76 ng
RT: 10.38 min Scan# 752
Delta R.T. -0.09 min
Lab File: BF092326.D
Acq: 17 Jan 2017 20:00

Tgt Ion:330 Resp: 344463
Ion Ratio Lower Upper
330 100
332 96.0 77.4 116.2
141 40.5 34.1 51.1









#42
 2,4,6-Trichlorophenol
 Concen: 38.72 ng
 RT: 8.85 min Scan# 618
 Delta R.T. -0.08 min
 Lab File: BF092326.D
 Acq: 17 Jan 2017 20:00




Instrument :
 BNA_F
 ClientSampleId :
 B35MS


Tgt Ion:196 Resp: 222883
 Ion Ratio Lower Upper
 196 100
 198 102.8 82.1 123.1
 200 32.2 27.0 40.4



#43
 2,4,5-Trichlorophenol
 Concen: 40.86 ng
 RT: 8.90 min Scan# 622
 Delta R.T. -0.08 min
 Lab File: BF092326.D
 Acq: 17 Jan 2017 20:00

Tgt Ion:196 Resp: 242056
 Ion Ratio Lower Upper
 196 100
 198 99.9 79.4 119.2
 97 63.1 51.5 77.3
 132 34.9 27.4 41.2





#44

2-Fluorobiphenyl

Concen: 110.16 ng

RT: 8.93 min Scan# 625

Delta R.T. -0.08 min

Lab File: BF092326.D

Acq: 17 Jan 2017 20:00

Instrument :

BNA_F

ClientSampleId :

B35MS


Tgt Ion:172 Resp: 1690893

Ion Ratio Lower Upper

172 100

171 34.9 29.4 44.0




170 23.8 20.2 30.4



Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E



#45

1,1'-Biphenyl

Concen: 45.49 ng

RT: 9.02 min Scan# 633

Delta R.T. -0.09 min

Lab File: BF092326.D


Acq: 17 Jan 2017 20:00

Tgt Ion:154 Resp: 1014851

Ion Ratio Lower Upper

154 100





153 40.6 20.9 60.9



#46
 2-Chloronaphthalene
 Concen: 44.03 ng
 RT: 9.04 min Scan# 635
 Delta R.T. -0.09 min
 Lab File: BF092326.D
 Acq: 17 Jan 2017 20:00




Instrument :
 BNA_F
 ClientSampleId :
 B35MS


Tgt Ion: 162 Resp: 777845
 Ion Ratio Lower Upper
 162 100
 127 38.9 30.7 46.1
 164 33.3 27.6 41.4



#47
 2-Nitroaniline
 Concen: 36.59 ng
 RT: 9.15 min Scan# 644
 Delta R.T. -0.09 min
 Lab File: BF092326.D
 Acq: 17 Jan 2017 20:00

Tgt Ion: 65 Resp: 230180
 Ion Ratio Lower Upper
 65 100
 92 66.5 53.9 80.9
 138 93.1 76.8 115.2









#48
Acenaphthylene
Concen: 42.59 ng
RT: 9.46 min Scan# 671
Delta R.T. -0.09 min
Lab File: BF092326.D
Acq: 17 Jan 2017 20:00




Instrument :
BNA_F
ClientSampleId :
B35MS


Tgt Ion:152 Resp: 1157165
Ion Ratio Lower Upper
152 100
151 19.5 16.9 25.3
153 13.2 11.4 17.2



#49
Dimethylphthalate
Concen: 46.20 ng
RT: 9.33 min Scan# 660
Delta R.T. -0.09 min
Lab File: BF092326.D
Acq: 17 Jan 2017 20:00

Tgt Ion:163 Resp: 962652
Ion Ratio Lower Upper
163 100
194 3.1 3.0 4.4
164 10.6 8.0 12.0









#50
2,6-Dinitrotoluene
Concen: 46.85 ng
RT: 9.40 min Scan# 666
Delta R.T. -0.08 min
Lab File: BF092326.D
Acq: 17 Jan 2017 20:00

Instrument :
BNA_F
ClientSampleId :
B35MS

Tgt Ion:165 Resp: 213673
Ion Ratio Lower Upper
165 100
63 41.4 36.2 54.4
89 48.0 40.2 60.4




Abundance Ion 165.00 (164.70 to 165.70): E
Ion 63.00 (62.70 to 63.70): BF0
Ion 89.00 (88.70 to 89.70): BF0






#51
Acenaphthene
Concen: 39.70 ng
RT: 9.63 min Scan# 686
Delta R.T. -0.09 min
Lab File: BF092326.D
Acq: 17 Jan 2017 20:00

Tgt Ion:154 Resp: 731252
Ion Ratio Lower Upper
154 100
153 112.9 88.6 133.0
152 51.3 41.6 62.4



Abundance Ion 154.00 (153.70 to 154.70): E
Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E





#52

3-Nitroaniline

Concen: 23.61 ng

RT: 9.56 min Scan# 680

Delta R.T. -0.09 min

Lab File: BF092326.D

Acq: 17 Jan 2017 20:00

Instrument :

BNA_F

ClientSampleId :

B35MS


Tgt Ion:138 Resp: 133275

Ion Ratio Lower Upper

138 100

108 10.7 8.5 12.7




92 128.0 97.8 146.8



Abundance Ion 138.00 (137.70 to 138.70): E

Ion 108.00 (107.70 to 108.70): E

Ion 92.00 (91.70 to 92.70): E



#53

2,4-Dinitrophenol

Concen: 37.64 ng

RT: 9.68 min Scan# 691

Delta R.T. -0.08 min

Lab File: BF092326.D

Acq: 17 Jan 2017 20:00


Tgt Ion:184 Resp: 95524

Ion Ratio Lower Upper


184 100

63 55.9 28.4 42.6#

154 57.5 44.3 66.5




Abundance Ion 184.00 (183.70 to 184.70): E






#54
Dibenzofuran
Concen: 41.78 ng
RT: 9.80 min Scan# 701
Delta R.T. -0.09 min
Lab File: BF092326.D
Acq: 17 Jan 2017 20:00

Instrument :
BNA_F
ClientSampleId :
B35MS

Tgt Ion:168 Resp: 1039327
Ion Ratio Lower Upper
168 100
139 36.8 32.6 49.0
169 13.2 11.3 16.9




Abundance Ion 168.00 (167.70 to 168.70): E
Ion 139.00 (138.70 to 139.70): E
Ion 169.00 (168.70 to 169.70): E






#55
4-Nitrophenol
Concen: 172.32 ng
RT: 9.80 min Scan# 701
Delta R.T. -0.03 min
Lab File: BF092326.D
Acq: 17 Jan 2017 20:00

Tgt Ion:139 Resp: 660387
Ion Ratio Lower Upper
139 100
109 2.7 52.2 92.2#
65 7.3 85.8 125.8#



Abundance Ion 139.00 (138.70 to 139.70): E
Ion 109.00 (108.70 to 109.70): E
Ion 65.00 (64.70 to 65.70): BF0









#56
2,4-Dinitrotoluene
Concen: 39.60 ng
RT: 9.80 min Scan# 701
Delta R.T. -0.09 min
Lab File: BF092326.D
Acq: 17 Jan 2017 20:00

Instrument :
BNA_F
ClientSampleId :
B35MS

Tgt Ion:165 Resp: 226697
Ion Ratio Lower Upper
165 100
63 72.7 40.2 60.4#
89 101.0 62.5 93.7#
182 2.1 1.8 2.8




Abundance Ion 165.00 (164.70 to 165.70): E
Ion 63.00 (62.70 to 63.70): BF0
Ion 89.00 (88.70 to 89.70): BF0
Ion 182.00 (181.70 to 182.70): E






#57
Fluorene
Concen: 44.10 ng
RT: 10.14 min Scan# 731
Delta R.T. -0.09 min
Lab File: BF092326.D
Acq: 17 Jan 2017 20:00

Tgt Ion:166 Resp: 798089
Ion Ratio Lower Upper
166 100
165 97.5 77.8 116.8
167 13.2 10.8 16.2



Abundance Ion 166.00 (165.70 to 166.70): E
Ion 165.00 (164.70 to 165.70): E
Ion 167.00 (166.70 to 167.70): E









#58
 2,3,4,6-Tetrachlorophenol
 Concen: 39.21 ng
 RT: 9.92 min Scan# 712
 Delta R.T. -0.09 min
 Lab File: BF092326.D
 Acq: 17 Jan 2017 20:00


Instrument :
 BNA_F
 ClientSampleId :
 B35MS

Tgt Ion:	232	Resp:	183734
Ion	Ratio	Lower	Upper
232	100		
131	52.8	40.1	60.1
130	2.4	1.8	2.8
166	33.2	26.6	39.8



Abundance Ion 232.00 (231.70 to 232.70): E
 Ion 131.00 (130.70 to 131.70): E
 Ion 130.00 (129.70 to 130.70): E
 Ion 166.00 (165.70 to 166.70): E





#60

4-Chlorophenyl-phenylether

Concen: 40.83 ng

RT: 10.13 min Scan# 730

Delta R.T. -0.09 min

Lab File: BF092326.D

Acq: 17 Jan 2017 20:00

Instrument :

BNA_F

ClientSampleId :

B35MS


Tgt Ion:204 Resp: 323545

Ion Ratio Lower Upper

204 100

206 32.5 25.8 38.6




141 75.7 59.4 89.0



Abundance Ion 204.00 (203.70 to 204.70): E

Ion 206.00 (205.70 to 206.70): E

Ion 141.00 (140.70 to 141.70): E



#61

4-Nitroaniline

Concen: 34.61 ng

RT: 10.18 min Scan# 734

Delta R.T. -0.09 min

Lab File: BF092326.D

Acq: 17 Jan 2017 20:00


Tgt Ion:138 Resp: 202466

Ion Ratio Lower Upper


138 100

92 51.9 31.7 71.7

108 67.2 52.6 92.6



Abundance Ion 138.00 (137.70 to 138.70): E</



#62

Azobenzene

Concen: 43.55 ng

RT: 10.29 min Scan# 744

Delta R.T. -0.09 min

Lab File: BF092326.D

Acq: 17 Jan 2017 20:00

Instrument :

BNA_F

ClientSampleId :

B35MS

Tgt Ion: 77 Resp: 970268


Ion Ratio Lower Upper

77 100

182 18.3 0.0 39.3

105 22.7 2.3 42.3

51 28.2 8.9 48.9




Abundance Ion 77.00 (76.70 to 77.70): BF0



Ion 182.00 (181.70 to 182.70): E

Ion 105.00 (104.70 to 105.70): E

Ion 51.00 (50.70 to 51.70): BF0



Time-->



#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.07 min Scan# 812

Delta R.T. -0.09 min

Lab File: BF092326.D


Acq: 17 Jan 2017 20:00

Tgt Ion: 188 Resp: 511562

Ion Ratio Lower Upper

188 100





94 8.8 10.0 15.0#



#64
 4,6-Dinitro-2-methylphenol
 Concen: 39.17 ng
 RT: 10.21 min Scan# 737
 Delta R.T. -0.08 min
 Lab File: BF092326.D
 Acq: 17 Jan 2017 20:00




Instrument :
 BNA_F
 ClientSampleId :
 B35MS


Tgt Ion:198 Resp: 121161
 Ion Ratio Lower Upper
 198 100
 51 57.3 6.7 46.7#
 105 56.3 16.6 56.6



#65
 n-Nitrosodiphenylamine
 Concen: 44.74 ng
 RT: 10.26 min Scan# 741
 Delta R.T. -0.09 min
 Lab File: BF092326.D
 Acq: 17 Jan 2017 20:00

Tgt Ion:169 Resp: 679171
 Ion Ratio Lower Upper
 169 100
 168 66.9 54.2 81.2
 167 37.1 30.2 45.4





#66

4-Bromophenyl-phenylether

Concen: 46.27 ng

RT: 10.62 min Scan# 773

Delta R.T. -0.09 min

Lab File: BF092326.D

Acq: 17 Jan 2017 20:00

Instrument :

BNA_F

ClientSampleId :

B35MS


Tgt Ion:248 Resp: 246215

Ion Ratio Lower Upper

248 100

250 98.6 76.9 115.3




141 56.8 68.2 102.4#



Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E



#67

Hexachlorobenzene

Concen: 41.58 ng

RT: 10.68 min Scan# 778

Delta R.T. -0.09 min

Lab File: BF092326.D

Acq: 17 Jan 2017 20:00


Tgt Ion:284 Resp: 236487


Ion Ratio Lower Upper

284 100

142 50.1 22.6 33.8#

249 34.0 25.4 38.0





#68

Atrazine

Concen: 47.62 ng

RT: 10.79 min Scan# 788

Delta R.T. -0.09 min

Lab File: BF092326.D

Acq: 17 Jan 2017 20:00

Instrument :

BNA_F

ClientSampleId :

B35MS


Tgt Ion:200 Resp: 233184

Ion Ratio Lower Upper

200 100

173 27.1 9.6 49.6




215 45.2 25.7 65.7



Abundance Ion 200.00 (199.70 to 200.70): E

Ion 173.00 (172.70 to 173.70): E

Ion 215.00 (214.70 to 215.70): E



#69

Pentachlorophenol

Concen: 61.50 ng

RT: 10.88 min Scan# 796

Delta R.T. -0.09 min

Lab File: BF092326.D

Acq: 17 Jan 2017 20:00

Tgt Ion:266 Resp: 171658

Ion Ratio Lower Upper

266 100

268 65.4 53.3 79.9