


Data Path : Z:\HPCHEM1\BNA F\Data\BF011717\  
 Data File : BF092317.D  
 Acq On : 17 Jan 2017 15:11  
 Operator : UM/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF122116.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Jan 06 15:43:51 2017

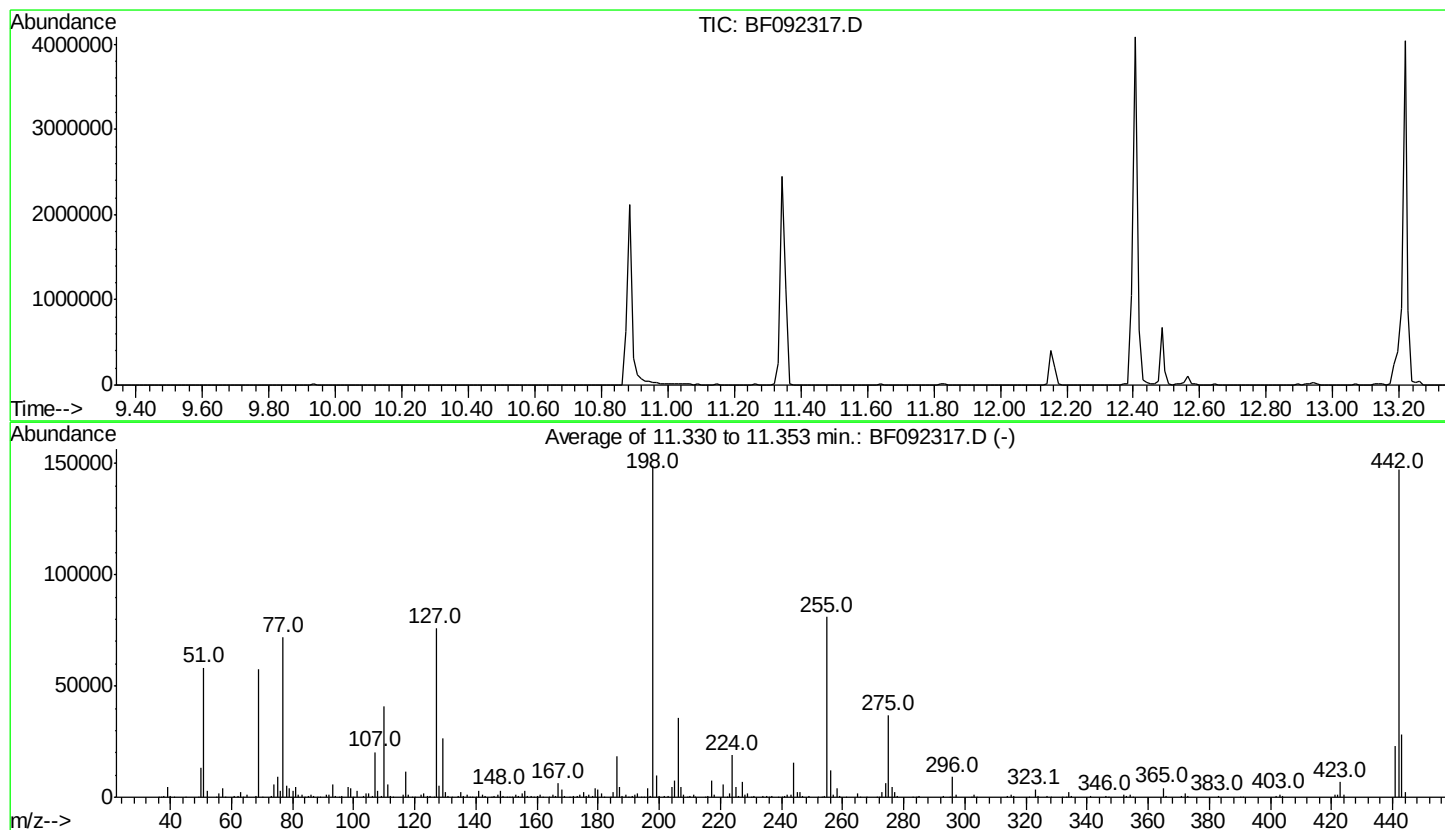

AutoFind: Scans 835, 836, 837; Background Corrected with Scan 831

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 39.1      | 58311   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.5       | 887     | PASS             |
| 69          | 198          | 0.00         | 100          | 38.7      | 57696   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.4       | 224     | PASS             |
| 127         | 198          | 10           | 80           | 50.8      | 75709   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.5       | 757     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 149085  | PASS             |
| 199         | 198          | 5            | 9            | 6.7       | 9994    | PASS             |
| 275         | 198          | 10           | 60           | 24.6      | 36610   | PASS             |
| 365         | 198          | 1            | 100          | 2.8       | 4140    | PASS             |
| 441         | 442          | 0.01         | 24           | 15.8      | 23276   | PASS             |
| 442         | 198          | 50           | 100          | 98.8      | 147236  | PASS             |
| 443         | 442          | 15           | 24           | 19.3      | 28402   | PASS             |