
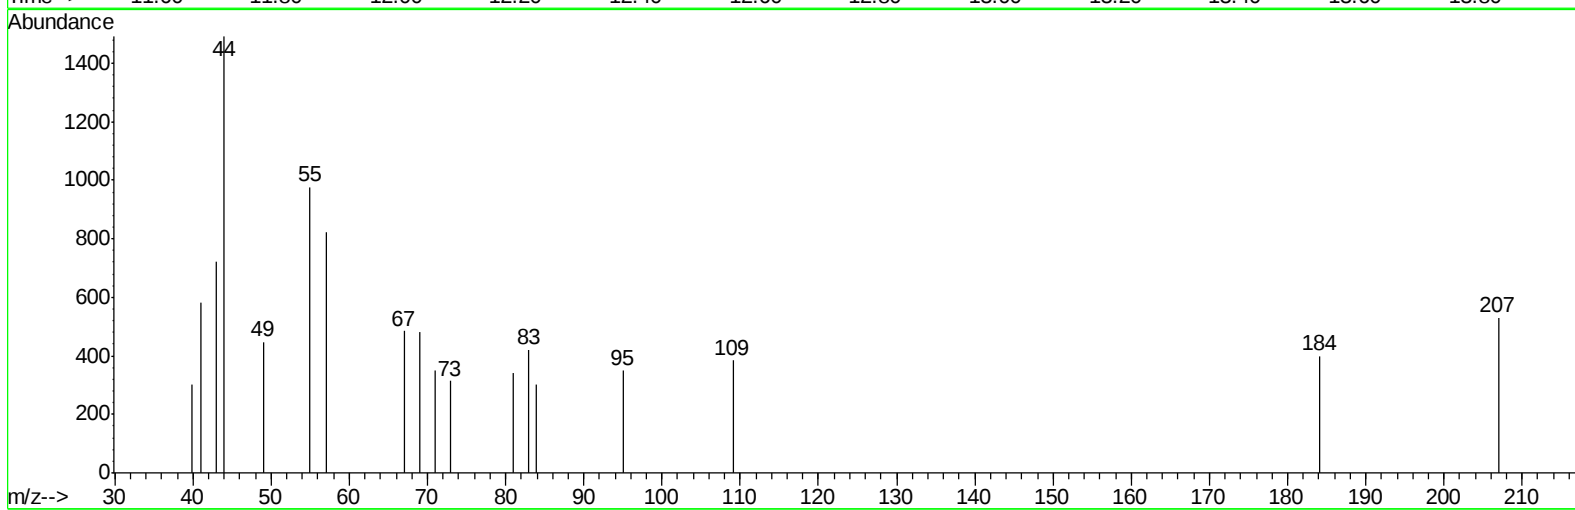


Data Path : Z:\HPCHEM1\BNA F\DATA\BF011718\
Data File : BF102146.D
Acq On : 17 Jan 2018 12:10
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 08:36:10 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 17 15:28:18 2018
Response via : Initial Calibration

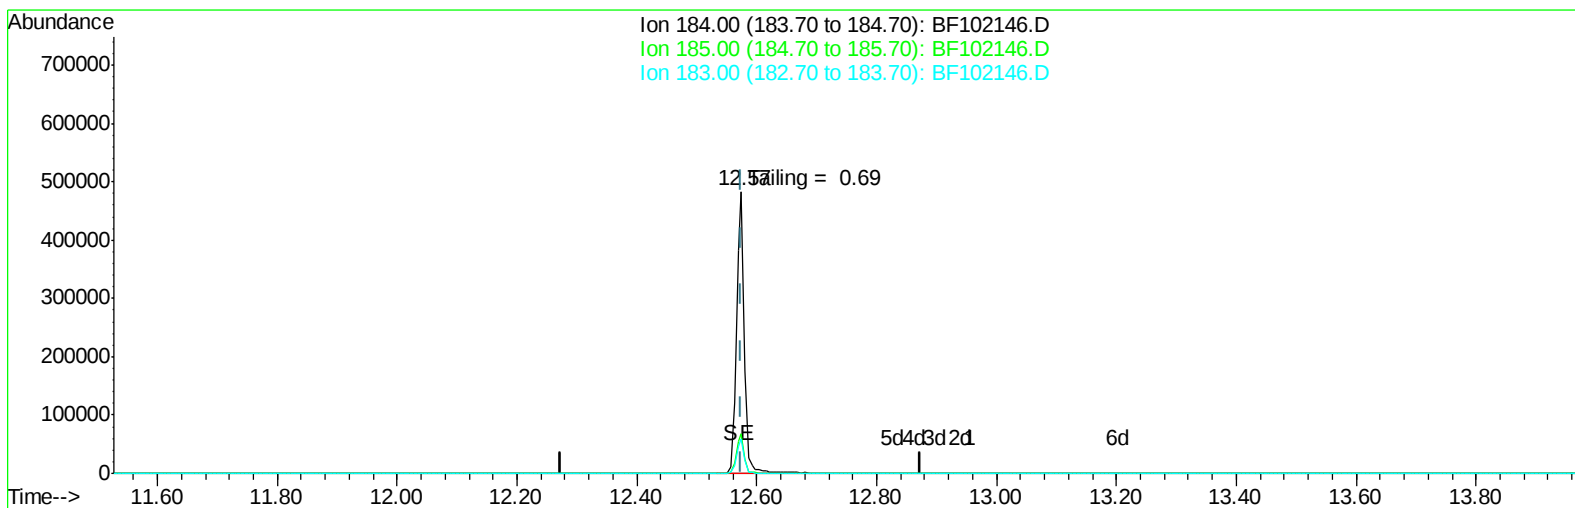

TIC: BF102146.D

(76) Benzidine



12.957min (+0.382) 27.04ng

response 141

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	0.00#
183.00	11.60	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF011718\
Data File : BF102146.D
Acq On : 17 Jan 2018 12:10
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 08:36:10 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 17 15:28:18 2018
Response via : Initial Calibration

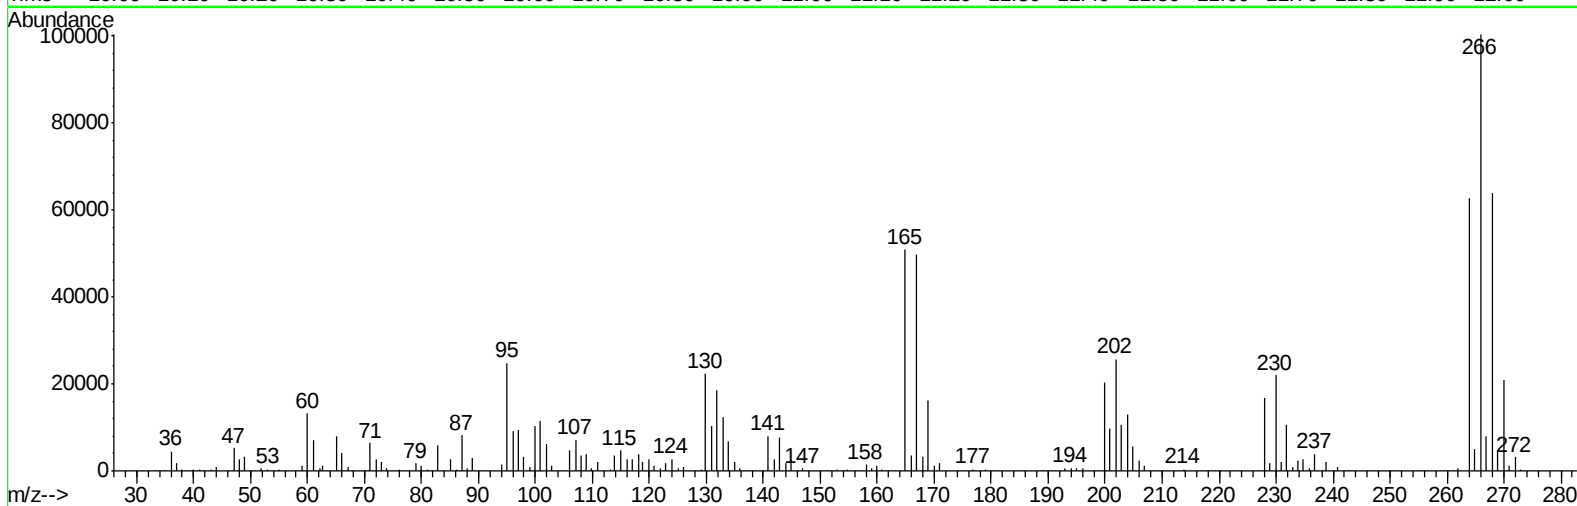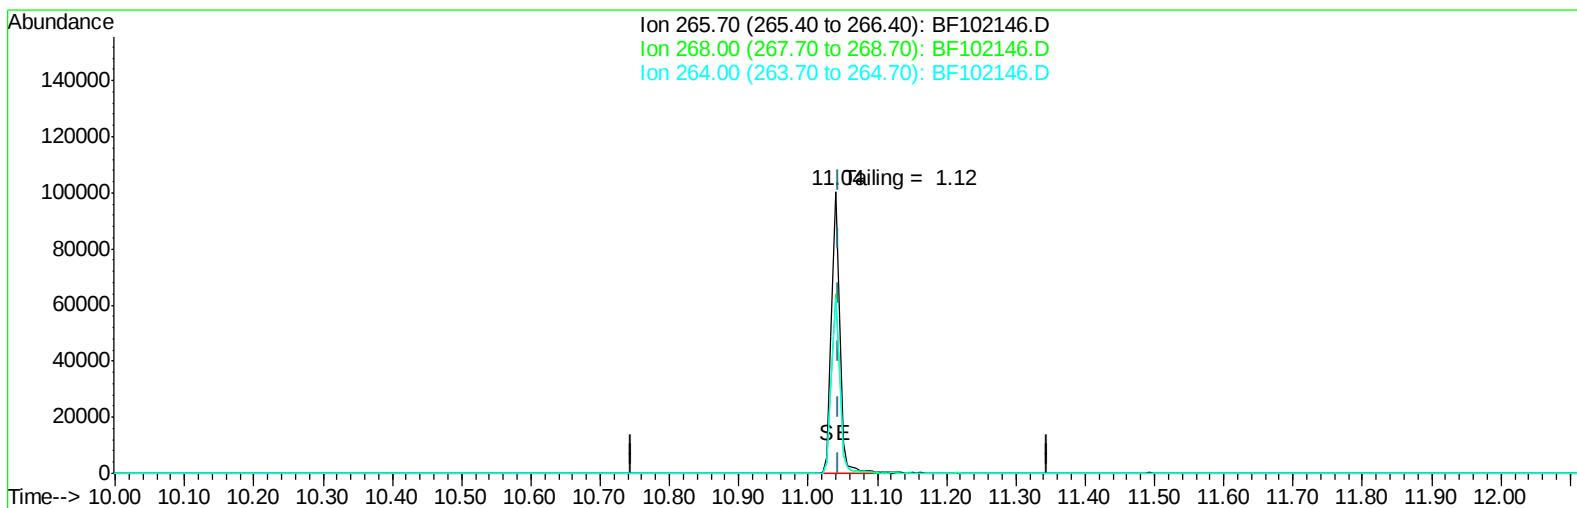

TIC: BF102146.D

(69) Pentachlorophenol (C)

11.039min (-0.006) 64729.50ng

response 82365

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.55
264.00	61.90	62.41
0.00	0.00	0.00