
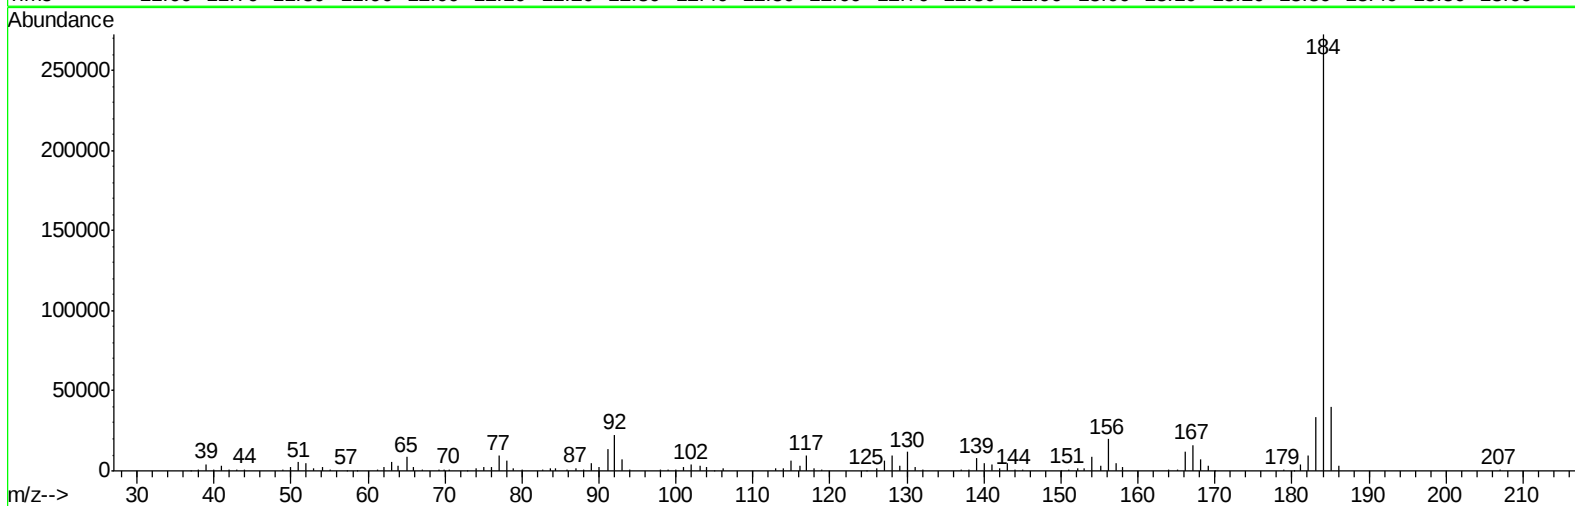


Data Path : Z:\HPCHEM1\BNA F\DATA\BF011718\
Data File : BF102171.D
Acq On : 18 Jan 2018 1:41
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 08:37:22 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 17 15:28:18 2018
Response via : Initial Calibration

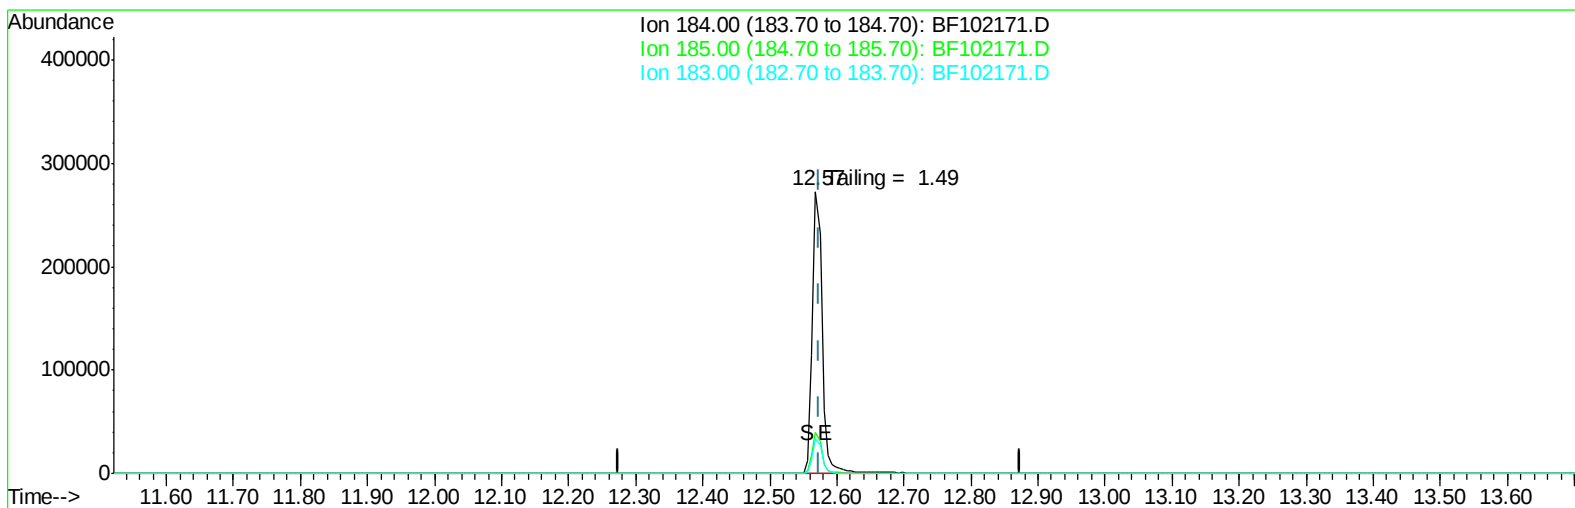

TIC: BF102171.D

(76) Benzidine



12.569min (-0.006) 0.00ng

response 265209

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.66
183.00	11.60	12.40
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF011718\
Data File : BF102171.D
Acq On : 18 Jan 2018 1:41
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 08:37:22 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 17 15:28:18 2018
Response via : Initial Calibration

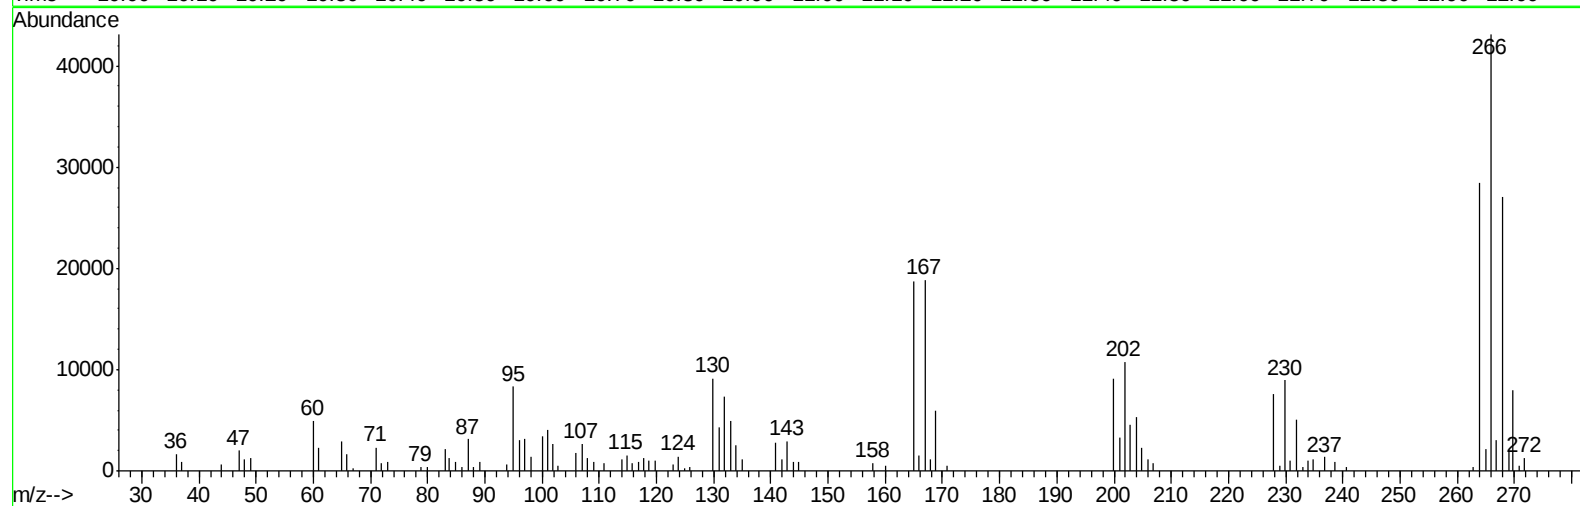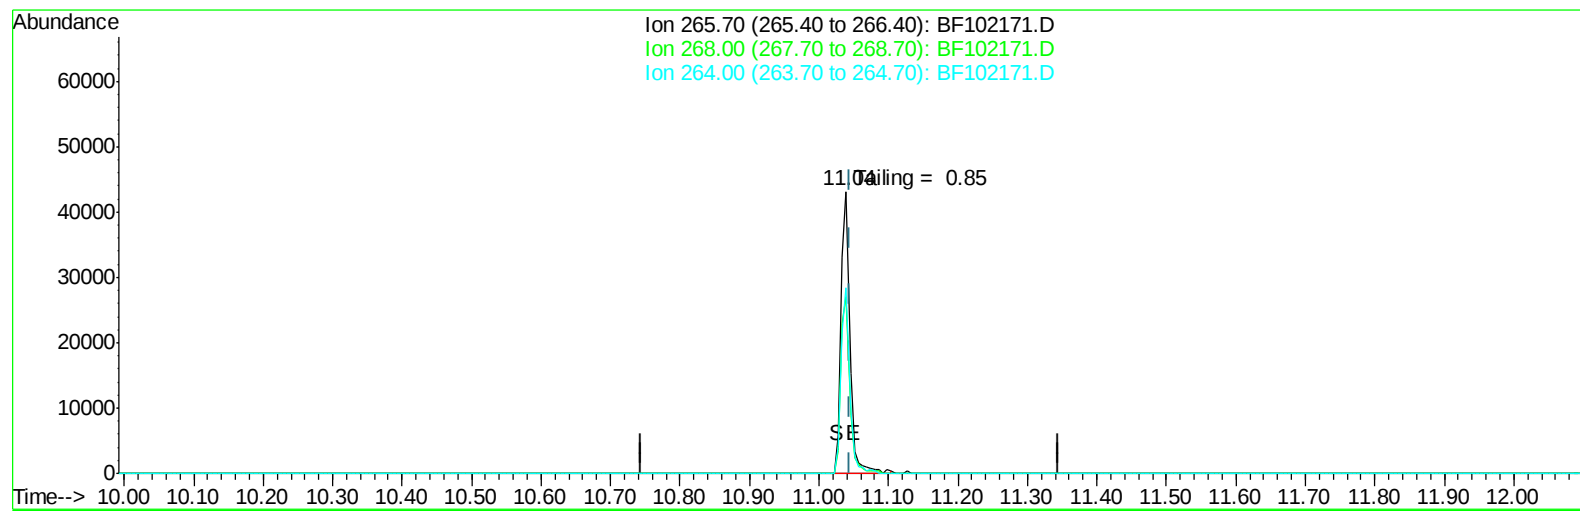

TIC: BF102171.D

(69) Pentachlorophenol (C)

11.039min (-0.006) 49901.54ng

response 37537

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.66
264.00	61.90	65.85
0.00	0.00	0.00