


Data Path : U:\HPCHEM1\BNA F\DATA\BF011718\
 Data File : BF102146.D
 Acq On : 17 Jan 2018 12:10
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF010918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 17 15:28:18 2018

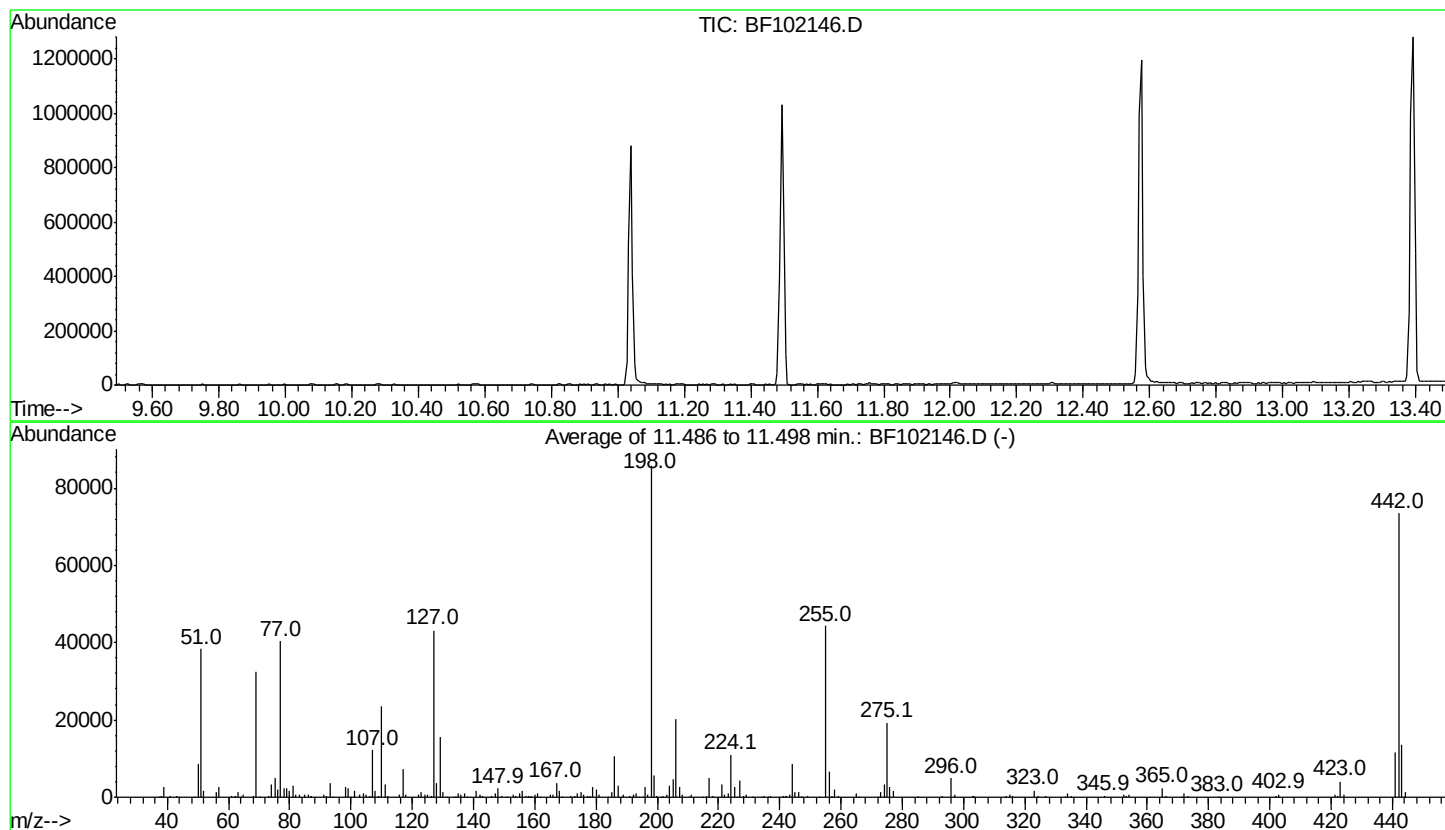

AutoFind: Scans 1598, 1599, 1600; Background Corrected with Scan 1594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.6	38296	PASS
68	69	0.00	2	1.5	501	PASS
69	198	0.00	100	38.0	32624	PASS
70	69	0.00	2	0.5	153	PASS
127	198	10	80	50.3	43125	PASS
197	198	0.00	2	0.9	766	PASS
198	198	100	100	100.0	85805	PASS
199	198	5	9	6.4	5497	PASS
275	198	10	60	22.6	19354	PASS
365	198	1	100	2.9	2453	PASS
441	443	0.01	100	85.1	11573	PASS
442	198	50	100	85.6	73472	PASS
443	442	15	24	18.5	13599	PASS