


Data Path : U:\HPCHEM1\BNA F\DATA\BF011718\
 Data File : BF102171.D
 Acq On : 18 Jan 2018 1:41
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF010918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 17 15:28:18 2018

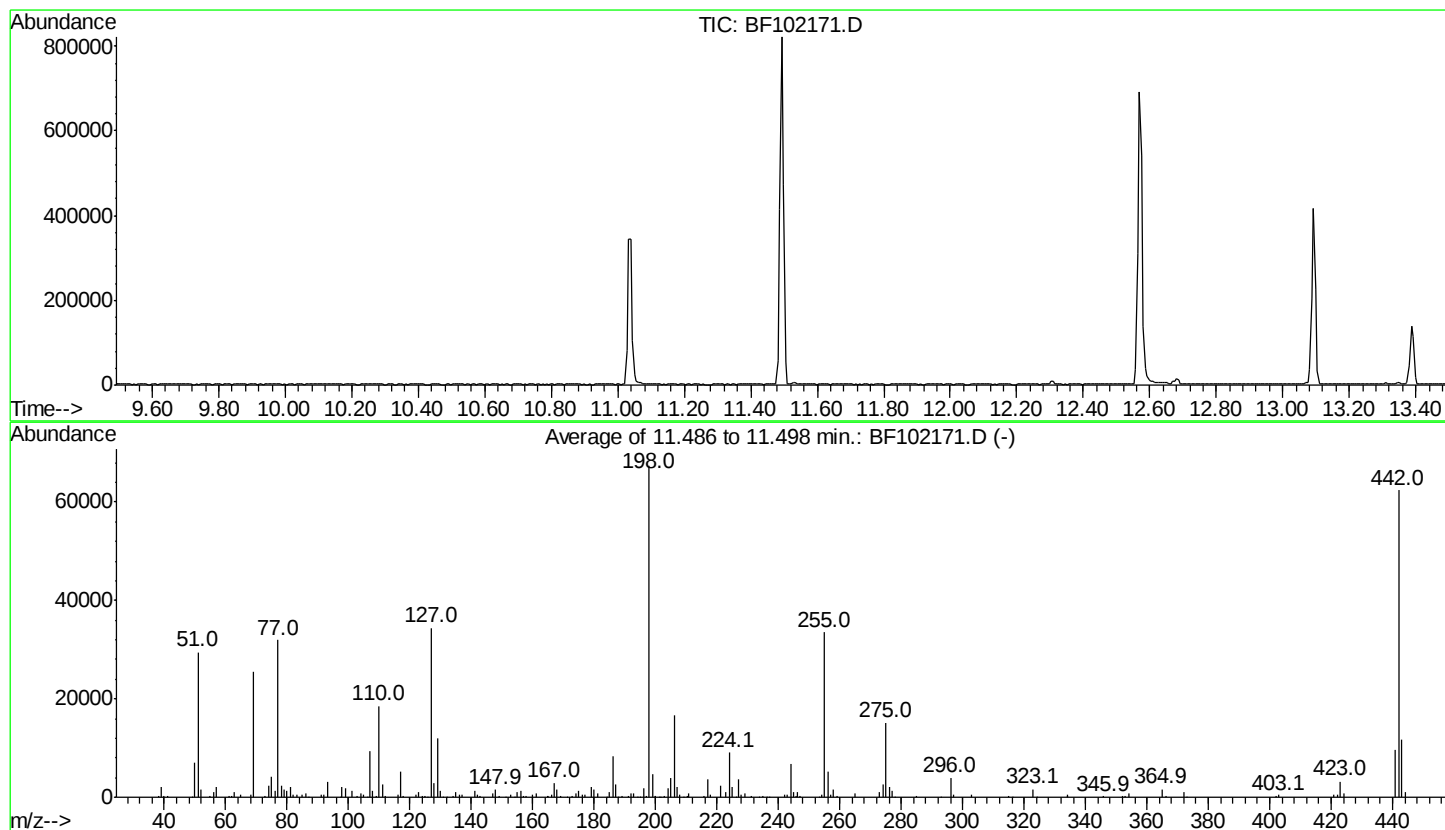

AutoFind: Scans 1598, 1599, 1600; Background Corrected with Scan 1594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.6	29400	PASS
68	69	0.00	2	1.7	428	PASS
69	198	0.00	100	37.8	25458	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.0	34349	PASS
197	198	0.00	2	0.5	351	PASS
198	198	100	100	100.0	67394	PASS
199	198	5	9	7.0	4707	PASS
275	198	10	60	22.4	15123	PASS
365	198	1	100	2.4	1588	PASS
441	443	0.01	100	81.3	9602	PASS
442	198	50	100	92.6	62400	PASS
443	442	15	24	18.9	11816	PASS