
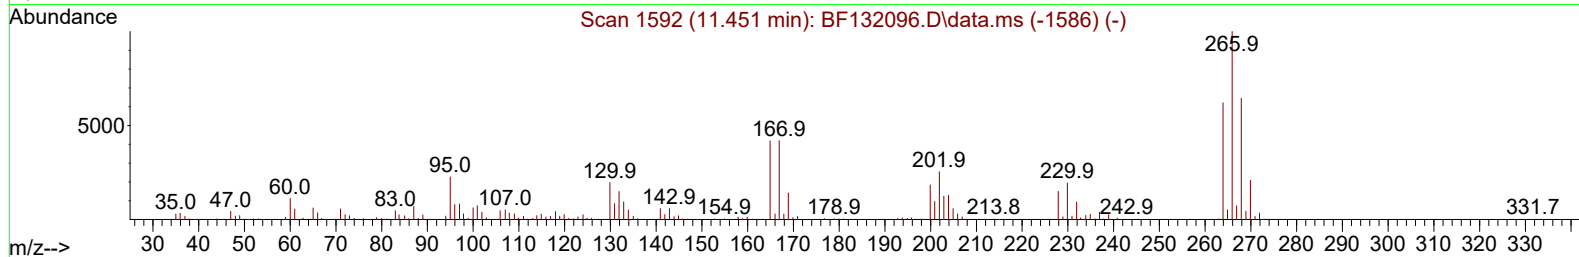
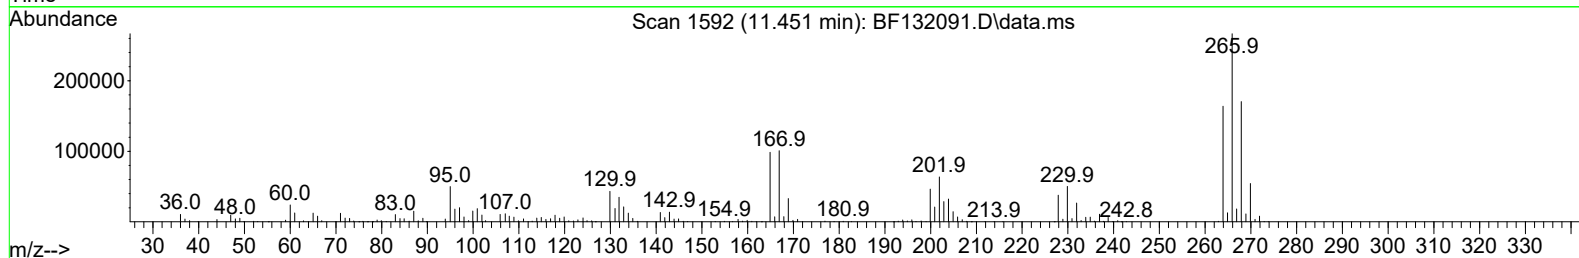


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011723\
Data File : BF132091.D
Acq On : 17 Jan 2023 12:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 07:26:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 18 00:47:03 2023
Response via : Initial Calibration

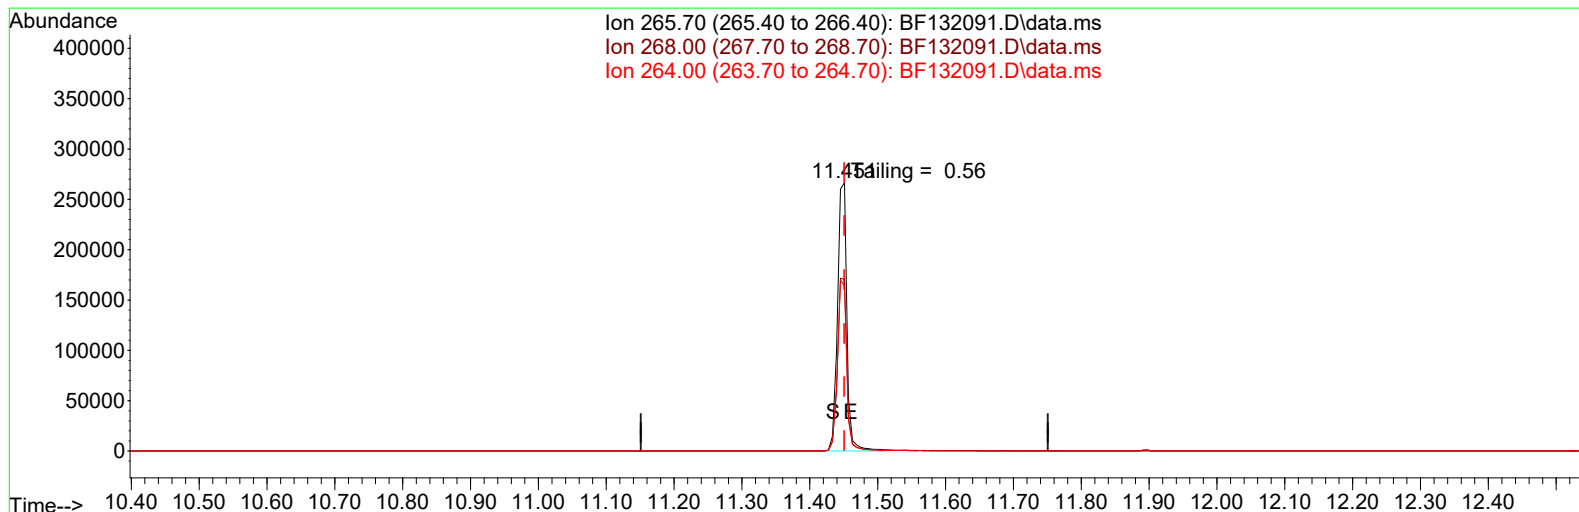

TIC: BF132091.D\data.ms

(70) Pentachlorophenol (C)




11.451min (+ 0.000) 604632.91 ng

response 256470

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.97
264.00	62.10	61.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011723\
Data File : BF132091.D
Acq On : 17 Jan 2023 12:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 07:26:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 18 00:47:03 2023
Response via : Initial Calibration

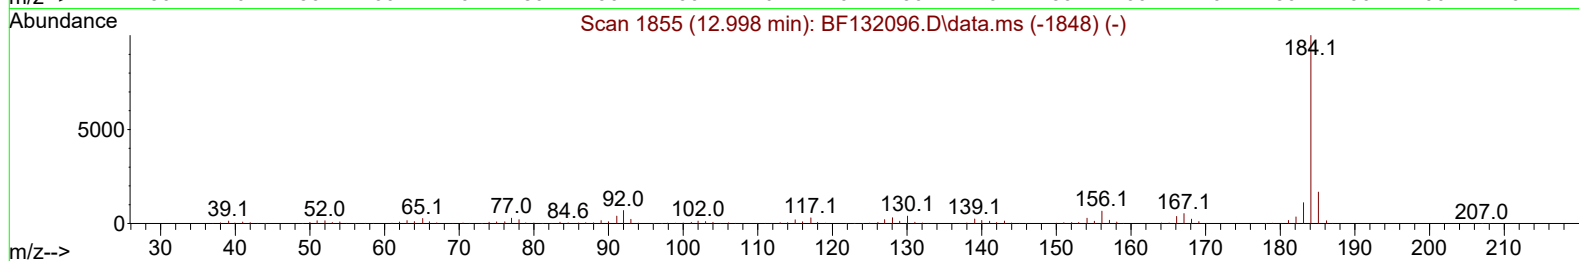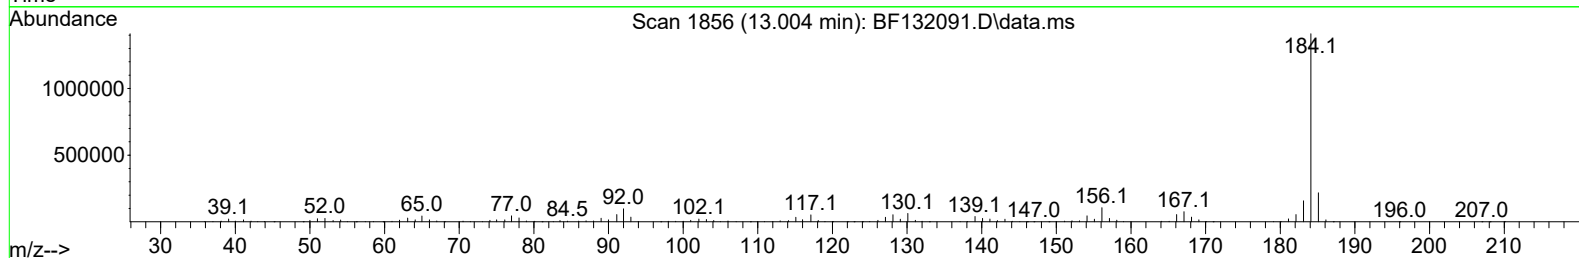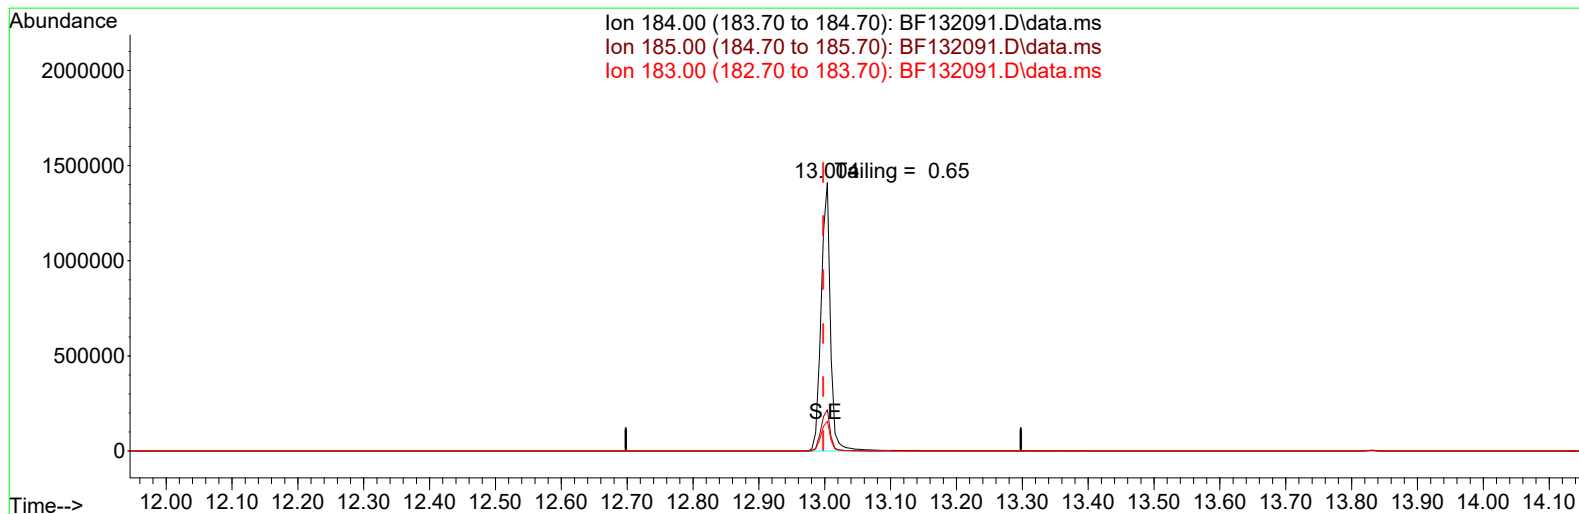

TIC: BF132091.D\data.ms

(77) Benzidine

13.004min (+ 0.006) 0.00 ng

response 1387867

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.60	15.40
183.00	11.10	11.13
0.00	0.00	0.00