

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011723\
 Data File : BF132102.D
 Acq On : 17 Jan 2023 19:37
 Operator : CG\JU
 Sample : PB150088BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB150088BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011723.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF132102.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.366	423	430	439	rVB	1892093	2659118	36.07%	5.588%
2	5.737	487	493	496	rBV	4678272	5418575	73.51%	11.386%
3	6.713	652	659	662	rBV	4197235	5602110	76.00%	11.772%
4	7.095	720	724	728	rBV	1767784	1453602	19.72%	3.055%
5	7.660	813	820	823	rBV	3309625	3782180	51.31%	7.948%
6	8.383	937	943	946	rBV	2226319	1924266	26.10%	4.044%
7	9.466	1120	1127	1130	rBV	6369264	6360572	86.29%	13.366%
8	10.148	1237	1243	1247	rBV	2555913	2291685	31.09%	4.816%
9	10.948	1371	1379	1382	rBV	4630549	4713236	63.94%	9.904%
10	11.648	1494	1498	1502	rBV	2713648	2557270	34.69%	5.374%
11	13.254	1765	1771	1774	rBV	6800138	7371494	100.00%	15.490%
12	14.313	1947	1951	1955	rBV	2237097	2004397	27.19%	4.212%
13	15.918	2218	2224	2236	rBV	1035247	1449413	19.66%	3.046%




Sum of corrected areas: 47587918

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011723\
Data File : BF132102.D
Acq On : 17 Jan 2023 19:37
Operator : CG\JU
Sample : PB150088BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB150088BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

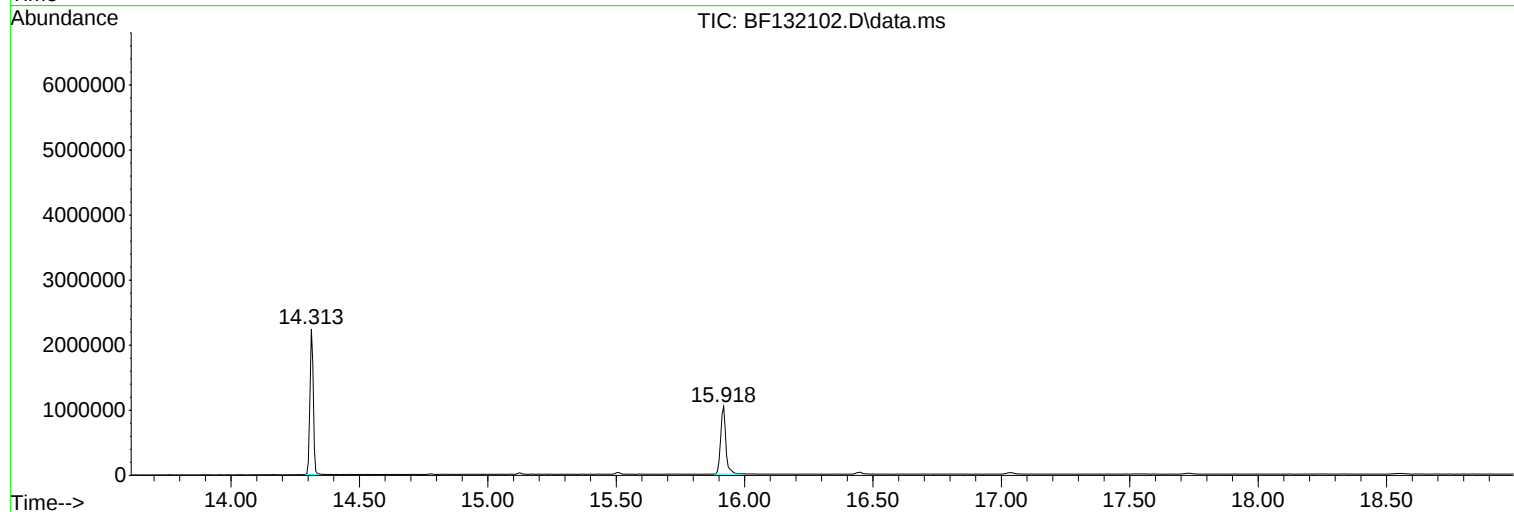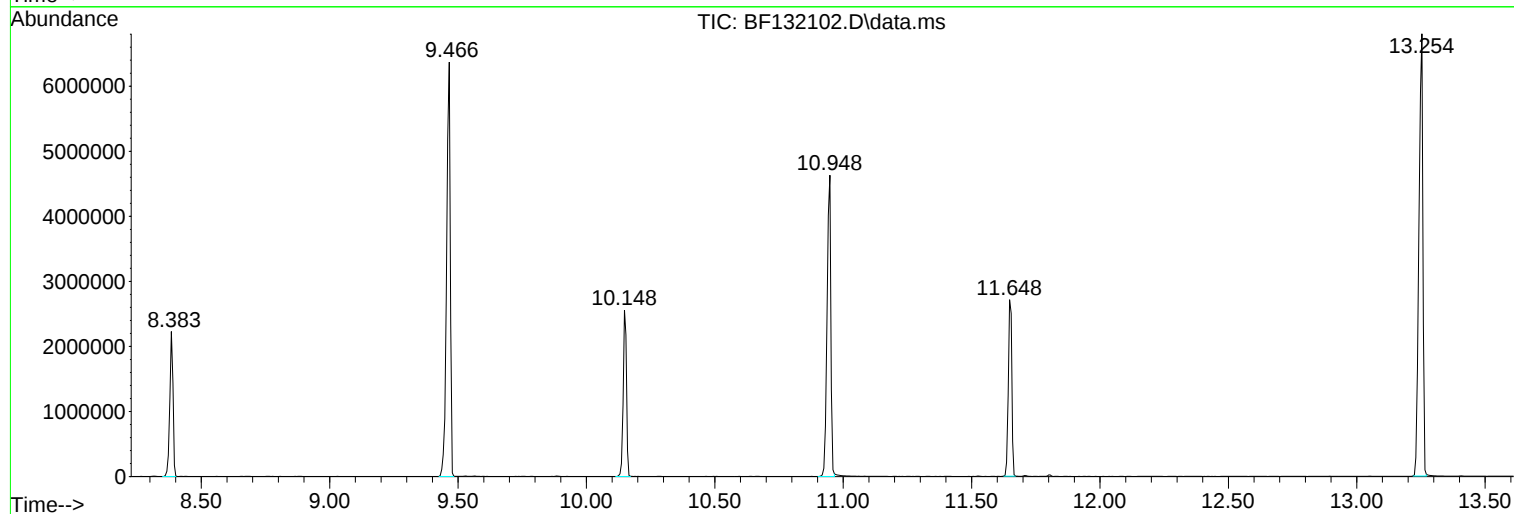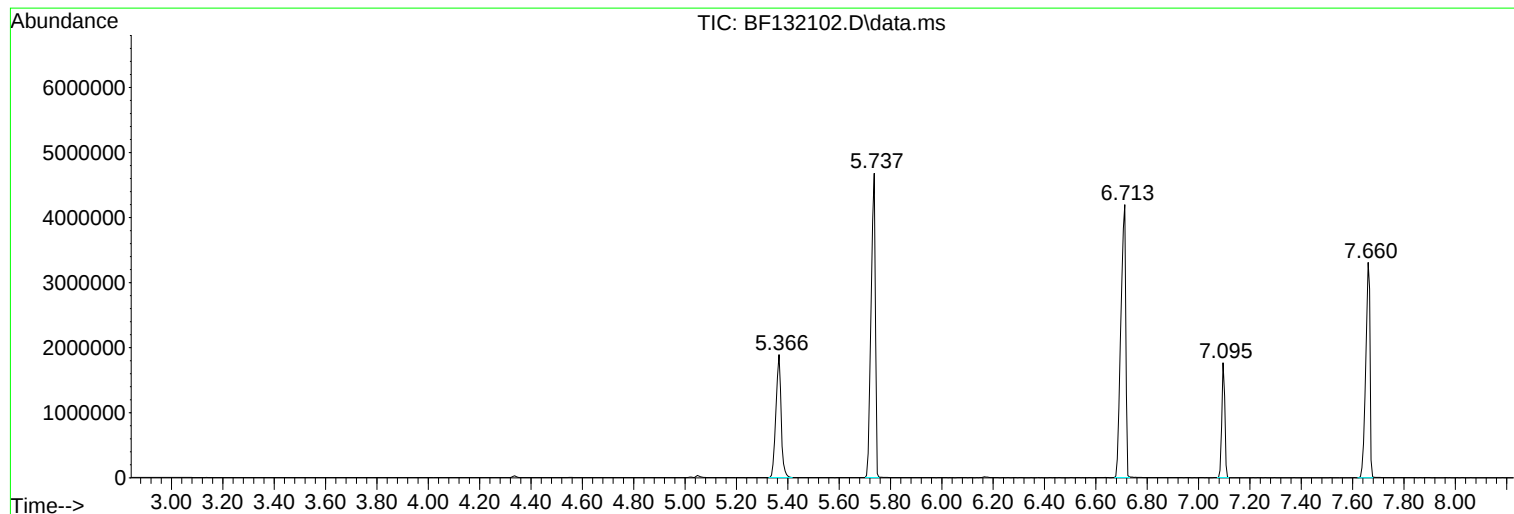

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011723\
Data File : BF132102.D
Acq On : 17 Jan 2023 19:37
Operator : CG\JU
Sample : PB150088BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB150088BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.366	36.59 ng	2659120	1,4-Dichlorobenzene-d4	7.095

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	59		
2	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	27		
3	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	12		
4	Acetone	58	C3H6O	000067-64-1	12		
5	Butane	58	C4H10	000106-97-8	9		

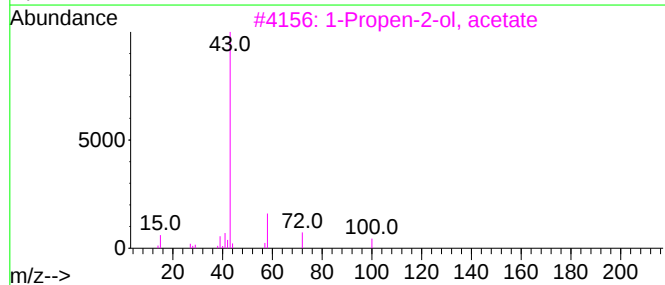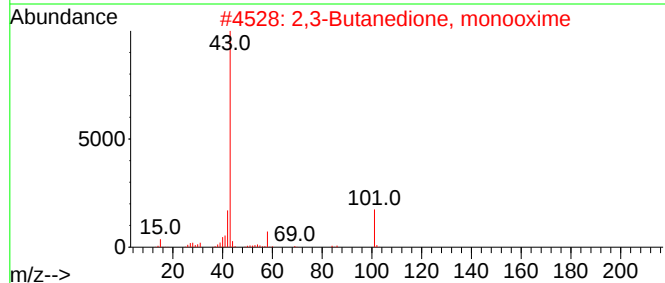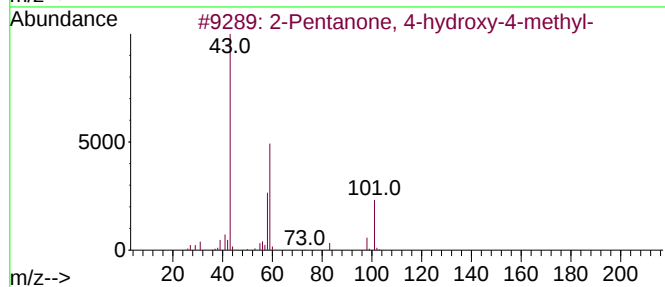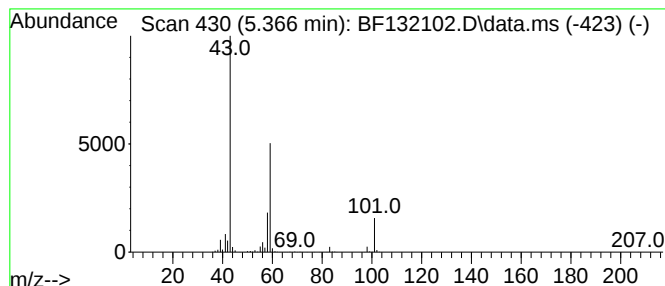

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011723\
Data File : BF132102.D
Acq On : 17 Jan 2023 19:37
Operator : CG\JU
Sample : PB150088BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB150088BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.366	36.6	ng	2659120	1	7.095	1453600	20.0