
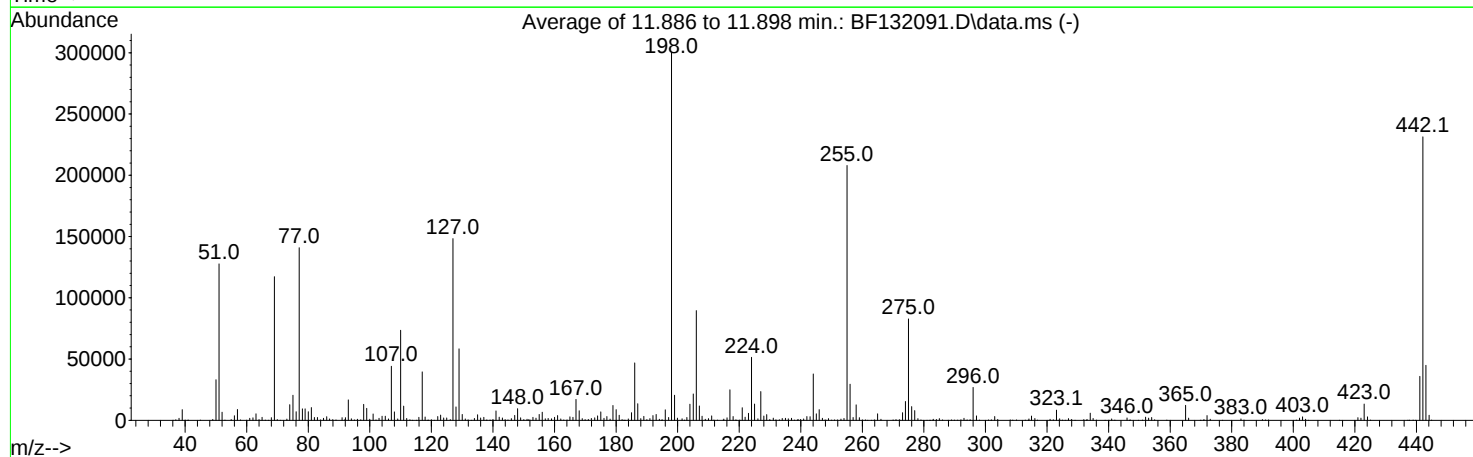


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011723\
 Data File : BF132091.D
 Acq On : 17 Jan 2023 12:28
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011723.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 18 00:47:03 2023

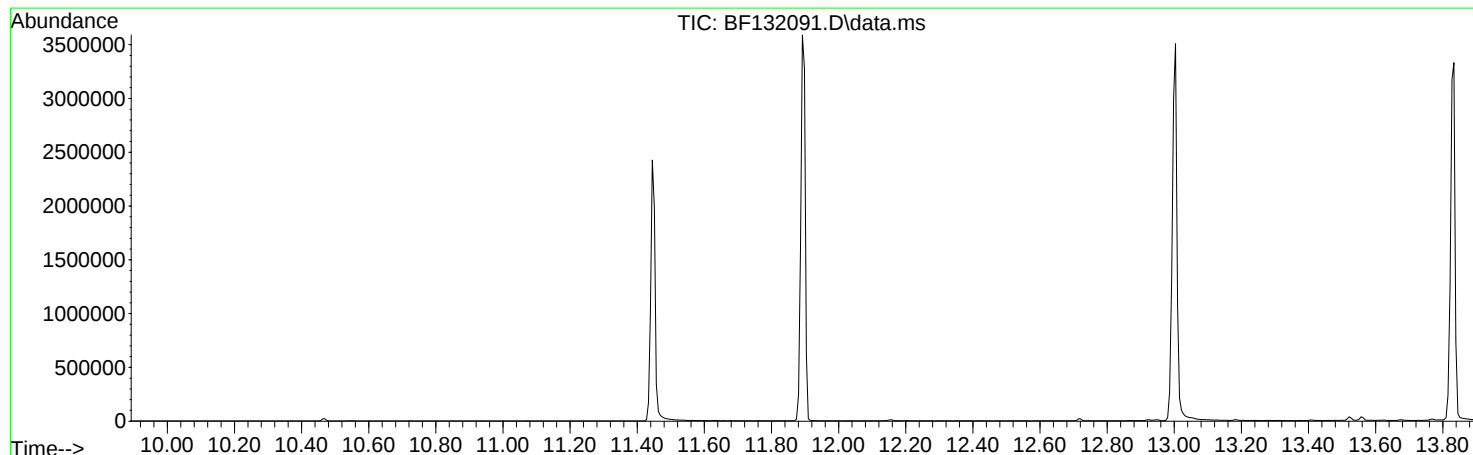




AutoFind: Scans 1666, 1667, 1668; Background Corrected with Scan 1661

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.5	127699	PASS
68	69	0.00	2	1.9	2202	PASS
69	198	0.00	100	39.1	117288	PASS
70	69	0.00	2	0.5	627	PASS
127	198	10	80	49.4	148296	PASS
197	198	0.00	2	0.8	2333	PASS
198	198	100	100	100.0	300288	PASS
199	198	5	9	6.8	20388	PASS
275	198	10	60	27.5	82709	PASS
365	198	1	100	4.1	12190	PASS
441	198	0.01	100	11.9	35844	PASS
442	442	50	100	100.0	231411	PASS
443	442	15	24	19.4	44924	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011723\
Data File : BF132091.D
Acq On : 17 Jan 2023 12:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 18 07:26:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 18 00:47:03 2023
Response via : Initial Calibration

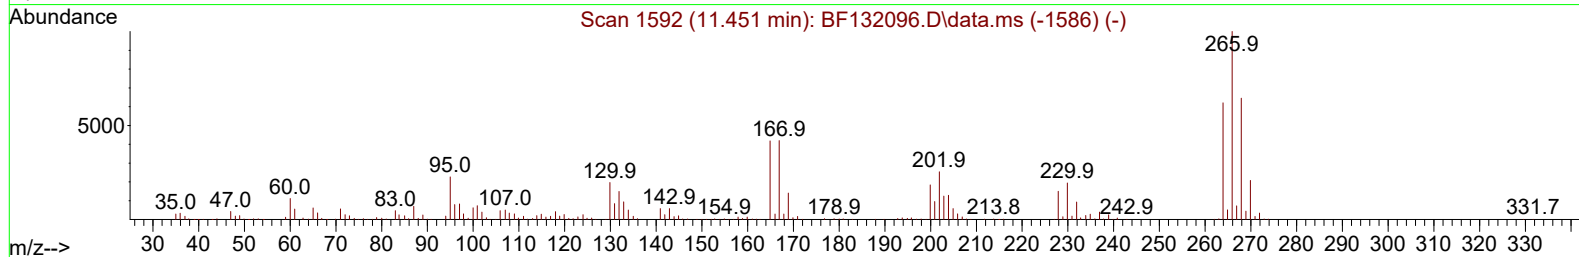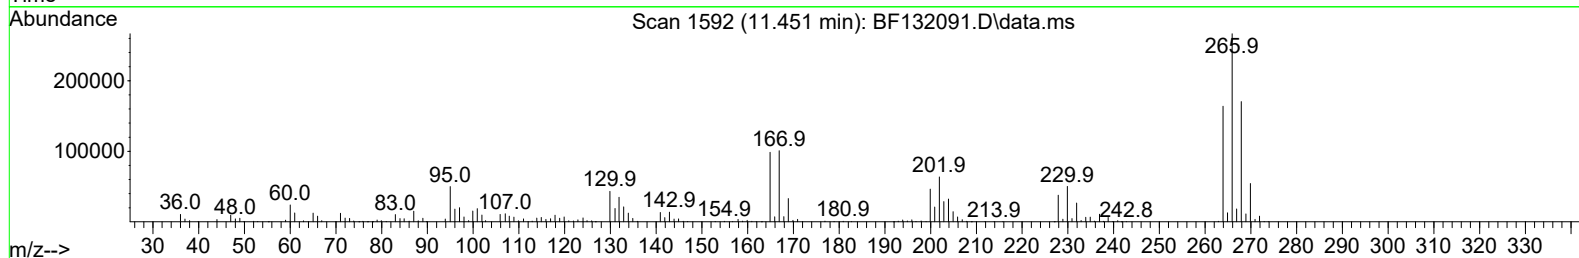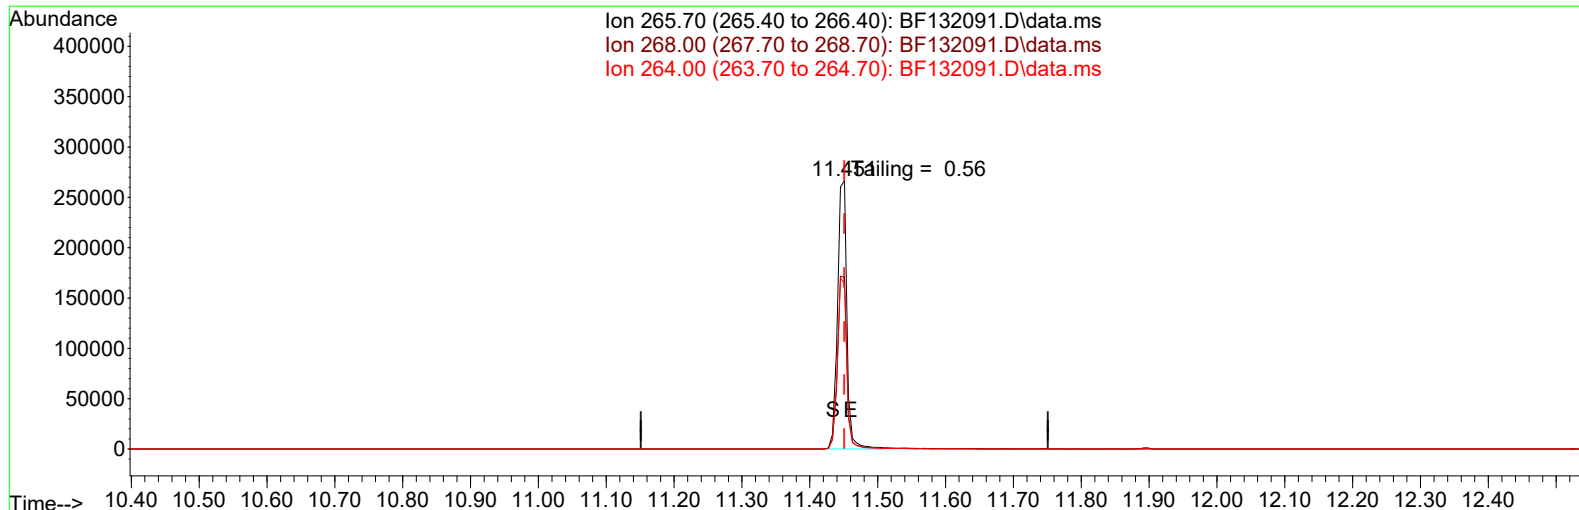

TIC: BF132091.D\data.ms

(70) Pentachlorophenol (C)

11.451min (+ 0.000) 604632.91 ng




response 256470

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.97
264.00	62.10	61.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011723\
Data File : BF132091.D
Acq On : 17 Jan 2023 12:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 18 07:26:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 18 00:47:03 2023
Response via : Initial Calibration

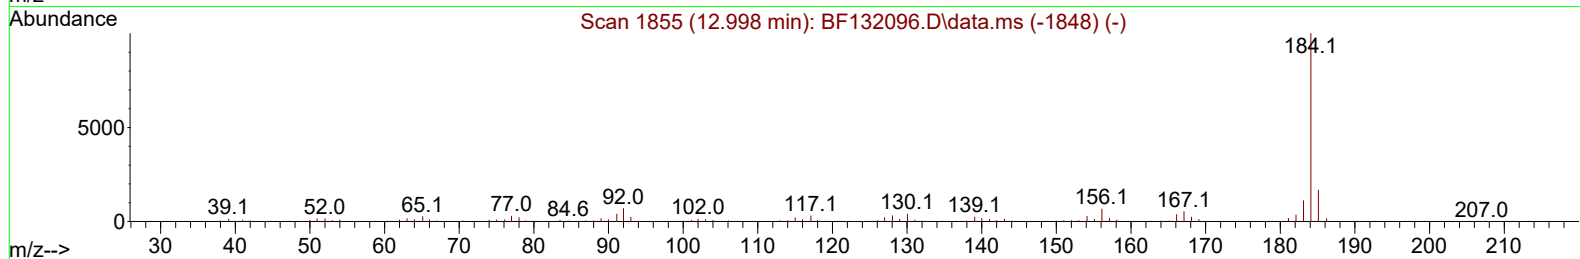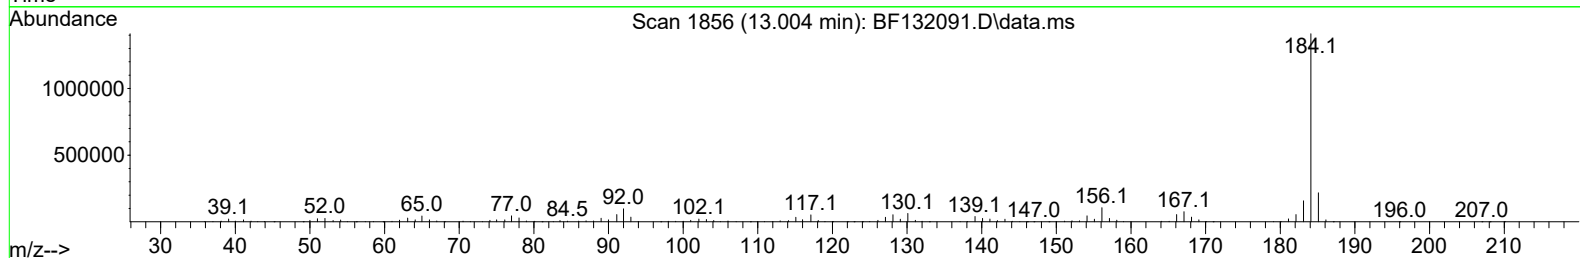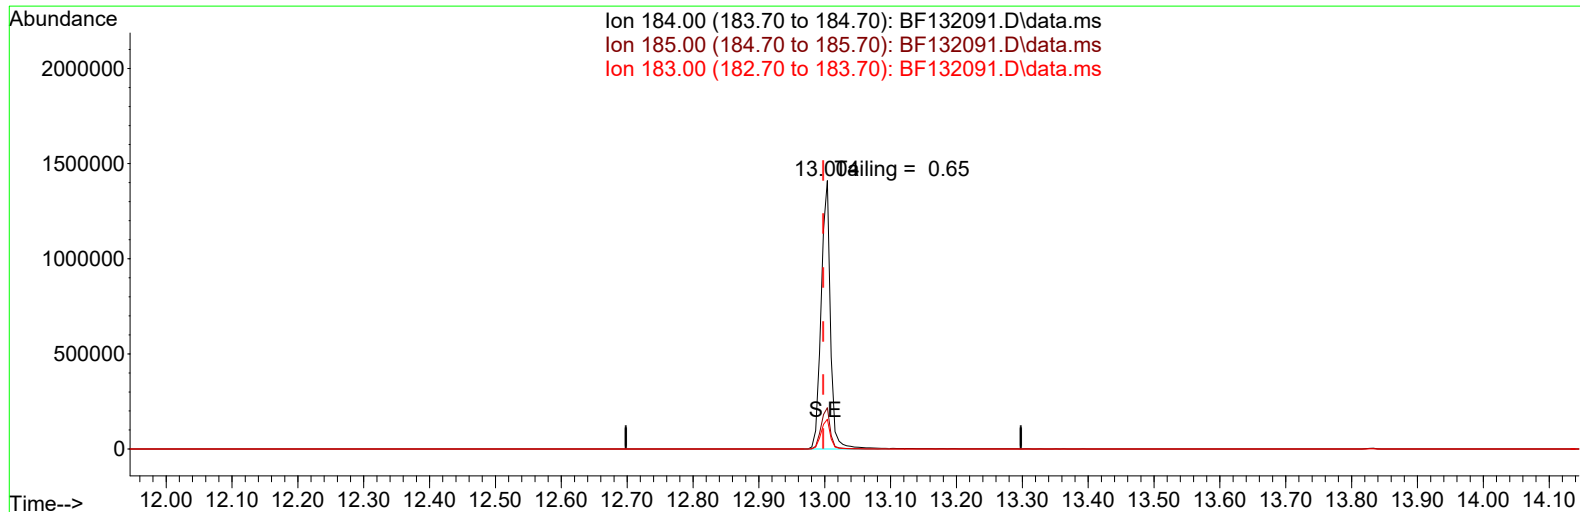

TIC: BF132091.D\data.ms

(77) Benzidine

13.004min (+ 0.006) 0.00 ng

response 1387867

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.60	15.40
183.00	11.10	11.13
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/17/2023	BNA_F	<u>BF132091.D</u>
Compound Name	Response	Retention Time
DDT	496076	13.833
DDD	8479	13.521
DDE	80	12.922
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8559	504635	1.70

Instrument :
BNA_F
ClientSampleId :
DFTPP