
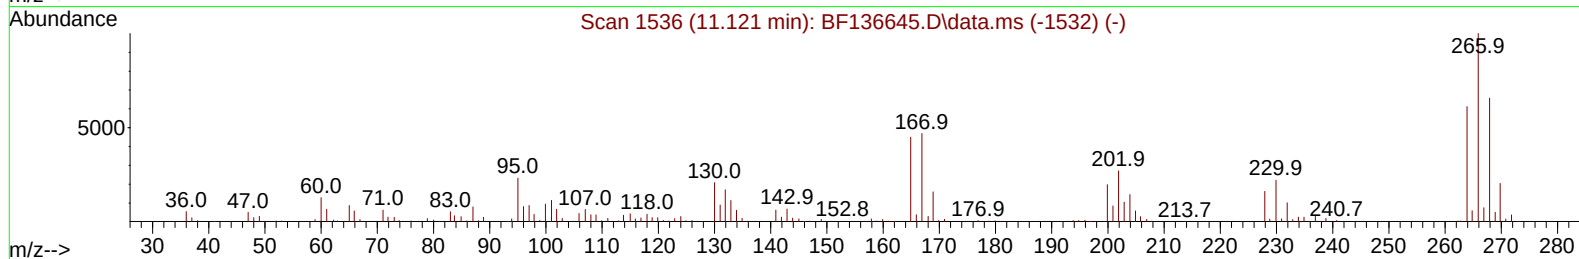
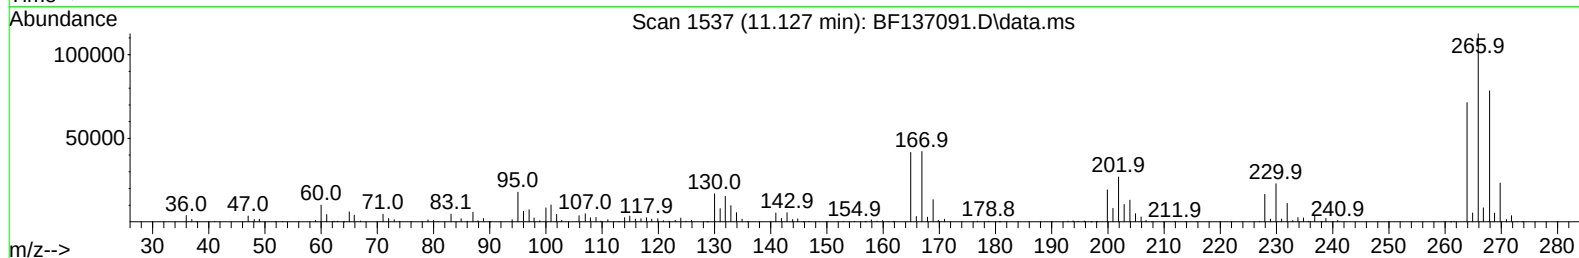


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011724\
Data File : BF137091.D
Acq On : 17 Jan 2024 13:33
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 17 14:04:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

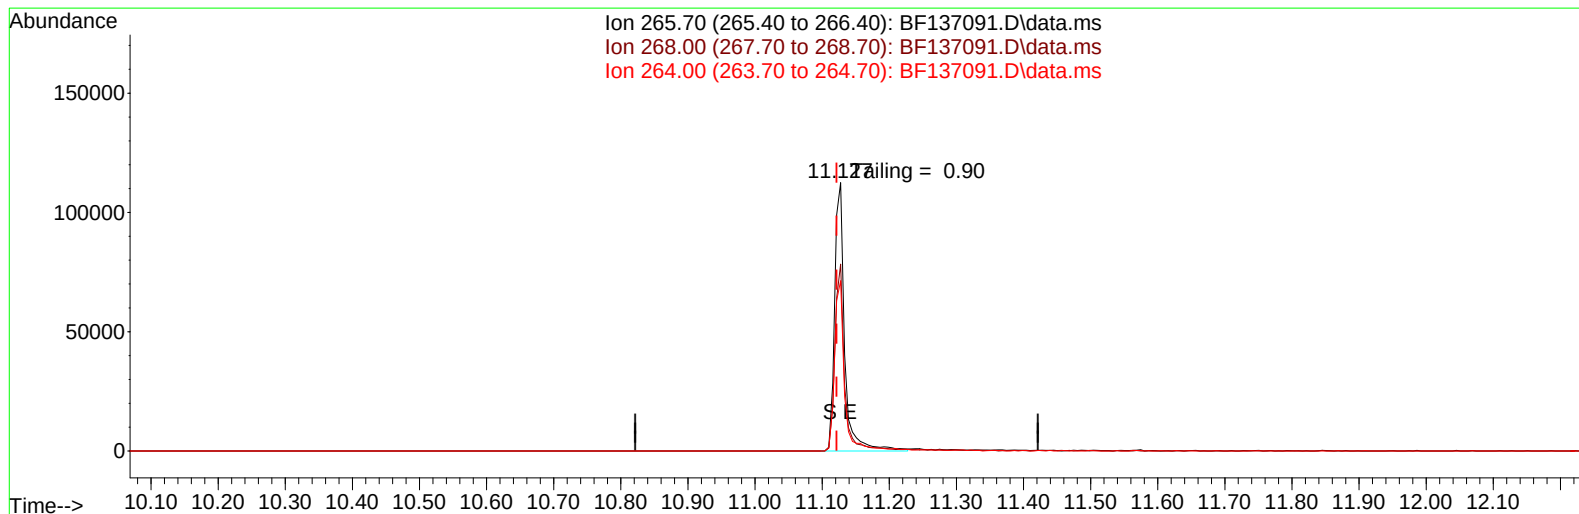

TIC: BF137091.D\data.ms

(70) Pentachlorophenol (C)




11.127min (+ 0.006) 35261.41 ng m

response 117167

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	69.66
264.00	61.20	63.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011724\
Data File : BF137091.D
Acq On : 17 Jan 2024 13:33
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 17 14:04:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

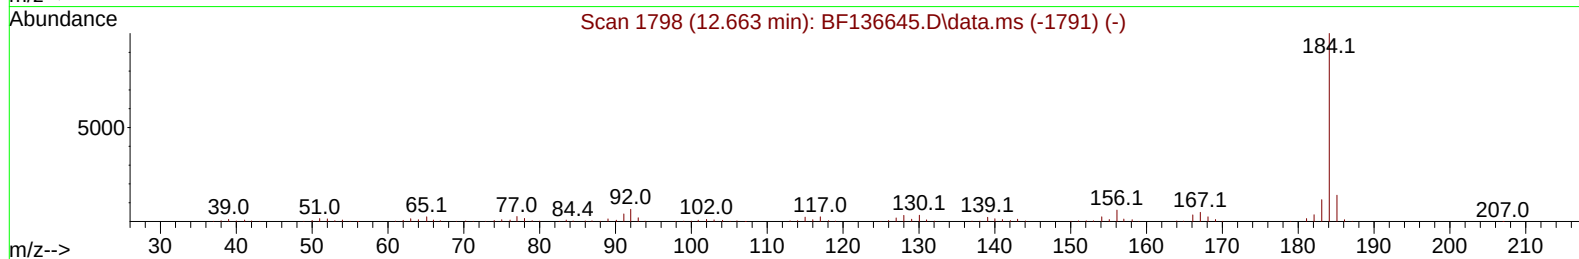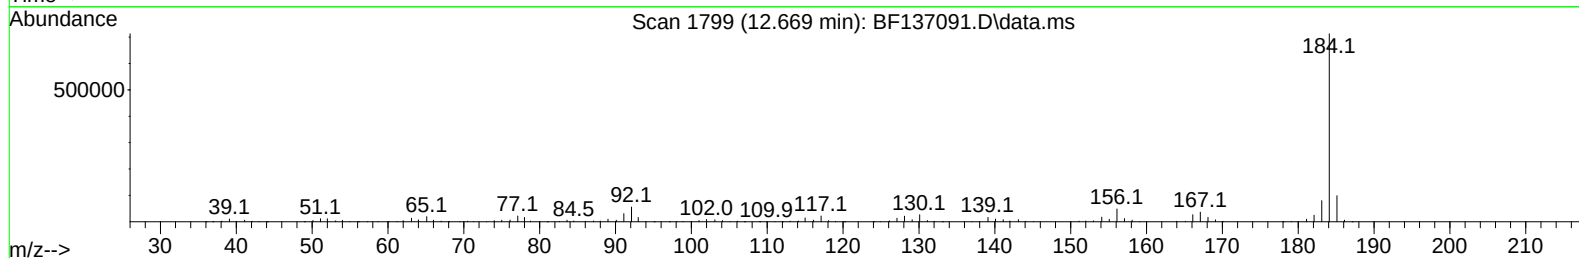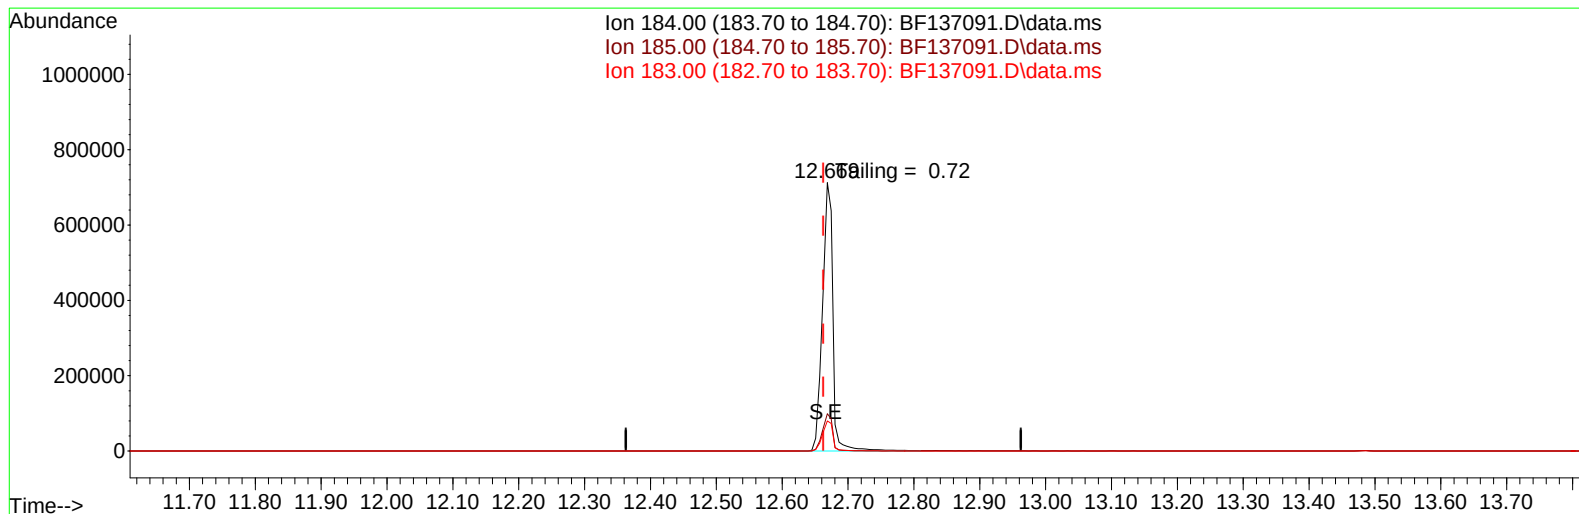

TIC: BF137091.D\data.ms

(77) Benzidine

12.669min (+ 0.006) 0.00 ng m

response 783443

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.89
183.00	11.60	11.26
0.00	0.00	0.00