
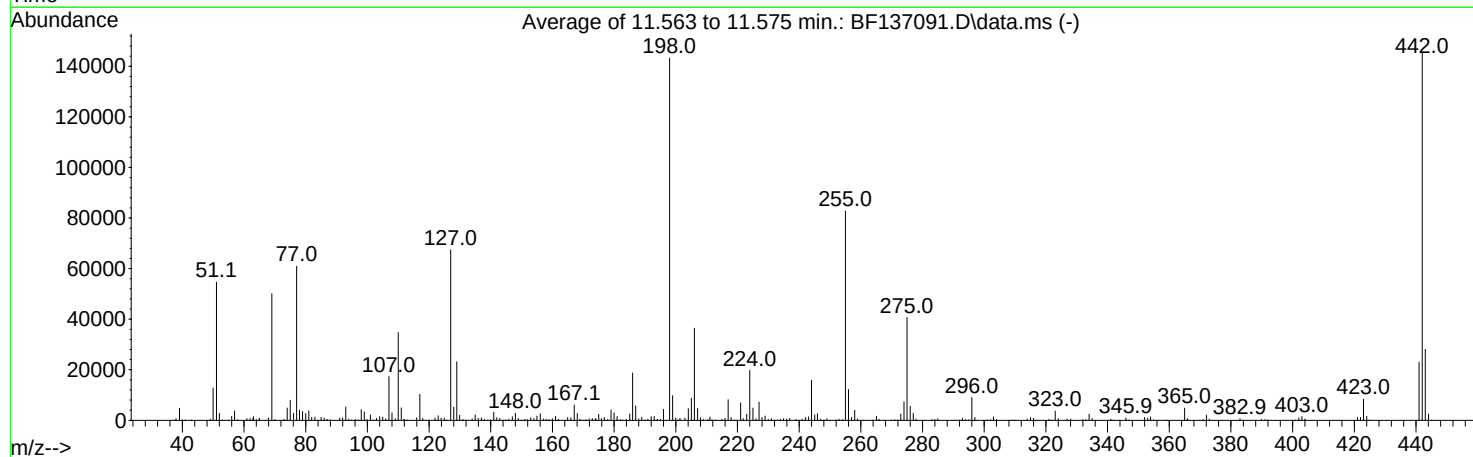


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011724\
Data File : BF137091.D
Acq On : 17 Jan 2024 13:33
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 21 01:54:25 2023

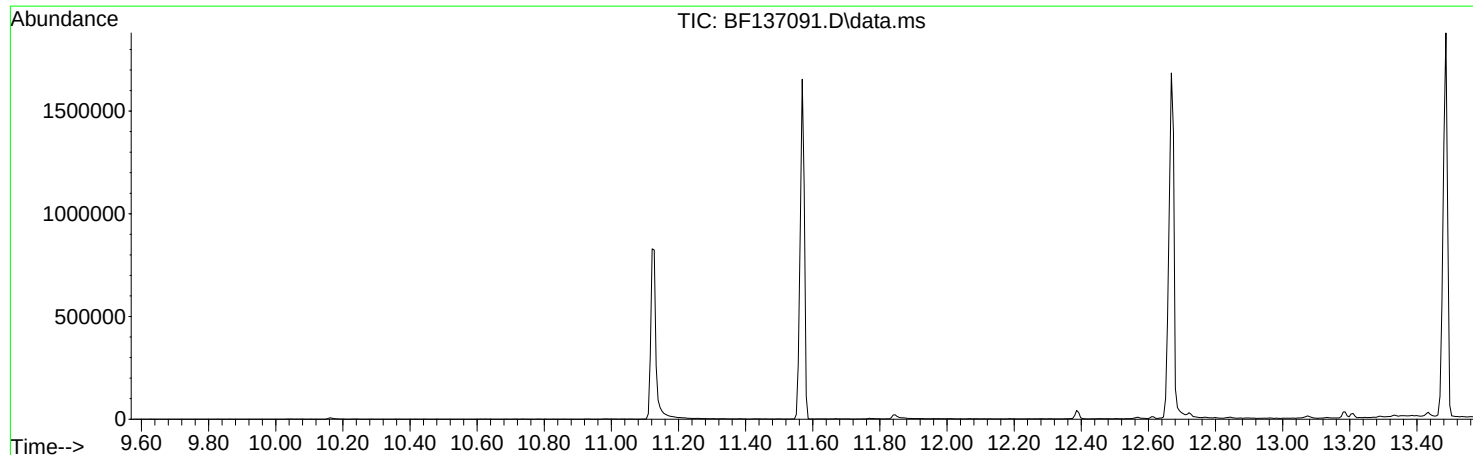




AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.2	54667	PASS
68	69	0.00	2	1.7	856	PASS
69	198	0.00	100	35.0	50093	PASS
70	69	0.00	2	0.6	303	PASS
127	198	10	80	47.1	67427	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	143267	PASS
199	198	5	9	6.8	9692	PASS
275	198	10	60	28.4	40685	PASS
365	198	1	100	3.3	4773	PASS
441	198	0.01	100	16.0	22976	PASS
442	442	50	100	100.0	145499	PASS
443	442	15	24	19.3	28062	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011724\
Data File : BF137091.D
Acq On : 17 Jan 2024 13:33
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 17 14:04:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

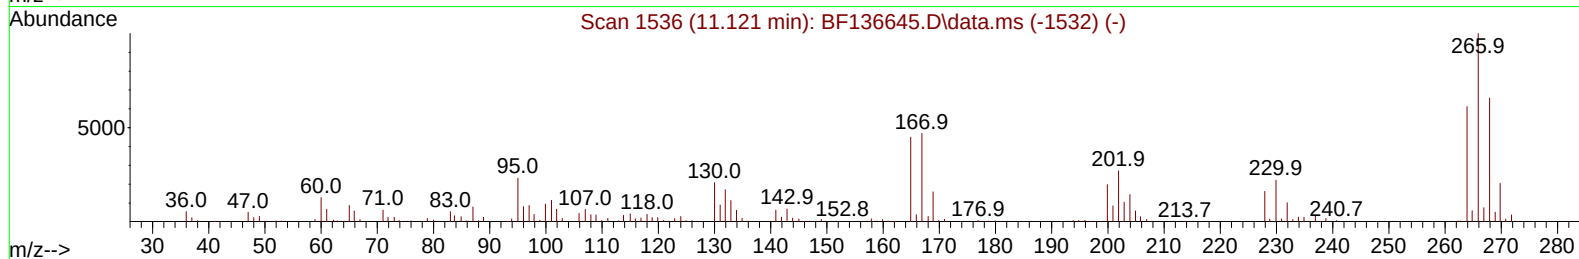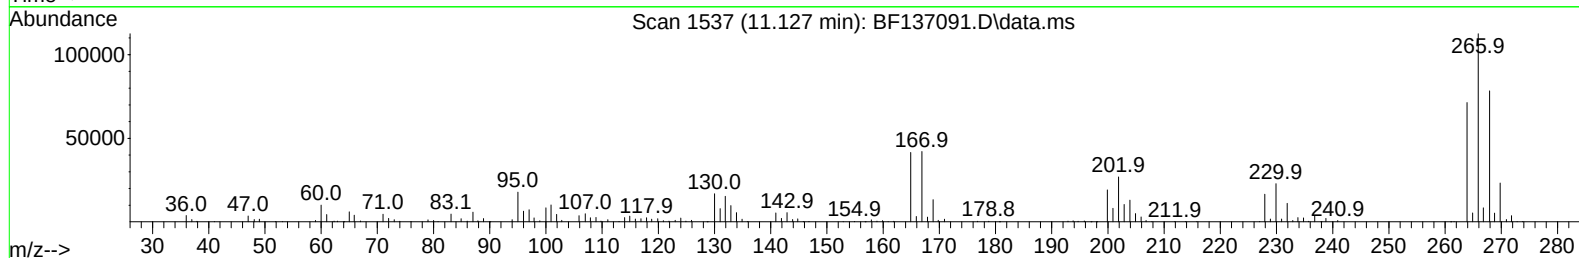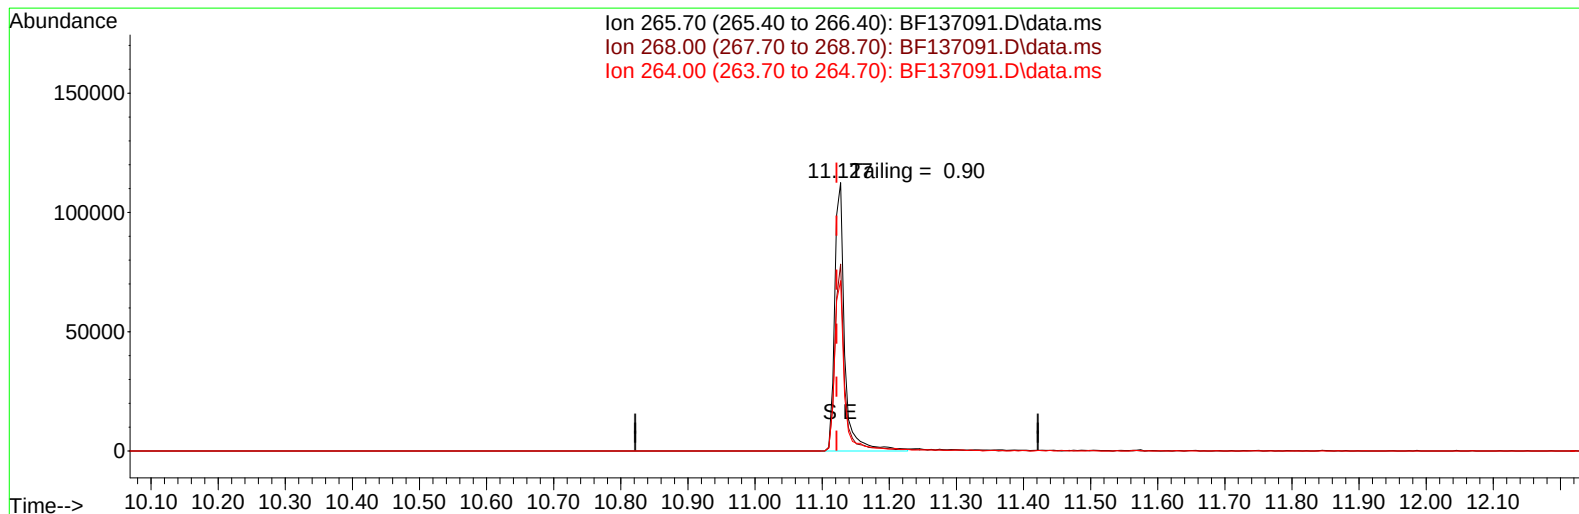

TIC: BF137091.D\data.ms

(70) Pentachlorophenol (C)

11.127min (+ 0.006) 35261.41 ng m




response 117167

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	69.66
264.00	61.20	63.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011724\
Data File : BF137091.D
Acq On : 17 Jan 2024 13:33
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 17 14:04:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

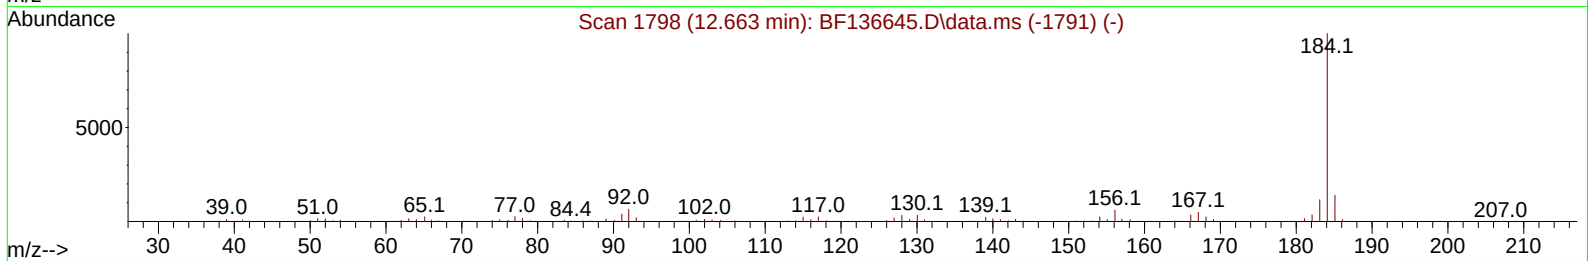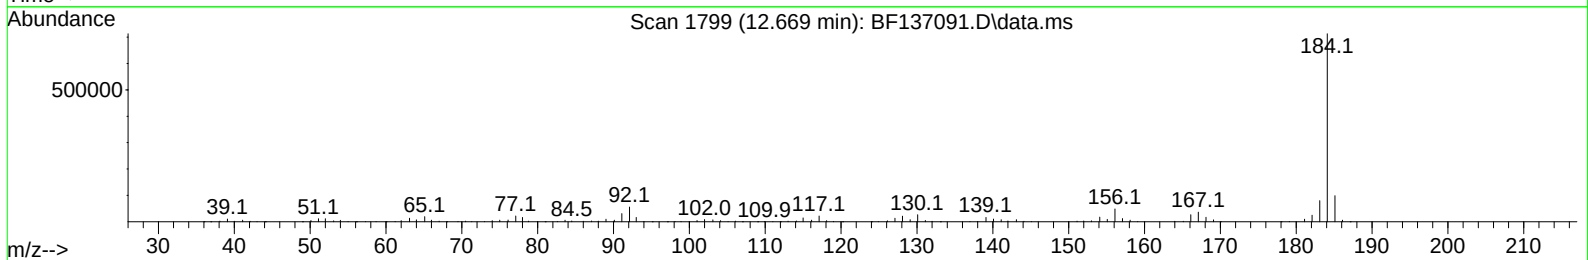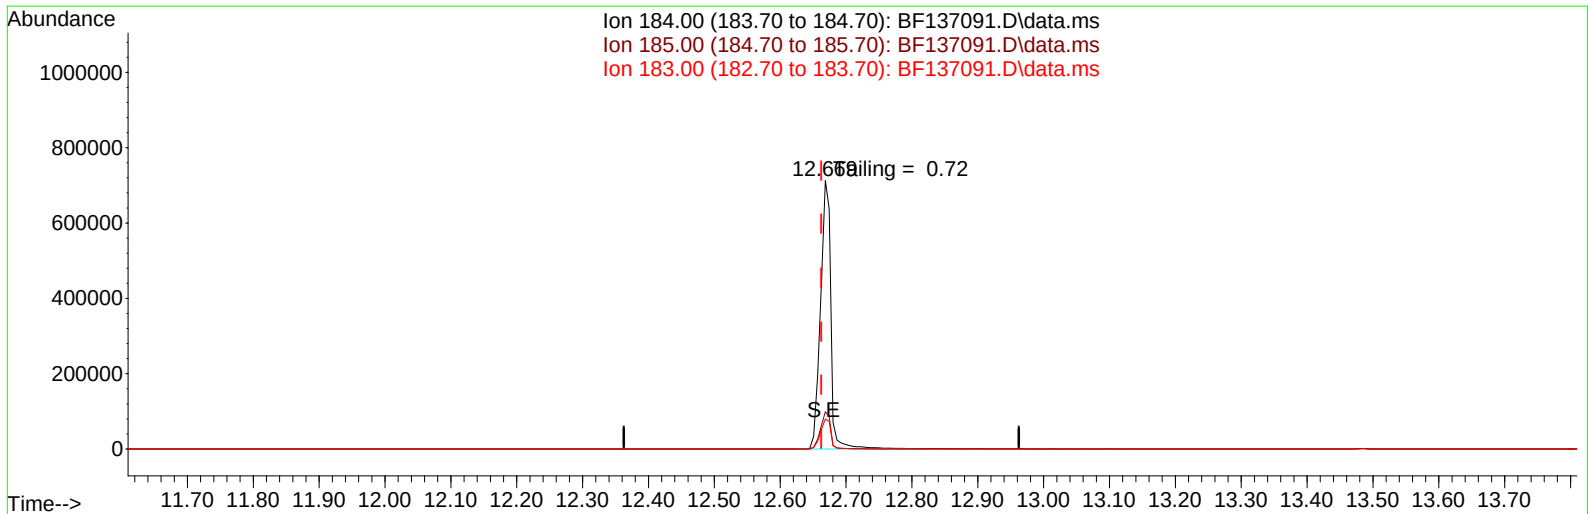

TIC: BF137091.D\data.ms

(77) Benzidine

12.669min (+ 0.006) 0.00 ng m

response 783443

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.89
183.00	11.60	11.26
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/17/2024	BNA_F	<u>BF137091.D</u>
Compound Name	Response	Retention Time
DDT	362416	13.486
DDD	11502	13.186
DDE	765	12.839
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12267	374683	3.27

Instrument :
BNA_F
ClientSampleId :
DFTPP