
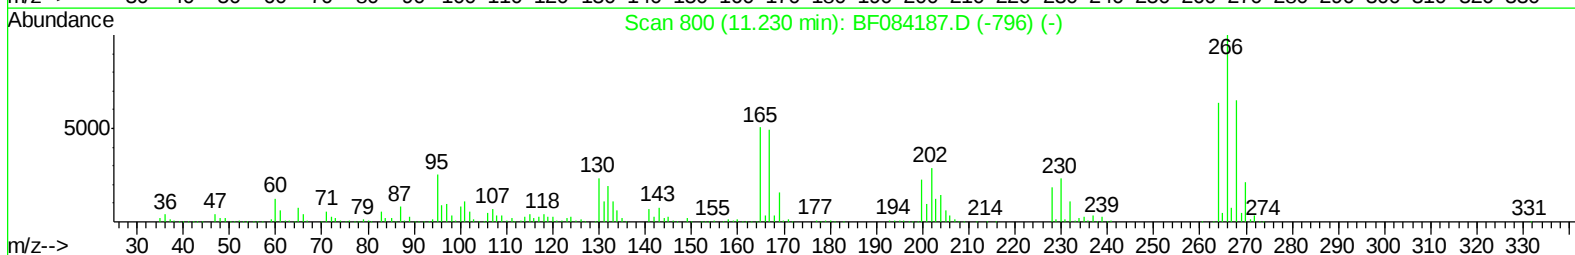
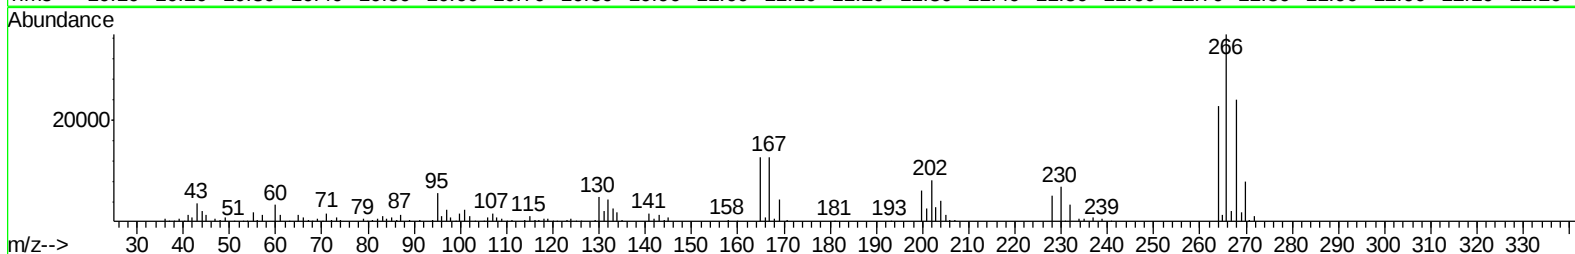


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011816\
Data File : BF084537.D
Acq On : 18 Jan 2016 10:10
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 19 04:55:20 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 14 14:15:52 2016
Response via : Initial Calibration

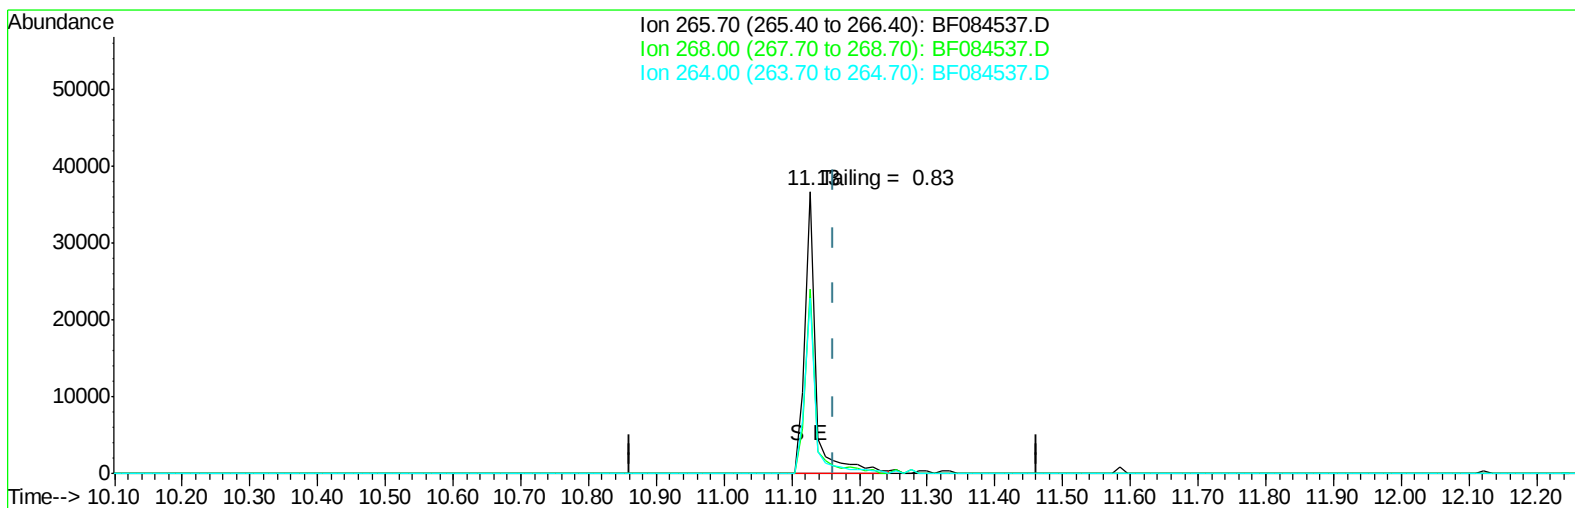

TIC: BF084537.D

(69) Pentachlorophenol (C)




11.128min (-0.034) 2712.61ng

response 42325

Ion	Exp%	Act%
265.70	100	100
268.00	65.50	65.29
264.00	62.70	62.30
0.00	0.00	0.00

```
Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011816\  
Data File : BF084537.D  
Acq On    : 18 Jan 2016   10:10  
Operator  : SJ/UM  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: Jan 19 04:55:20 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 14 14:15:52 2016
Response via : Initial Calibration

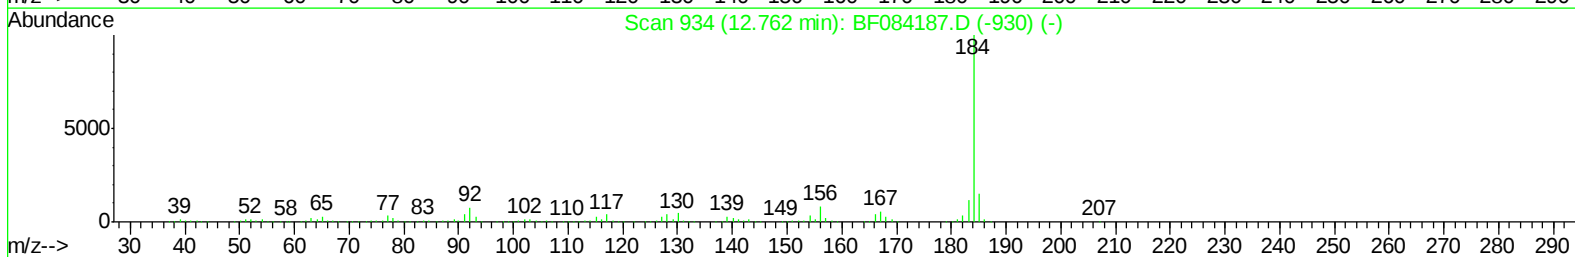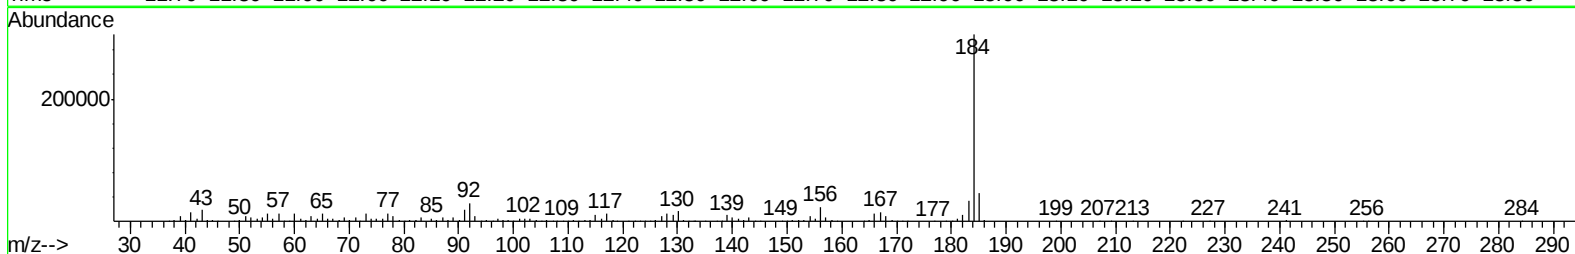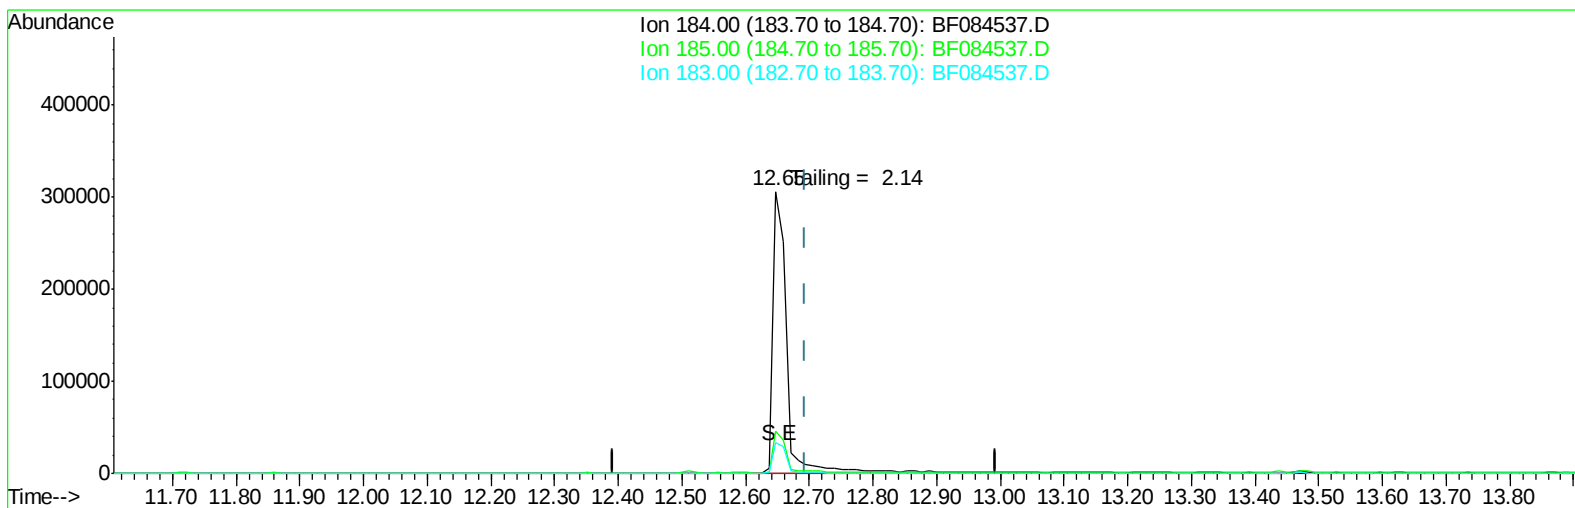

TIC: BF084537.D

(76) Benzidine

12.648min (-0.046) 3209.57ng

response 464345

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	15.20
183.00	12.30	10.96
0.00	0.00	0.00