


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011816\
 Data File : BF084537.D
 Acq On : 18 Jan 2016 10:10
 Operator : SJ/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 14 14:15:52 2016

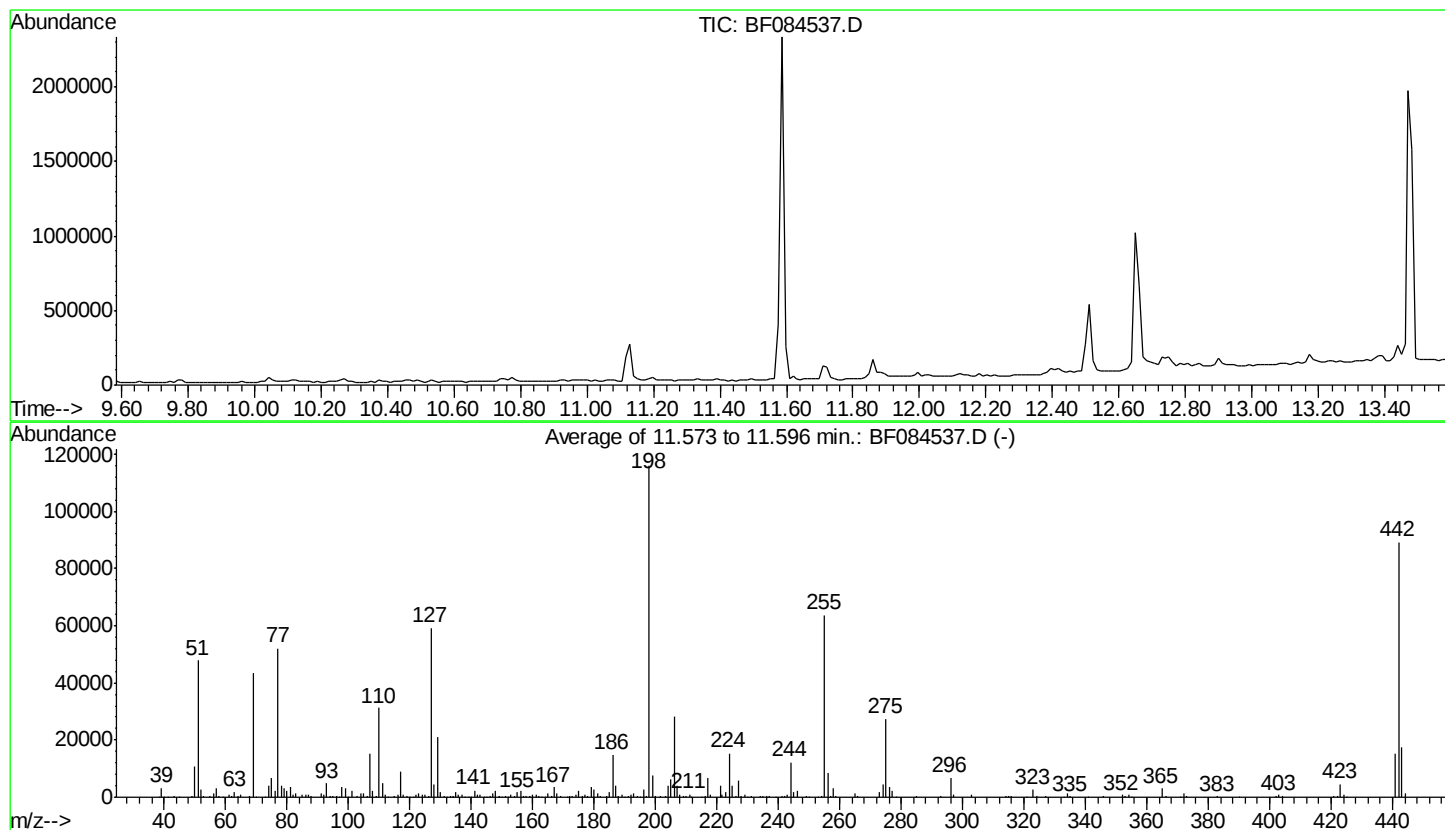

AutoFind: Scans 830, 831, 832; Background Corrected with Scan 827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.3	47868	PASS
68	69	0.00	2	0.7	315	PASS
69	198	0.00	100	37.4	43368	PASS
70	69	0.00	2	0.1	54	PASS
127	198	10	80	51.0	59182	PASS
197	198	0.00	2	0.4	469	PASS
198	198	100	100	100.0	115930	PASS
199	198	5	9	6.7	7711	PASS
275	198	10	60	23.6	27348	PASS
365	198	1	100	2.6	3009	PASS
441	442	0.01	24	17.2	15287	PASS
442	198	50	100	76.9	89132	PASS
443	442	15	24	19.4	17330	PASS