
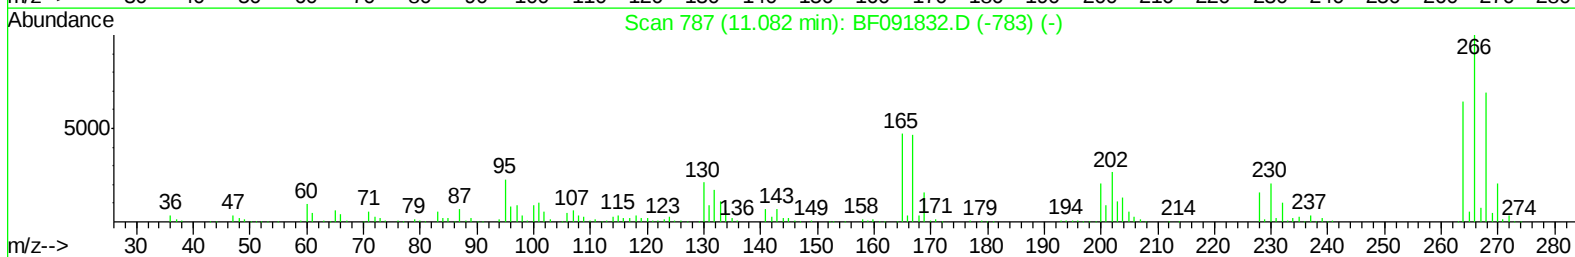
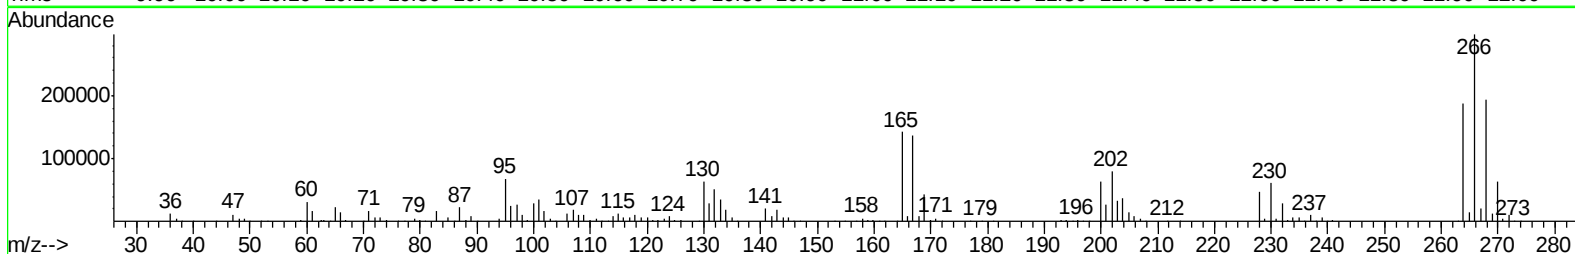


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011817\
Data File : BF092341.D
Acq On : 18 Jan 2017 10:07
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 19 07:11:00 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 19 01:06:01 2017
Response via : Initial Calibration

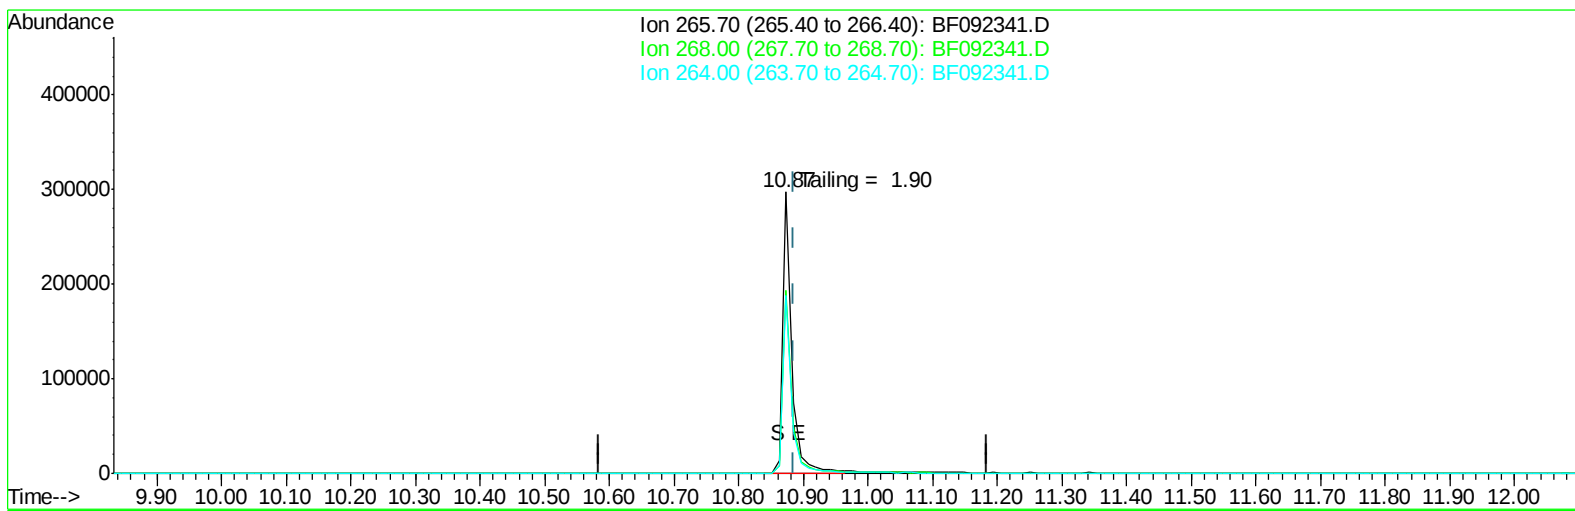

TIC: BF092341.D

(69) Pentachlorophenol (C)




10.873min (-0.012) 87553.53ng

response 309054

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	65.08
264.00	62.90	63.23
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011817\
Data File : BF092341.D
Acq On : 18 Jan 2017 10:07
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 19 07:11:00 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 19 01:06:01 2017
Response via : Initial Calibration

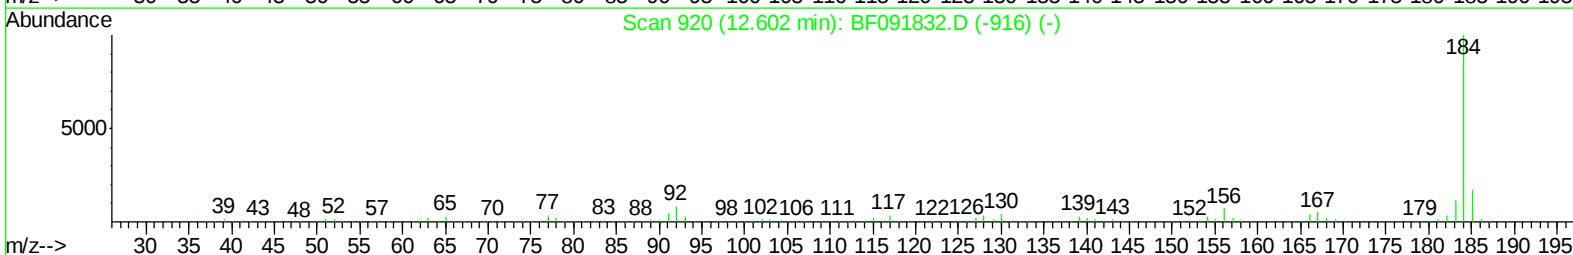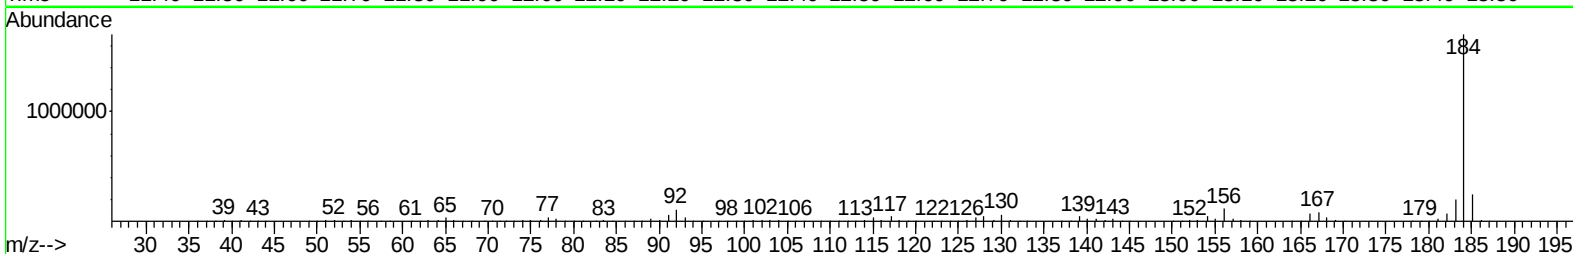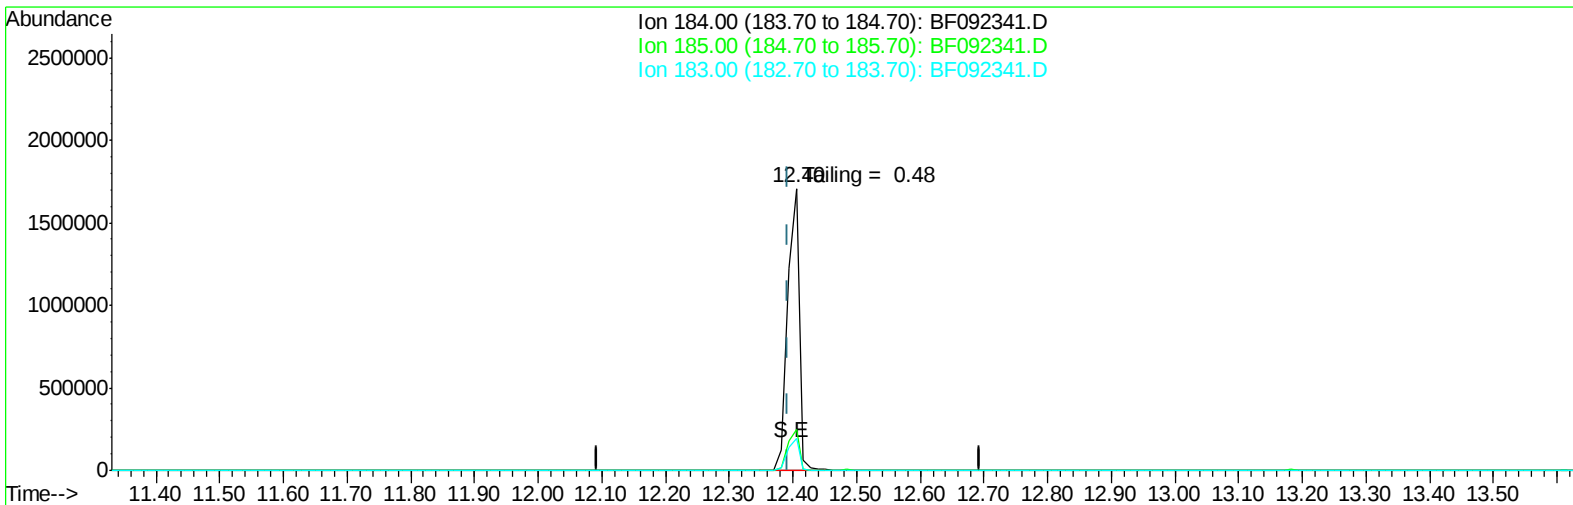

TIC: BF092341.D

(76) Benzidine

12.405min (+0.011) -20.00ng

response 2176393

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.59
183.00	11.50	11.58
0.00	0.00	0.00