

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011817\
 Data File : BF092358.D
 Acq On : 18 Jan 2017 18:32
 Operator : UM/SJ
 Sample : I1260-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MH-0-12FT-COMP

Quant Time: Jan 19 02:58:15 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 19 01:06:01 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.54	152	142798	20.00	ng	0.00
21) Naphthalene-d8	7.83	136	604413	20.00	ng	0.00
38) Acenaphthene-d10	9.57	164	349987	20.00	ng	-0.01
63) Phenanthrene-d10	11.06	188	517728	20.00	ng	0.00
75) Chrysene-d12	13.69	240	345633	20.00	ng	-0.01
86) Perylene-d12	15.03	264	375582	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.12	112	1046869	122.41	ng	0.00
7) Phenol-d6	6.21	99	1367608	130.98	ng	-0.01
23) Nitrobenzene-d5	7.11	82	770388	70.88	ng	-0.01
41) 2,4,6-Tribromophenol	10.37	330	344912	119.08	ng	0.00
44) 2-Fluorobiphenyl	8.91	172	1649919	98.67	ng	-0.01
78) Terphenyl-d14	12.63	244	1123766	78.85	ng	-0.01
Target Compounds						
10) Phenol	6.22	94	60759	5.11	ng	# 74
49) Dimethylphthalate	9.31	163	199769	8.92	ng	# 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011817\
Data File : BF092358.D
Acq On : 18 Jan 2017 18:32
Operator : UM/SJ
Sample : I1260-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MH-0-12FT-COMP

Quant Time: Jan 19 02:58:15 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 19 01:06:01 2017
Response via : Initial Calibration

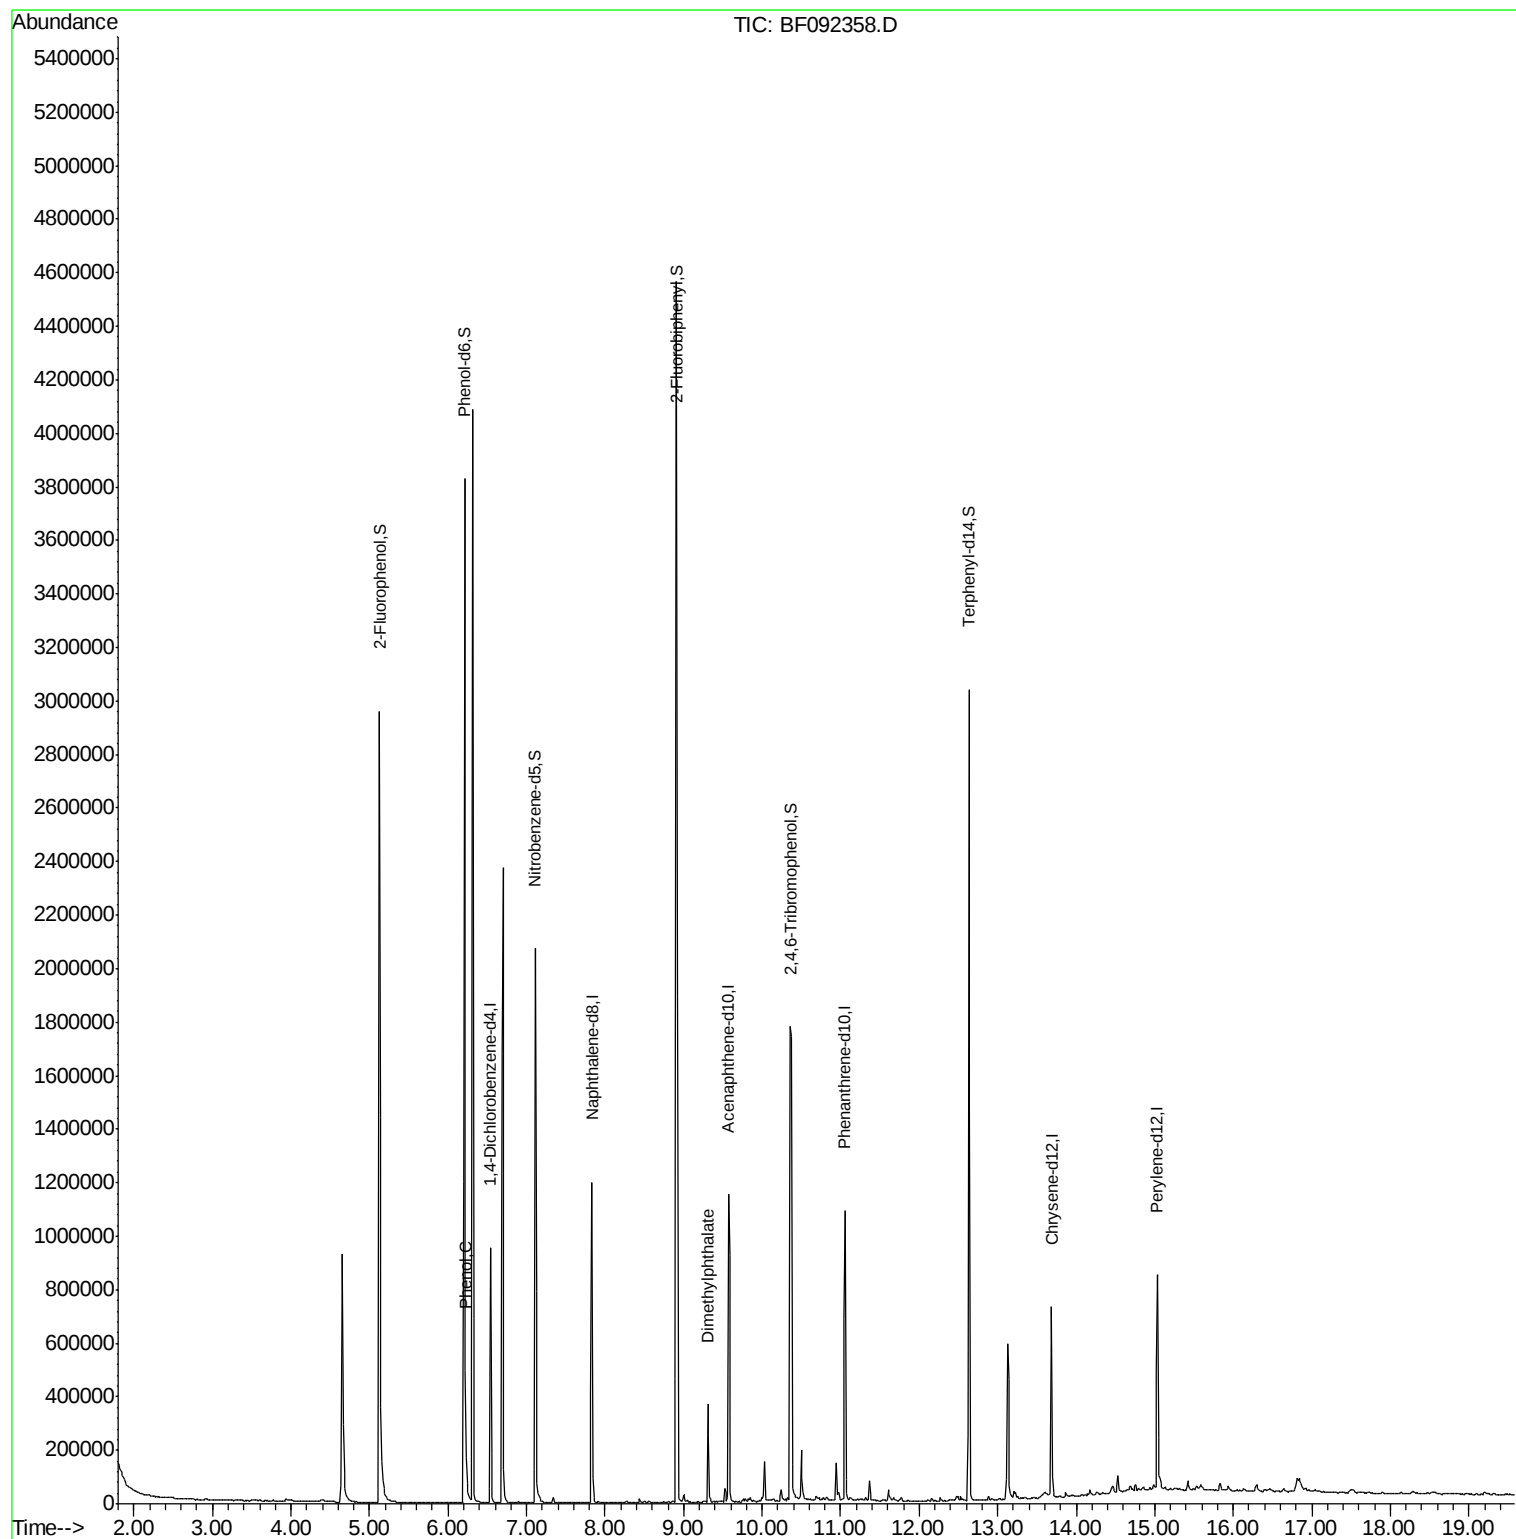

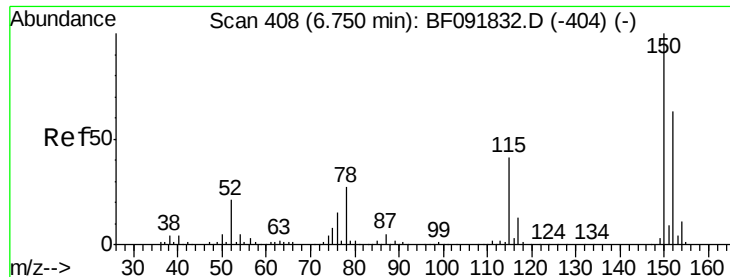

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.54 min Scan# 416

Delta R.T. -0.00 min

Lab File: BF092358.D

Acq: 18 Jan 2017 18:32

Instrument :

BNA_F

ClientSampleId :

MH-0-12FT-COMP


Tgt Ion:152 Resp: 142798

Ion Ratio Lower Upper

152 100

150 156.7 124.9 187.3



115 61.4 46.0 69.0

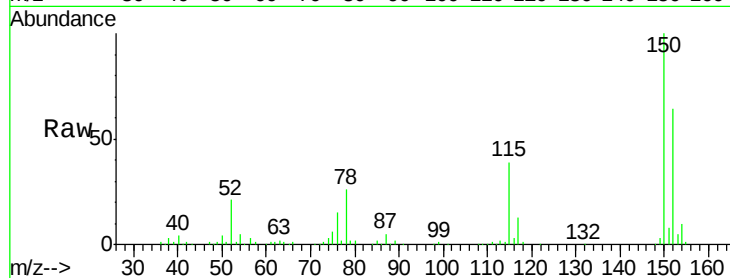

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

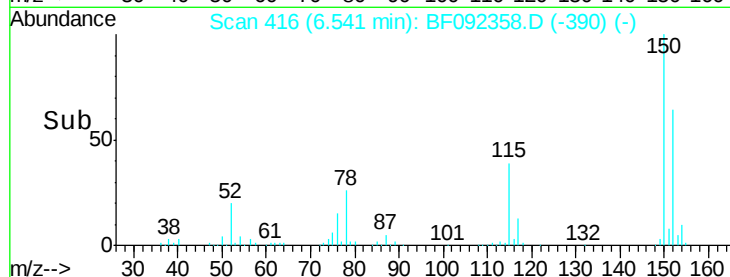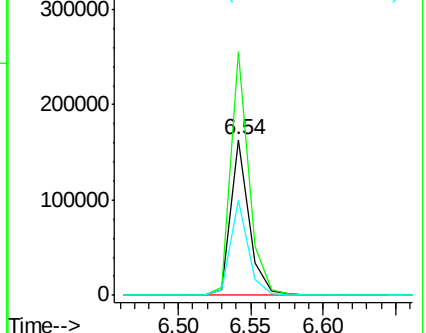

#5

2-Fluorophenol

Concen: 122.41 ng

RT: 5.12 min Scan# 292

Delta R.T. -0.00 min

Lab File: BF092358.D

Acq: 18 Jan 2017 18:32


Tgt Ion:112 Resp: 1046869

Ion Ratio Lower Upper

112 100

64 67.8 46.1 69.1



63 35.0 23.8 35.6

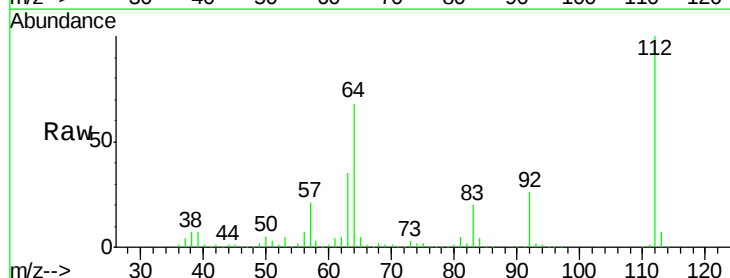

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

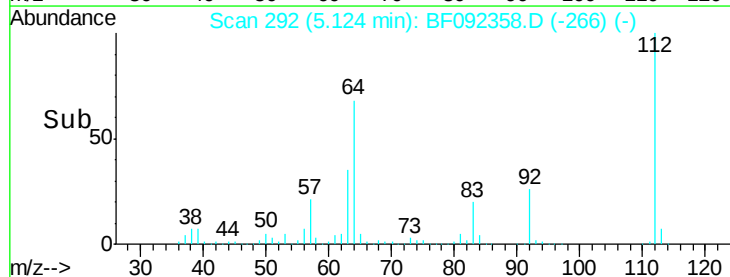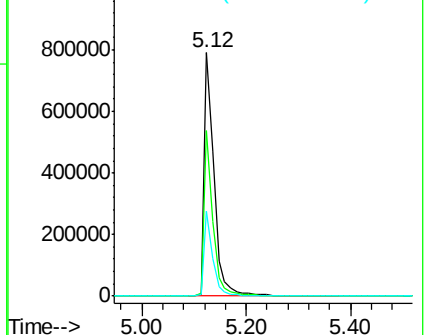



#7

Phenol-d6

Concen: 130.98 ng

RT: 6.21 min Scan# 387

Delta R.T. -0.01 min

Lab File: BF092358.D

Acq: 18 Jan 2017 18:32

Instrument :

BNA_F

ClientSampleId :

MH-0-12FT-COMP


Tgt Ion: 99 Resp: 1367608

Ion Ratio Lower Upper

99 100

42 19.2 15.6 23.4




71 34.5 27.5 41.3

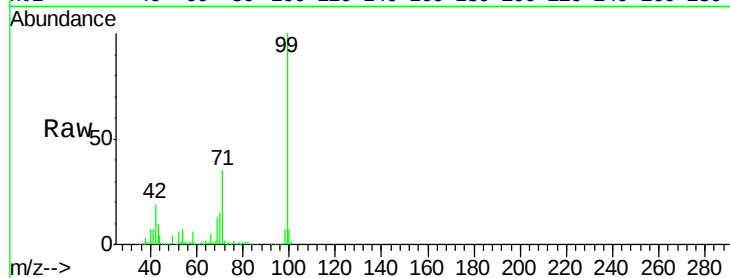

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

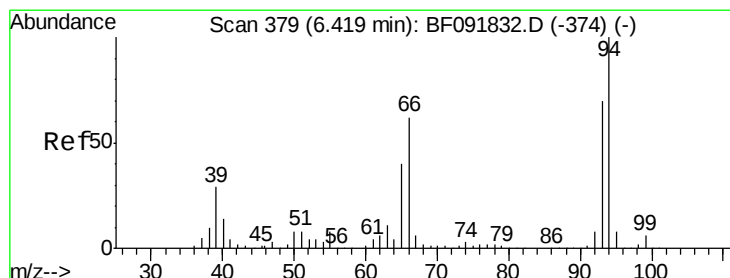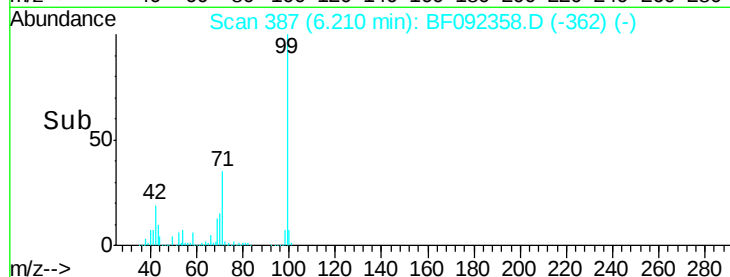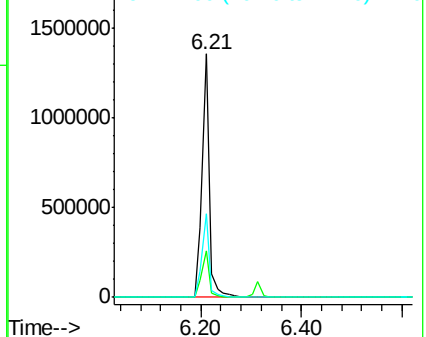

#10

Phenol

Concen: 5.11 ng

RT: 6.22 min Scan# 388

Delta R.T. -0.01 min

Lab File: BF092358.D

Acq: 18 Jan 2017 18:32


Tgt Ion: 94 Resp: 60759

Ion Ratio Lower Upper

94 100

65 27.5 21.4 61.4



66 41.5 44.0 84.0#

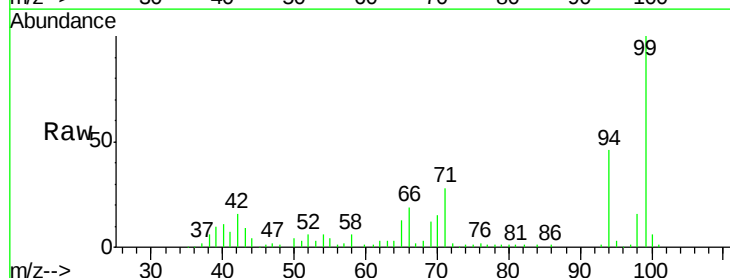


Abundance Ion 94.00 (93.70 to 94.70): BF0

Ion 65.00 (64.70 to 65.70): BF0

Ion 66.00 (65.70 to 66.70): BF0

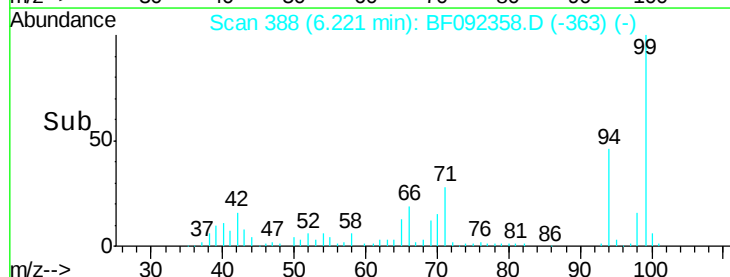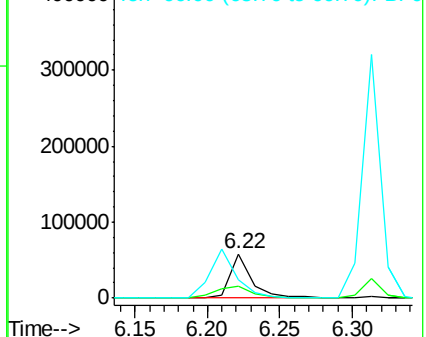


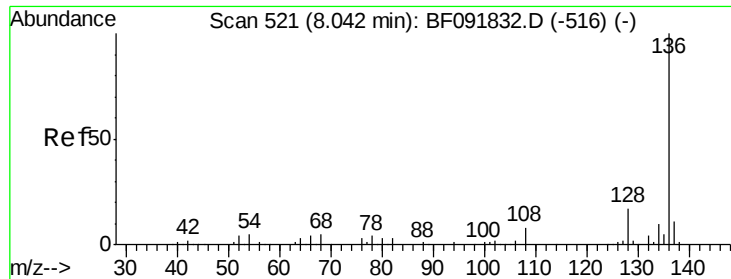




#21
Naphthalene-d8
Concen: 20.00 ng
RT: 7.83 min Scan# 529
Delta R.T. -0.00 min
Lab File: BF092358.D
Acq: 18 Jan 2017 18:32

Instrument :
BNA_F
ClientSampleId :
MH-0-12FT-COMP

Tgt Ion:	136	Resp:	604413
Ion	Ratio	Lower	Upper
136	100		
137	10.9	8.4	12.6
54	6.5	4.5	6.7
68	5.5	3.6	5.4#

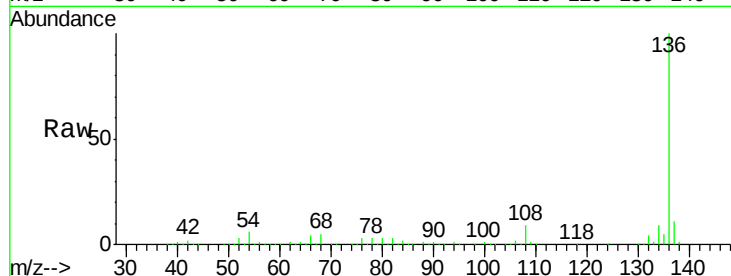


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

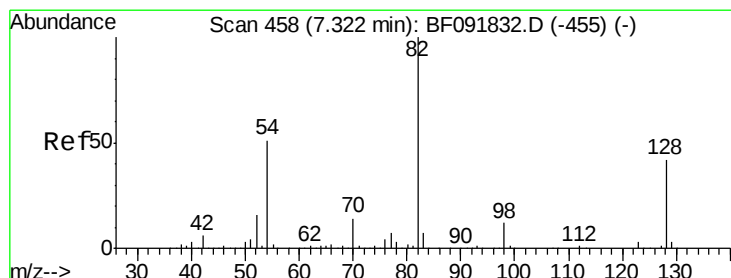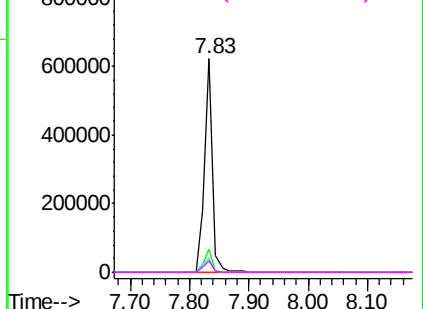
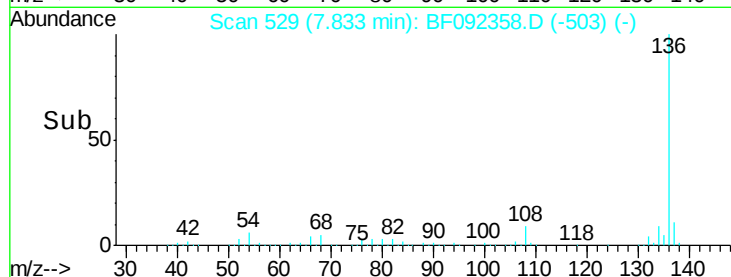



#23
Nitrobenzene-d5
Concen: 70.88 ng
RT: 7.11 min Scan# 466
Delta R.T. -0.01 min
Lab File: BF092358.D
Acq: 18 Jan 2017 18:32

Tgt Ion:	82	Resp:	770388
Ion	Ratio	Lower	Upper
82	100		
128	38.8	34.6	52.0
54	51.8	39.5	59.3

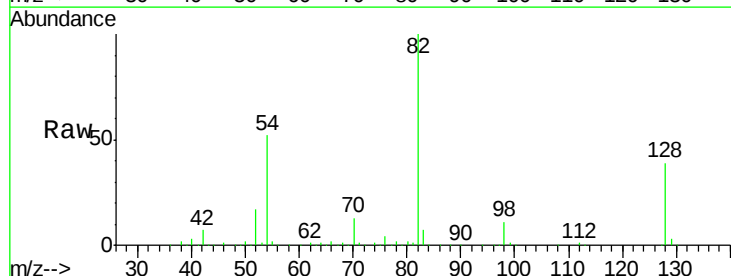

Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

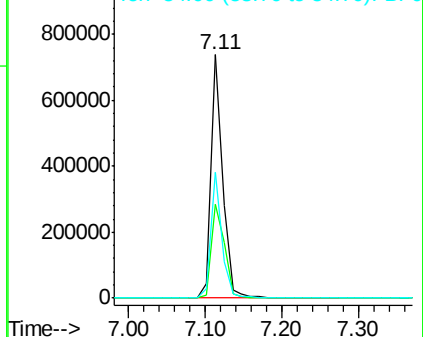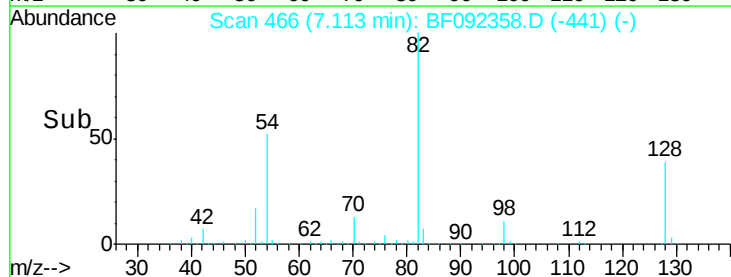

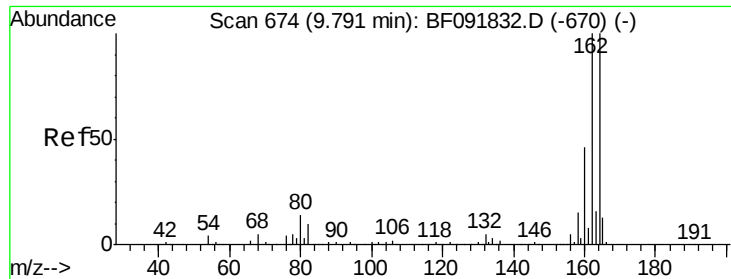

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.57 min Scan# 681

Delta R.T. -0.01 min

Lab File: BF092358.D

Acq: 18 Jan 2017 18:32

Instrument :

BNA_F

ClientSampleId :

MH-0-12FT-COMP


Tgt Ion:164 Resp: 349987

Ion Ratio Lower Upper

164 100

162 101.9 80.2 120.2




160 45.3 36.9 55.3

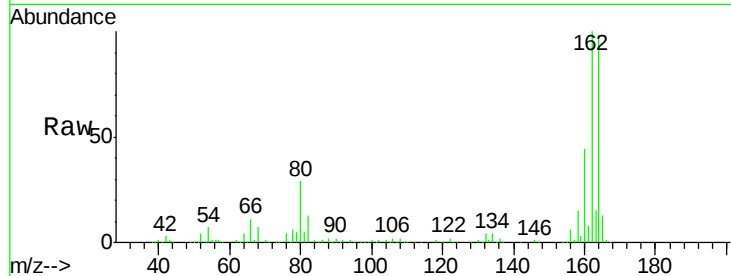

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

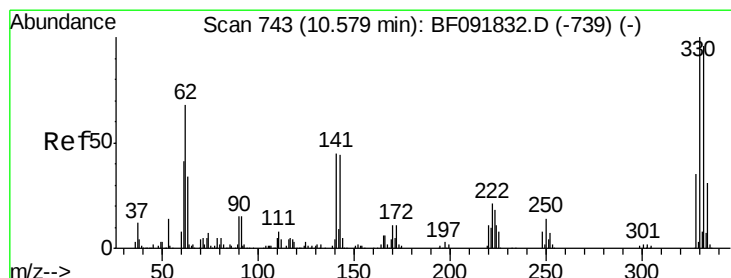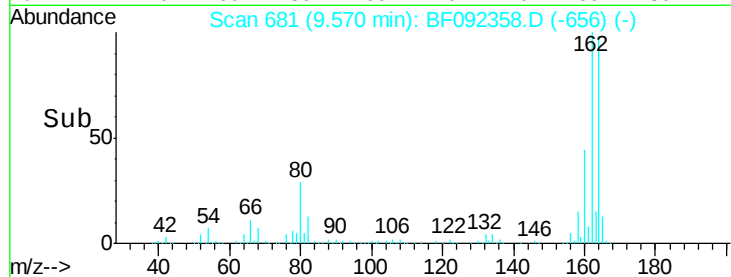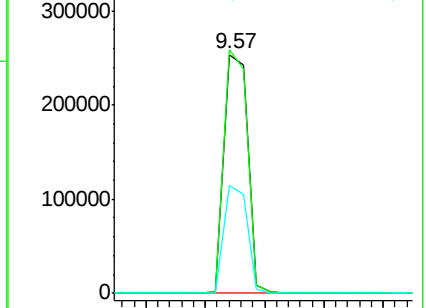

#41

2,4,6-Tribromophenol

Concen: 119.08 ng

RT: 10.37 min Scan# 751

Delta R.T. -0.00 min

Lab File: BF092358.D

Acq: 18 Jan 2017 18:32


Tgt Ion:330 Resp: 344912

Ion Ratio Lower Upper

330 100

332 97.0 77.4 116.2



141 33.5 34.1 51.1#

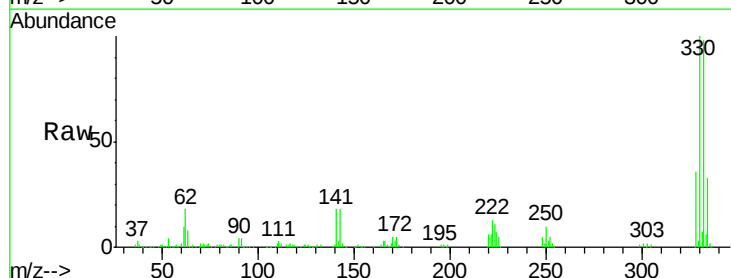


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

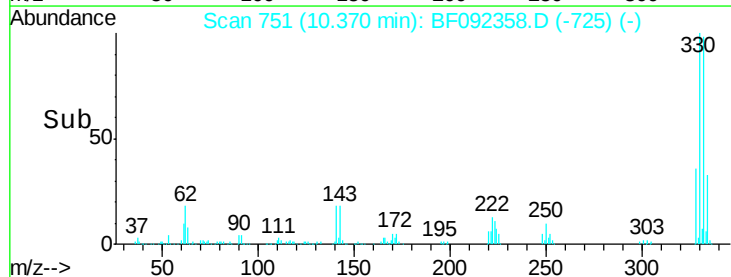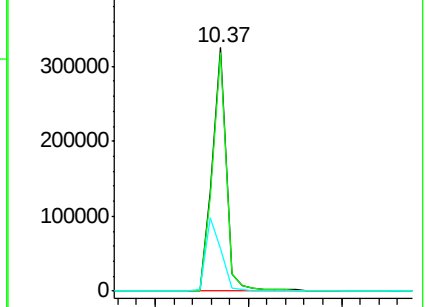


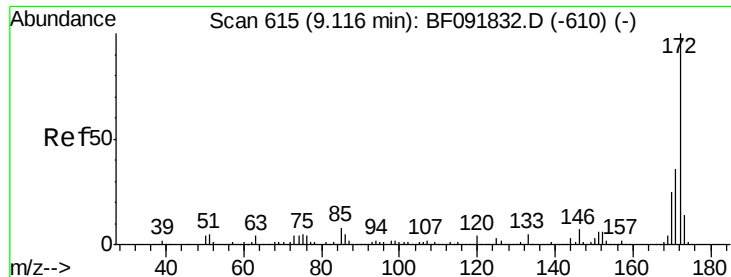




#44
 2-Fluorobiphenyl
 Concen: 98.67 ng
 RT: 8.91 min Scan# 623
 Delta R.T. -0.01 min
 Lab File: BF092358.D
 Acq: 18 Jan 2017 18:32

Instrument :
 BNA_F
 ClientSampleId :
 MH-0-12FT-COMP

Tgt Ion:172 Resp: 1649919
 Ion Ratio Lower Upper
 172 100
 171 36.2 29.4 44.0
 170 24.0 20.2 30.4

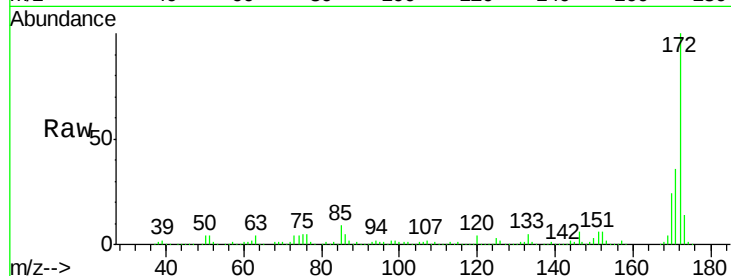


Abundance Ion 172.00 (171.70 to 172.70): E
 2000000 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

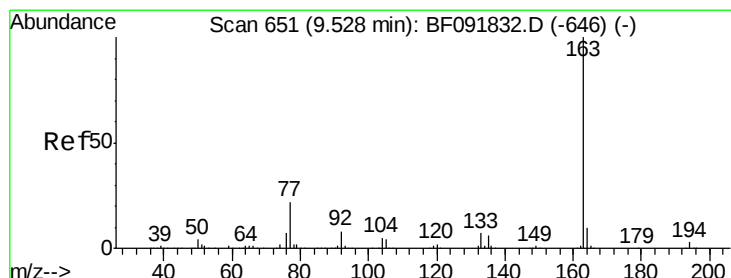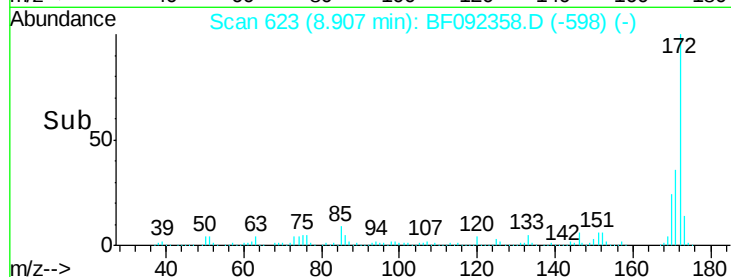
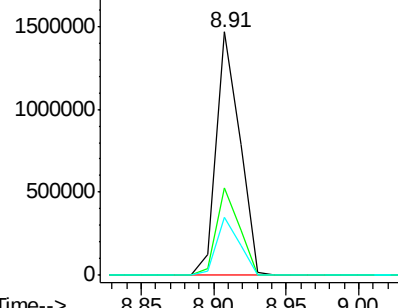



#49
 Dimethylphthalate
 Concen: 8.92 ng
 RT: 9.31 min Scan# 658
 Delta R.T. -0.02 min
 Lab File: BF092358.D
 Acq: 18 Jan 2017 18:32

Tgt Ion:163 Resp: 199769
 Ion Ratio Lower Upper
 163 100
 194 2.6 3.0 4.4#
 164 10.6 8.0 12.0

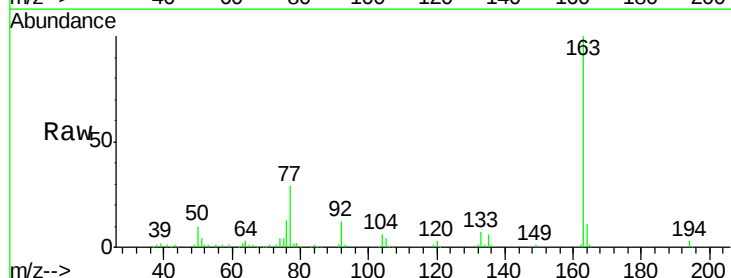

Abundance Ion 163.00 (162.70 to 163.70): E
 200000 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

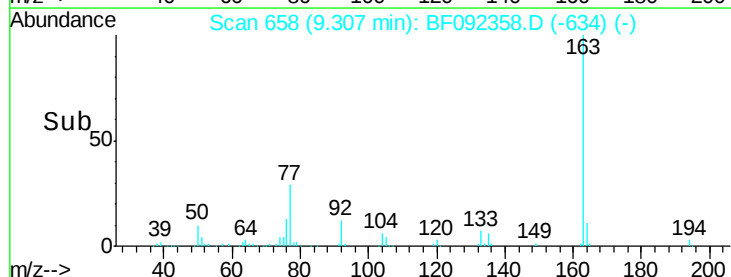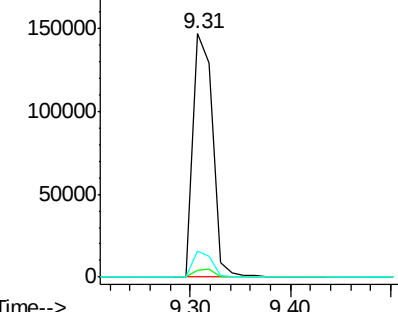


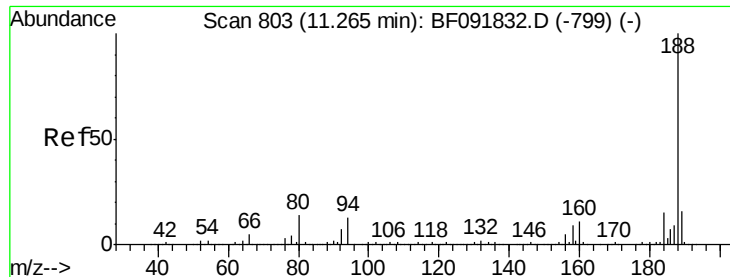




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.06 min Scan# 811
Delta R.T. -0.00 min
Lab File: BF092358.D
Acq: 18 Jan 2017 18:32

Instrument :
BNA_F
ClientSampleId :
MH-0-12FT-COMP

Tgt Ion:188 Resp: 517728
Ion Ratio Lower Upper
188 100
94 7.2 10.0 15.0#
80 7.6 11.2 16.8#

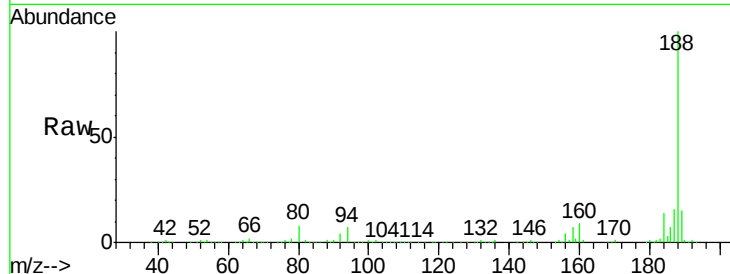


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

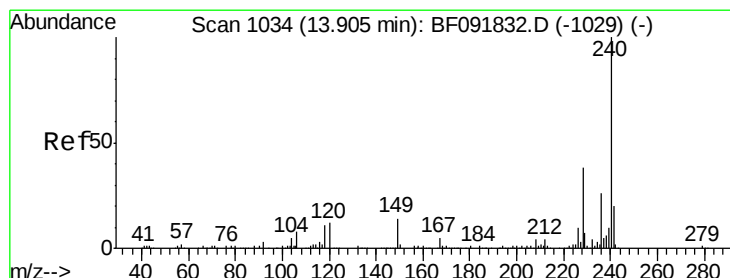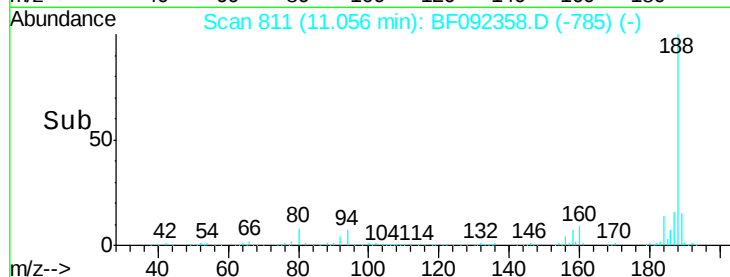
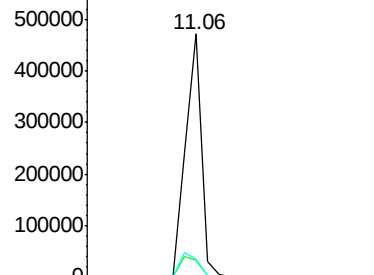



#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.69 min Scan# 1041
Delta R.T. -0.01 min
Lab File: BF092358.D
Acq: 18 Jan 2017 18:32

Tgt Ion:240 Resp: 345633
Ion Ratio Lower Upper
240 100
120 9.2 12.9 19.3#
236 24.7 20.9 31.3

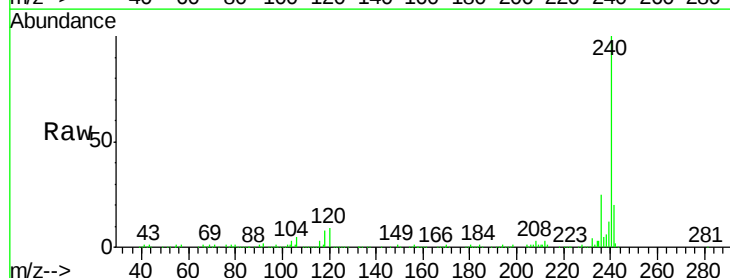

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

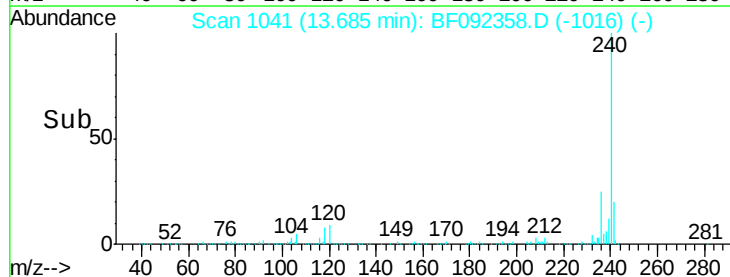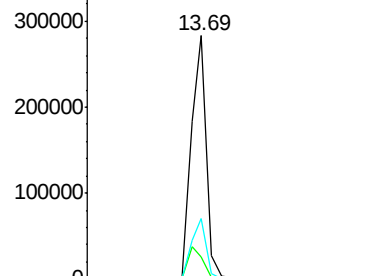

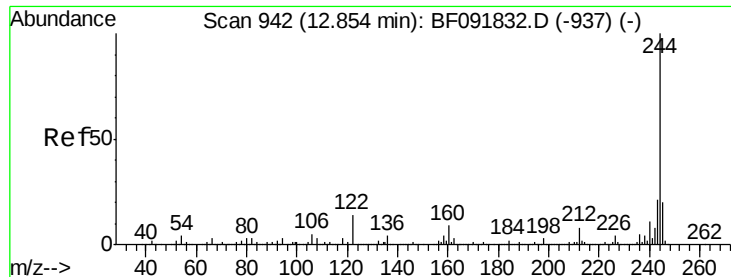

#78

Terphenyl-d14

Concen: 78.85 ng

RT: 12.63 min Scan# 949

Delta R.T. -0.01 min

Lab File: BF092358.D

Acq: 18 Jan 2017 18:32

Instrument :

BNA_F

ClientSampleId :

MH-0-12FT-COMP


Tgt Ion:244 Resp: 1123766

Ion Ratio Lower Upper

244 100

212 7.0 6.2 9.2




122 15.0 11.4 17.2

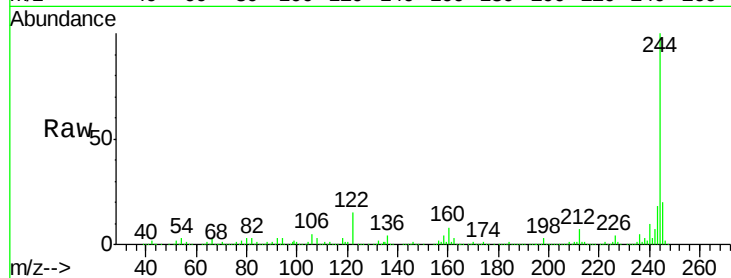

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

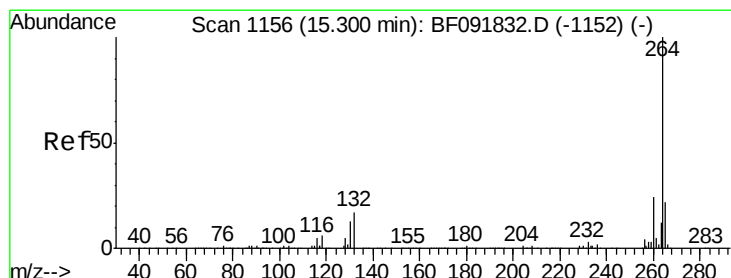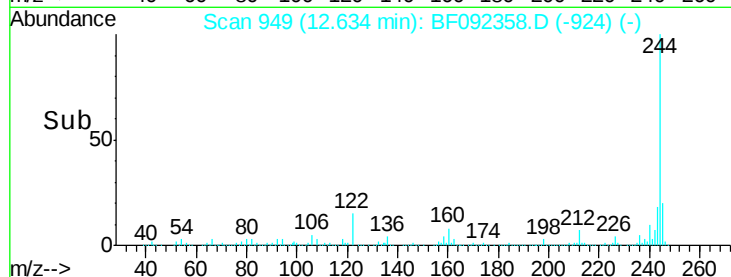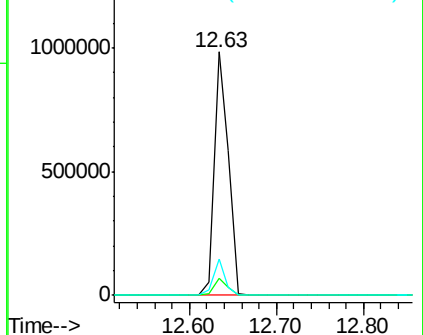

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.03 min Scan# 1159

Delta R.T. -0.00 min

Lab File: BF092358.D

Acq: 18 Jan 2017 18:32


Tgt Ion:264 Resp: 375582

Ion Ratio Lower Upper

264 100

260 22.9 19.2 28.8

265 21.7 17.4 26.0

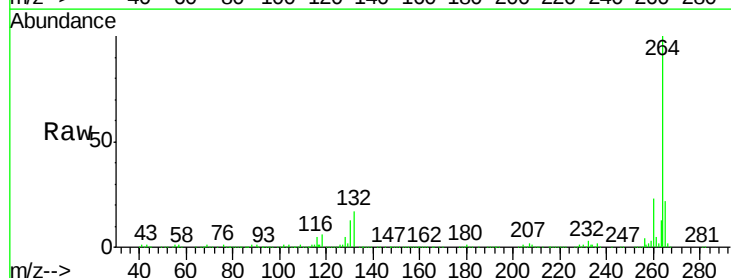

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

