

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011817\
 Data File : BF092361.D
 Acq On : 18 Jan 2017 19:57
 Operator : UM/SJ
 Sample : I1271-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SS-02

Quant Time: Jan 19 03:15:21 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 19 01:06:01 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.54	152	171540	20.00	ng	0.00
21) Naphthalene-d8	7.83	136	560104	20.00	ng	0.00
38) Acenaphthene-d10	9.57	164	270605	20.00	ng	-0.01
63) Phenanthrene-d10	11.06	188	480138	20.00	ng	0.00
75) Chrysene-d12	13.69	240	373046	20.00	ng	-0.01
86) Perylene-d12	15.03	264	421551	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.12	112	1039149	101.15	ng	0.00
7) Phenol-d6	6.21	99	1374767	109.60	ng	-0.01
23) Nitrobenzene-d5	7.11	82	741699	73.63	ng	-0.01
41) 2,4,6-Tribromophenol	10.37	330	320424	143.08	ng	0.00
44) 2-Fluorobiphenyl	8.91	172	1207479	92.58	ng	-0.01
78) Terphenyl-d14	12.63	244	1056489	68.69	ng	-0.01
Target Compounds						
10) Phenol	6.22	94	56035	3.92	ng	# 73
49) Dimethylphthalate	9.31	163	100139	5.79	ng	# 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011817\
Data File : BF092361.D
Acq On : 18 Jan 2017 19:57
Operator : UM/SJ
Sample : I1271-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SS-02

Quant Time: Jan 19 03:15:21 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 19 01:06:01 2017
Response via : Initial Calibration

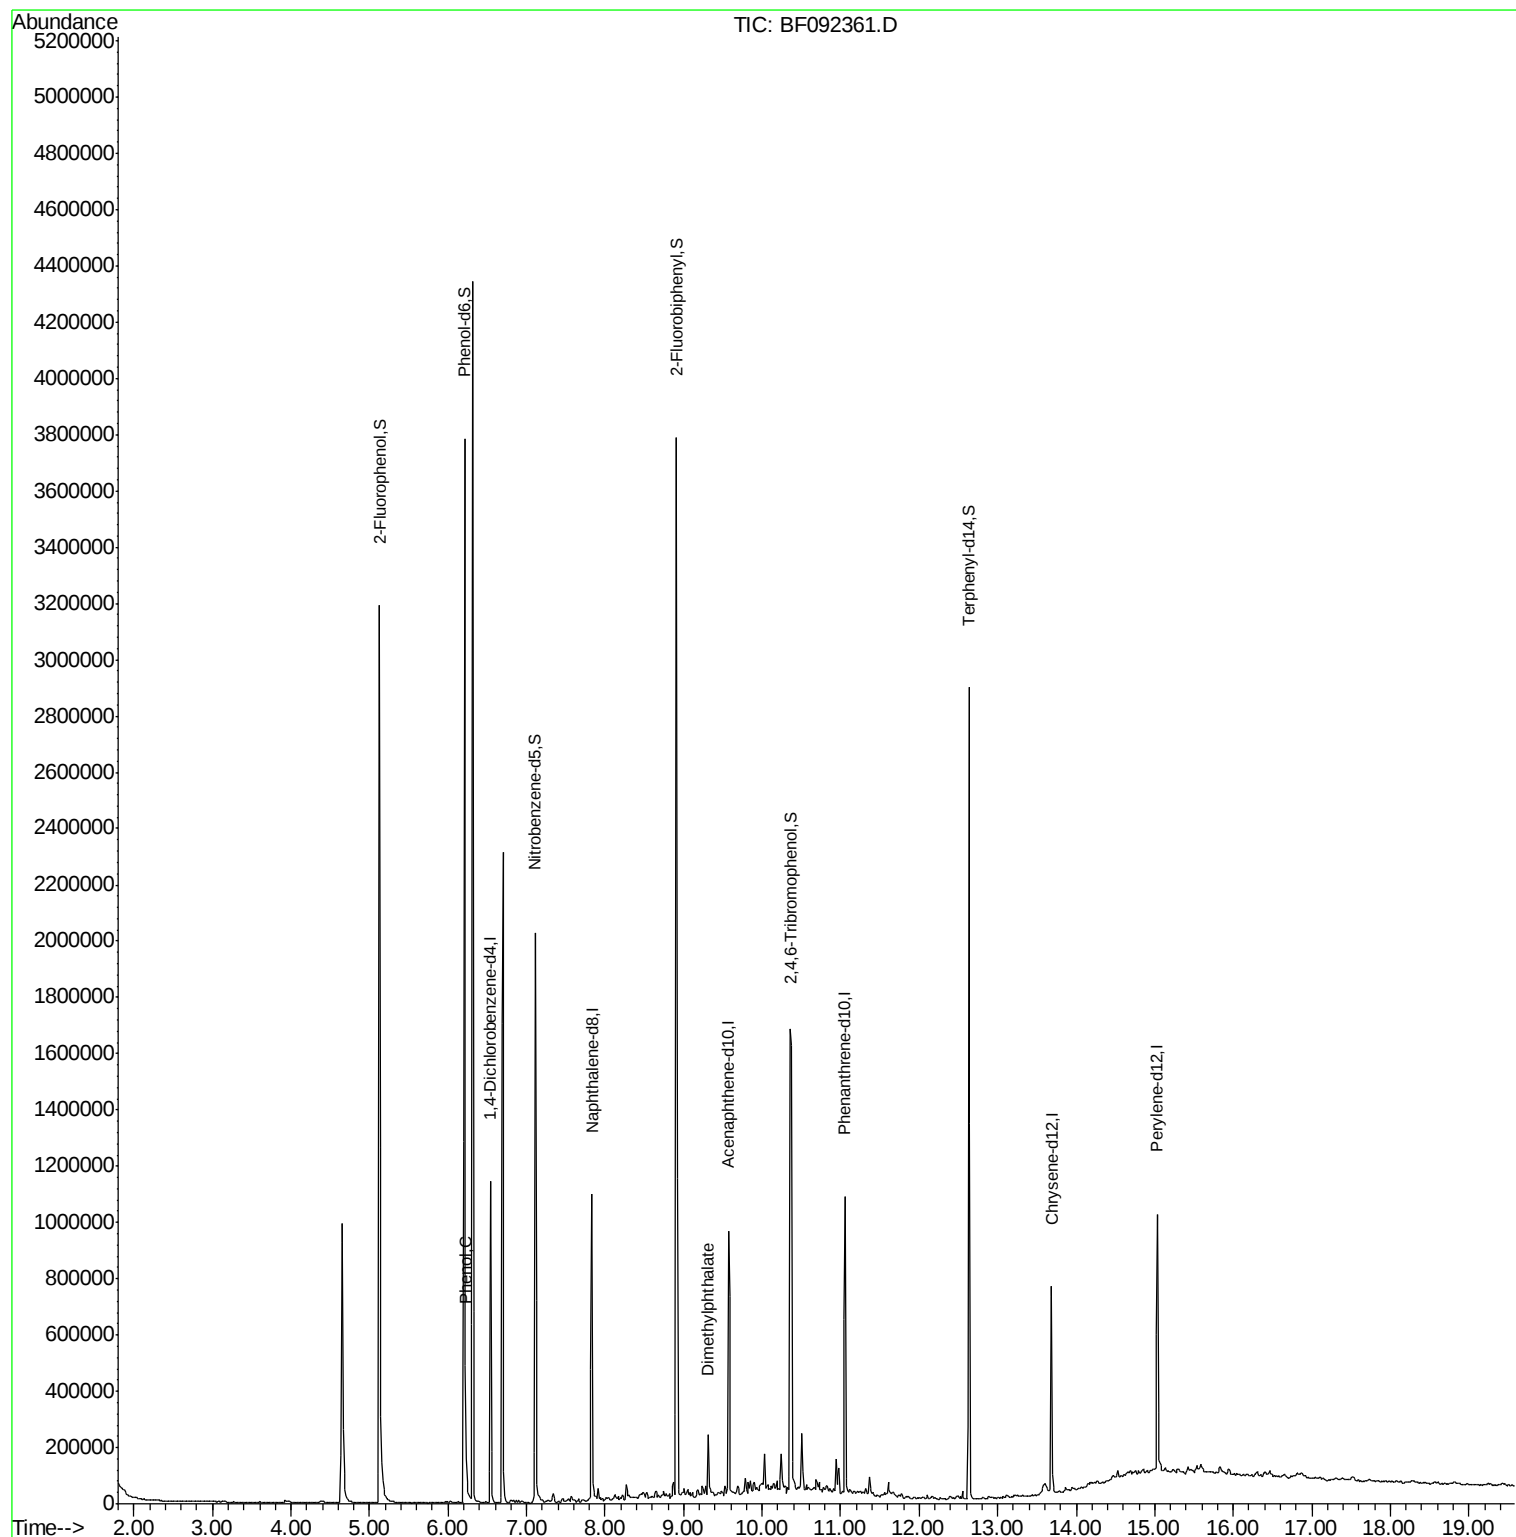

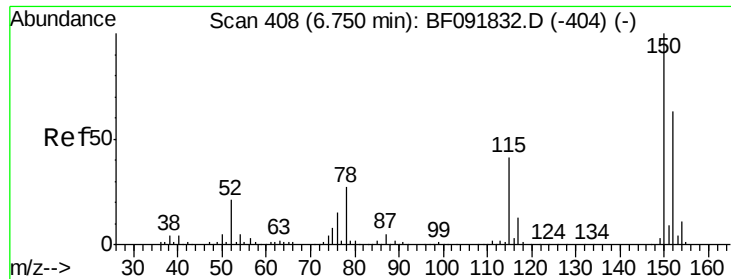

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.54 min Scan# 416

Delta R.T. 0.00 min

Lab File: BF092361.D

Acq: 18 Jan 2017 19:57

Instrument :

BNA_F

ClientSampleId :

SS-02


Tgt Ion:152 Resp: 171540

Ion Ratio Lower Upper

152 100

150 156.2 124.9 187.3




115 61.6 46.0 69.0

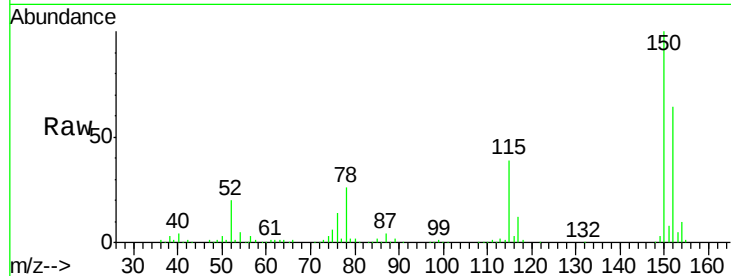

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

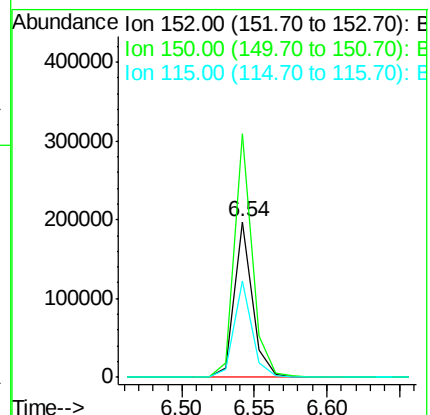

#5

2-Fluorophenol

Concen: 101.15 ng

RT: 5.12 min Scan# 292

Delta R.T. 0.00 min

Lab File: BF092361.D

Acq: 18 Jan 2017 19:57


Tgt Ion:112 Resp: 1039149

Ion Ratio Lower Upper

112 100

64 67.2 46.1 69.1



63 34.3 23.8 35.6



Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

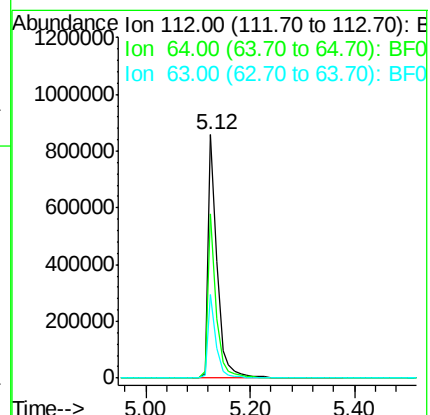



#7

Phenol-d6

Concen: 109.60 ng

RT: 6.21 min Scan# 387

Delta R.T. -0.01 min

Lab File: BF092361.D

Acq: 18 Jan 2017 19:57

Instrument :

BNA_F

ClientSampleId :

SS-02


Tgt Ion: 99 Resp: 1374767

Ion Ratio Lower Upper

99 100

42 19.6 15.6 23.4




71 34.6 27.5 41.3

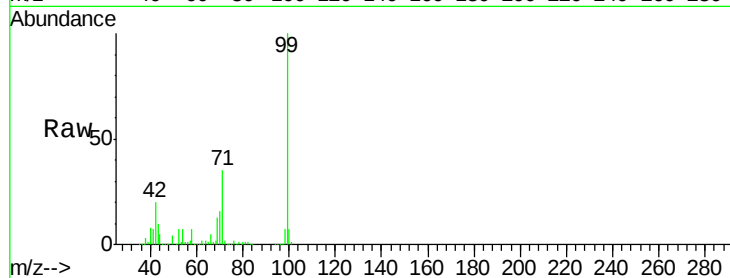

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

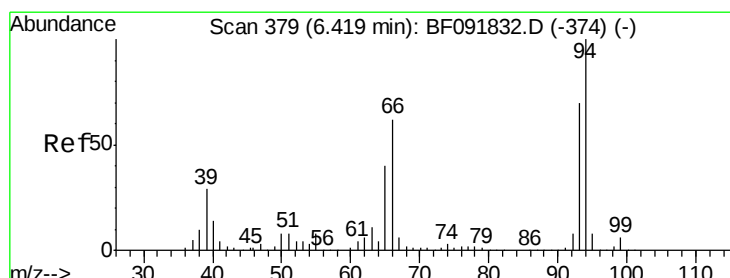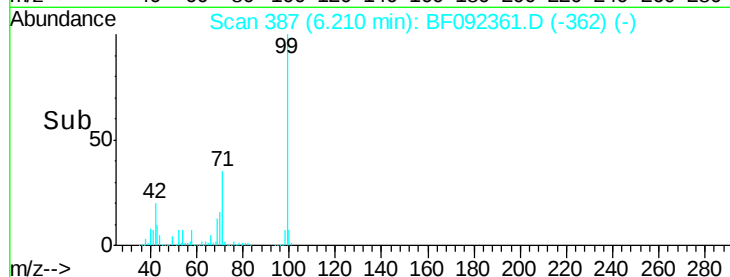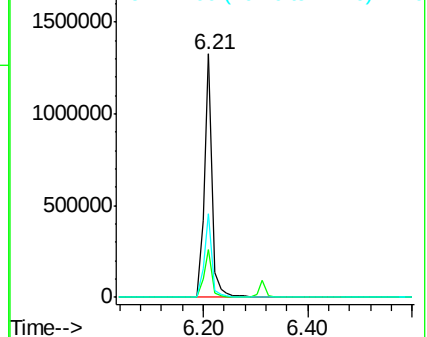

#10

Phenol

Concen: 3.92 ng

RT: 6.22 min Scan# 388

Delta R.T. -0.01 min

Lab File: BF092361.D

Acq: 18 Jan 2017 19:57


Tgt Ion: 94 Resp: 56035

Ion Ratio Lower Upper

94 100

65 26.7 21.4 61.4



66 41.4 44.0 84.0#

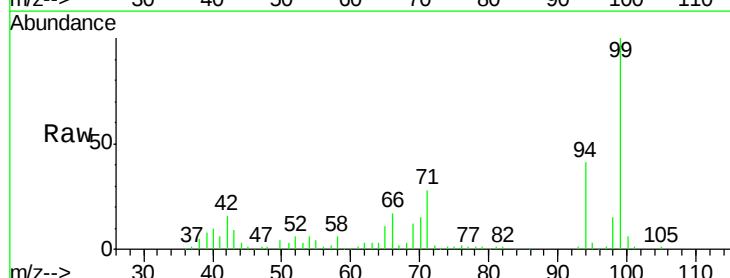


Abundance Ion 94.00 (93.70 to 94.70): BF0

Ion 65.00 (64.70 to 65.70): BF0

Ion 66.00 (65.70 to 66.70): BF0

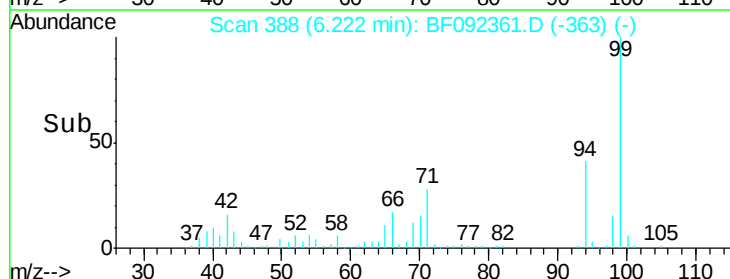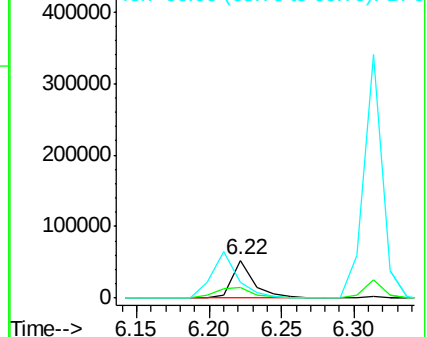


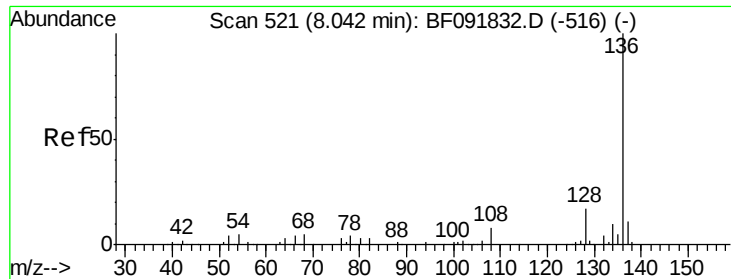




#21
Naphthalene-d8
Concen: 20.00 ng
RT: 7.83 min Scan# 529
Delta R.T. 0.00 min
Lab File: BF092361.D
Acq: 18 Jan 2017 19:57

Instrument :
BNA_F
ClientSampled :
SS-02

Tgt Ion:	136	Resp:	560104
Ion	Ratio	Lower	Upper
136	100		
137	10.8	8.4	12.6
54	6.2	4.5	6.7
68	5.1	3.6	5.4

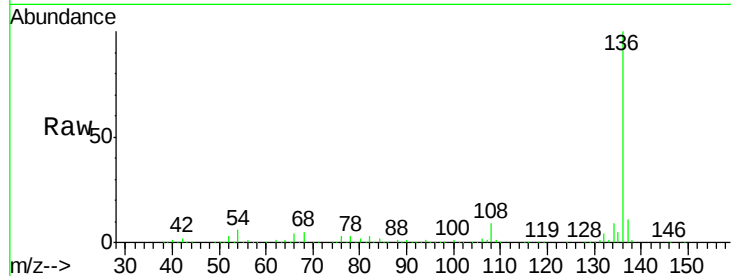


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

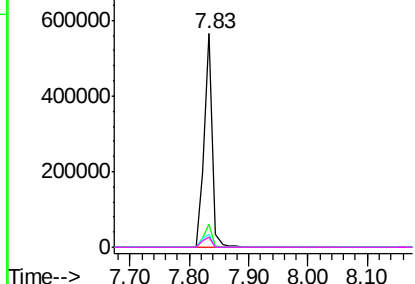




#23
Nitrobenzene-d5
Concen: 73.63 ng
RT: 7.11 min Scan# 466
Delta R.T. -0.01 min
Lab File: BF092361.D
Acq: 18 Jan 2017 19:57

Tgt Ion:	82	Resp:	741699
Ion	Ratio	Lower	Upper
82	100		
128	39.2	34.6	52.0
54	51.9	39.5	59.3



Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

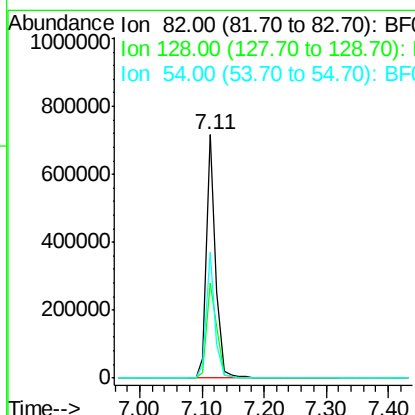


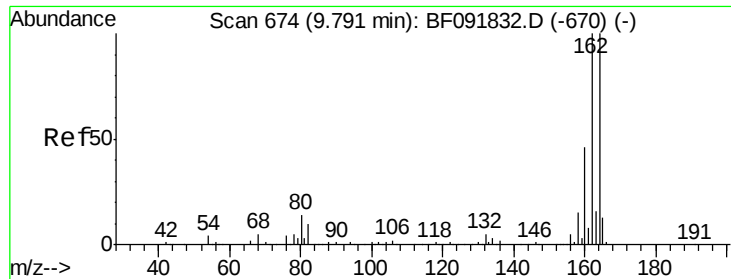




#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.57 min Scan# 681
Delta R.T. -0.01 min
Lab File: BF092361.D
Acq: 18 Jan 2017 19:57

Instrument :
BNA_F
ClientSampled :
SS-02

Tgt Ion:164 Resp: 270605
Ion Ratio Lower Upper
164 100
162 102.8 80.2 120.2
160 45.7 36.9 55.3

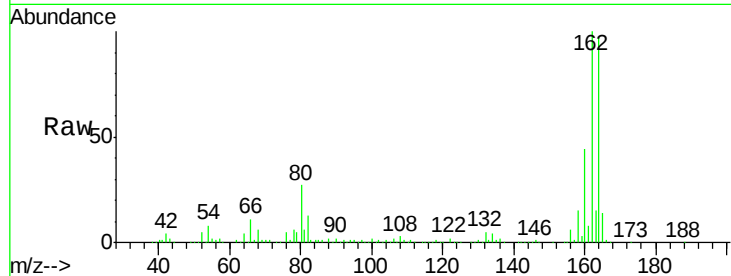


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E


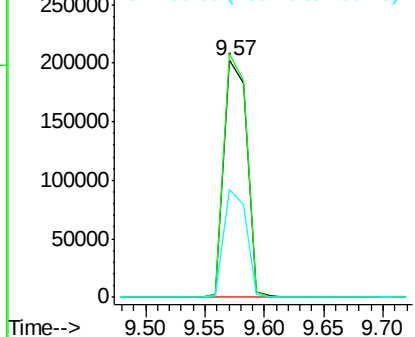



#41
2,4,6-Tribromophenol
Concen: 143.08 ng
RT: 10.37 min Scan# 751
Delta R.T. 0.00 min
Lab File: BF092361.D
Acq: 18 Jan 2017 19:57

Tgt Ion:330 Resp: 320424
Ion Ratio Lower Upper
330 100
332 96.3 77.4 116.2
141 33.1 34.1 51.1#



Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

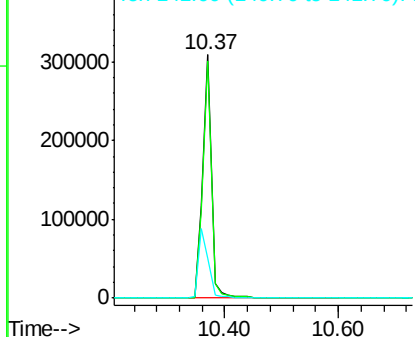


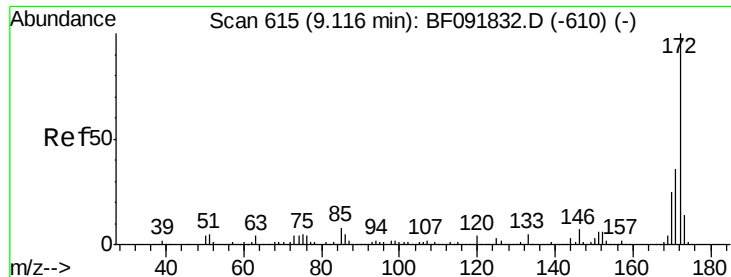




#44
 2-Fluorobiphenyl
 Concen: 92.58 ng
 RT: 8.91 min Scan# 623
 Delta R.T. -0.01 min
 Lab File: BF092361.D
 Acq: 18 Jan 2017 19:57

Instrument :
 BNA_F
 ClientSampleId :
 SS-02

Tgt Ion:172 Resp: 1207479
 Ion Ratio Lower Upper
 172 100
 171 35.8 29.4 44.0
 170 24.0 20.2 30.4




Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

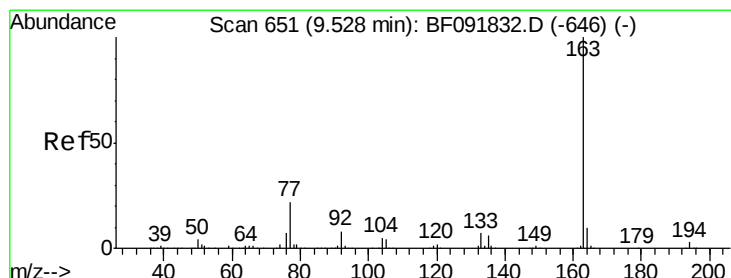
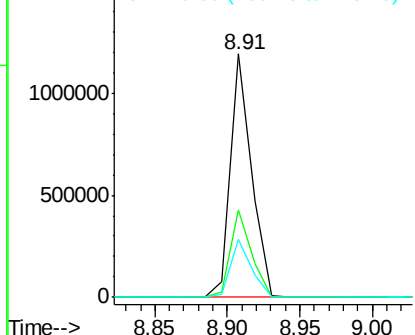



#49
 Dimethylphthalate
 Concen: 5.79 ng
 RT: 9.31 min Scan# 658
 Delta R.T. -0.02 min
 Lab File: BF092361.D
 Acq: 18 Jan 2017 19:57

Tgt Ion:163 Resp: 100139
 Ion Ratio Lower Upper
 163 100
 194 2.6 3.0 4.4#
 164 10.6 8.0 12.0



Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E




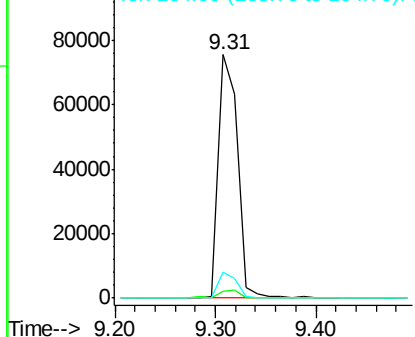


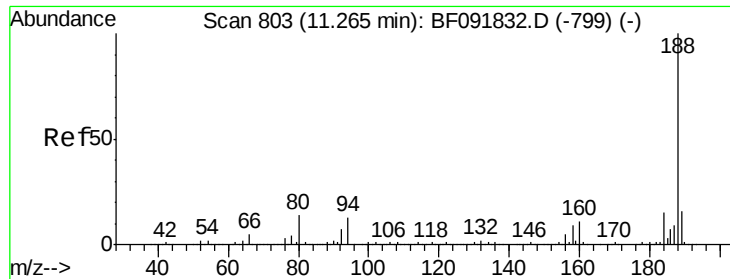

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.06 min Scan# 811
Delta R.T. 0.00 min
Lab File: BF092361.D
Acq: 18 Jan 2017 19:57




Instrument :
BNA_F
ClientSampleId :
SS-02


Tgt Ion:188 Resp: 480138
Ion Ratio Lower Upper
188 100
94 7.6 10.0 15.0#
80 7.7 11.2 16.8#

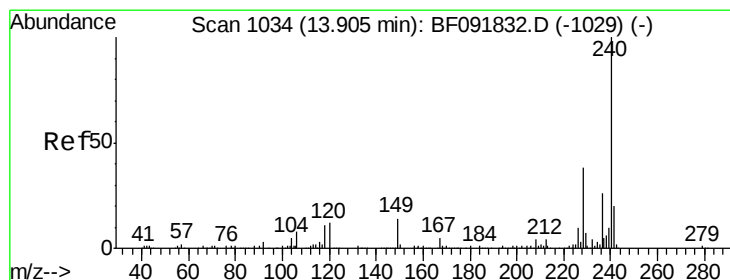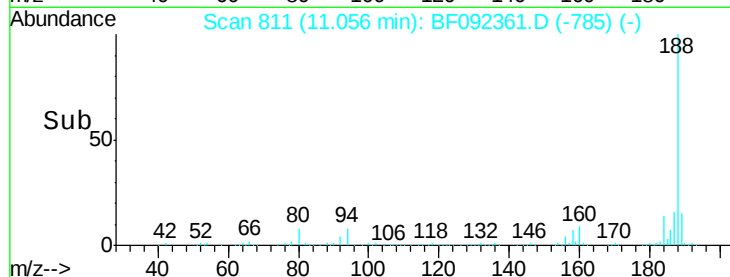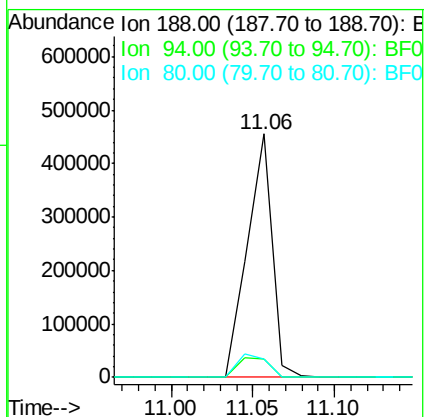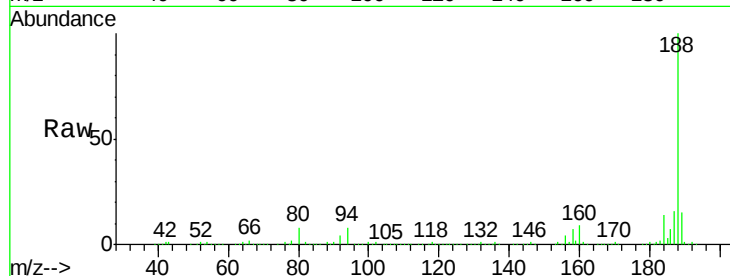

#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.69 min Scan# 1041
Delta R.T. -0.01 min
Lab File: BF092361.D
Acq: 18 Jan 2017 19:57

Tgt Ion:240 Resp: 373046
Ion Ratio Lower Upper
240 100
120 8.9 12.9 19.3#
236 24.0 20.9 31.3


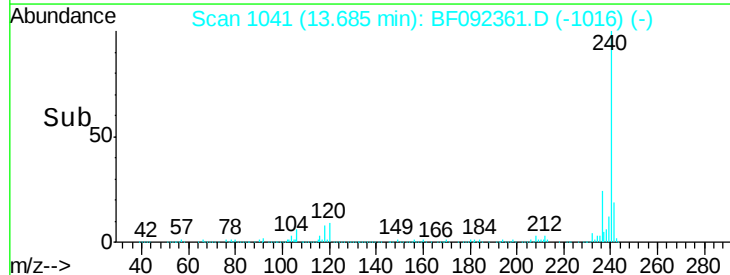
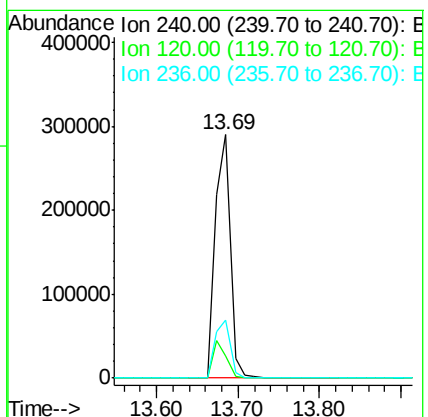
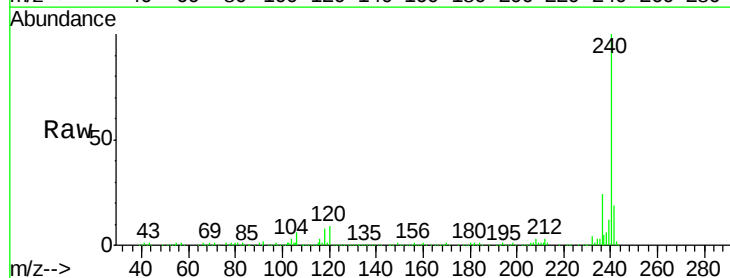




#78
 Terphenyl-d14
 Concen: 68.69 ng
 RT: 12.63 min Scan# 949
 Delta R.T. -0.01 min
 Lab File: BF092361.D
 Acq: 18 Jan 2017 19:57

Instrument :
 BNA_F
 ClientSampleId :
 SS-02

Tgt Ion:244 Resp: 1056489
 Ion Ratio Lower Upper
 244 100
 212 7.1 6.2 9.2
 122 14.6 11.4 17.2

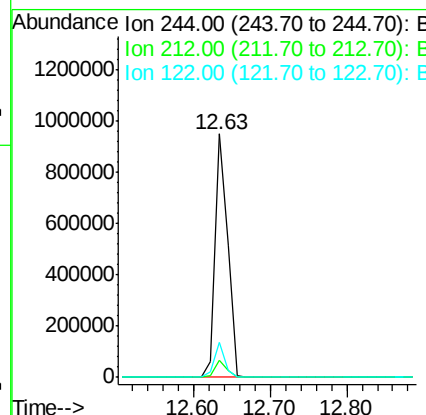

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.03 min Scan# 1159
 Delta R.T. 0.00 min
 Lab File: BF092361.D
 Acq: 18 Jan 2017 19:57

Tgt Ion:264 Resp: 421551
 Ion Ratio Lower Upper
 264 100
 260 23.7 19.2 28.8
 265 21.8 17.4 26.0

