


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011817\
 Data File : BF092341.D
 Acq On : 18 Jan 2017 10:07
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 06 15:43:51 2017

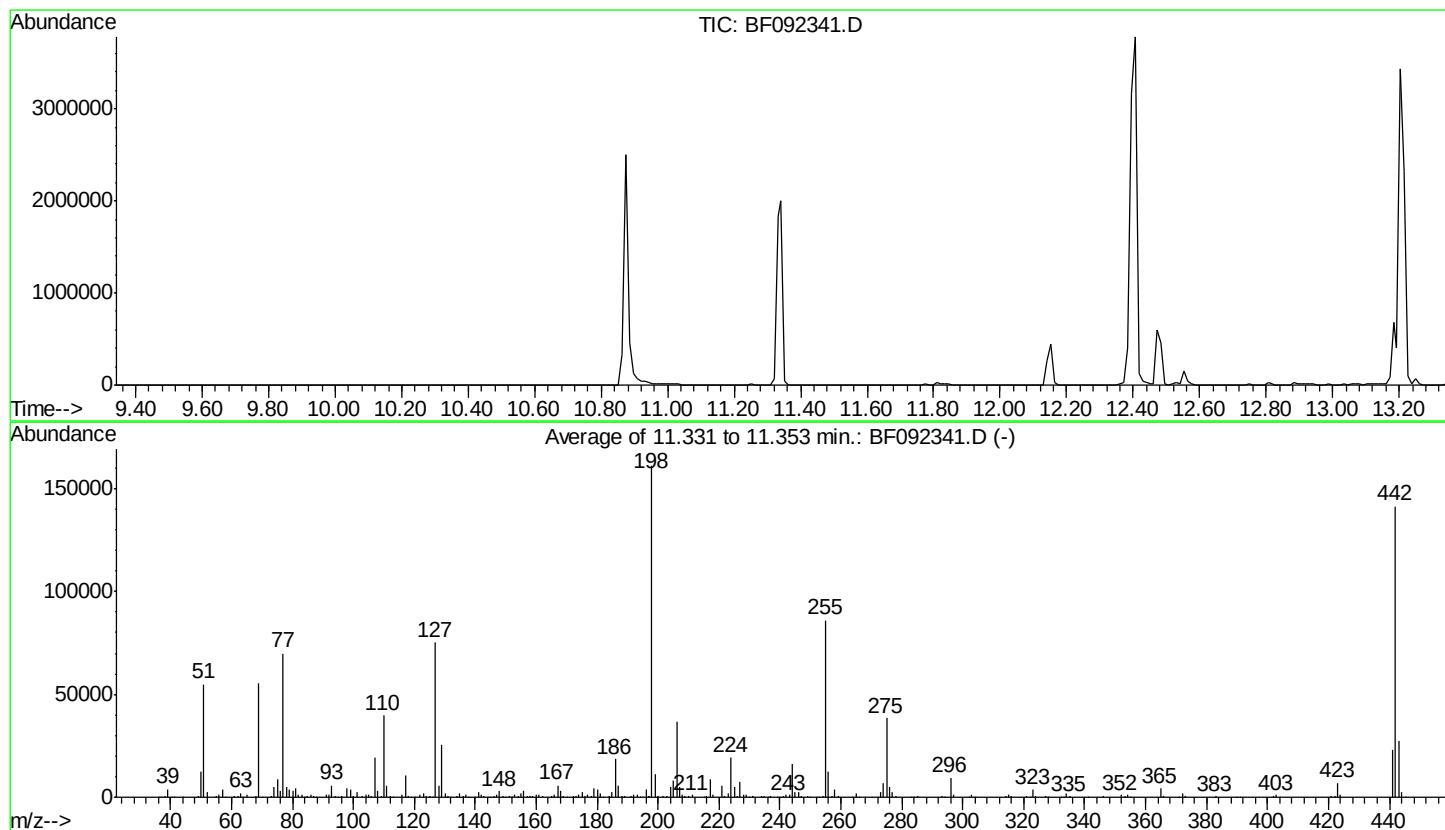

AutoFind: Scans 835, 836, 837; Background Corrected with Scan 831

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.1	54918	PASS
68	69	0.00	2	1.5	838	PASS
69	198	0.00	100	34.5	55659	PASS
70	69	0.00	2	0.4	205	PASS
127	198	10	80	46.7	75216	PASS
197	198	0.00	2	0.5	849	PASS
198	198	100	100	100.0	161175	PASS
199	198	5	9	6.8	10924	PASS
275	198	10	60	23.8	38340	PASS
365	198	1	100	2.6	4232	PASS
441	442	0.01	24	16.3	23094	PASS
442	198	50	100	87.8	141498	PASS
443	442	15	24	19.5	27531	PASS