
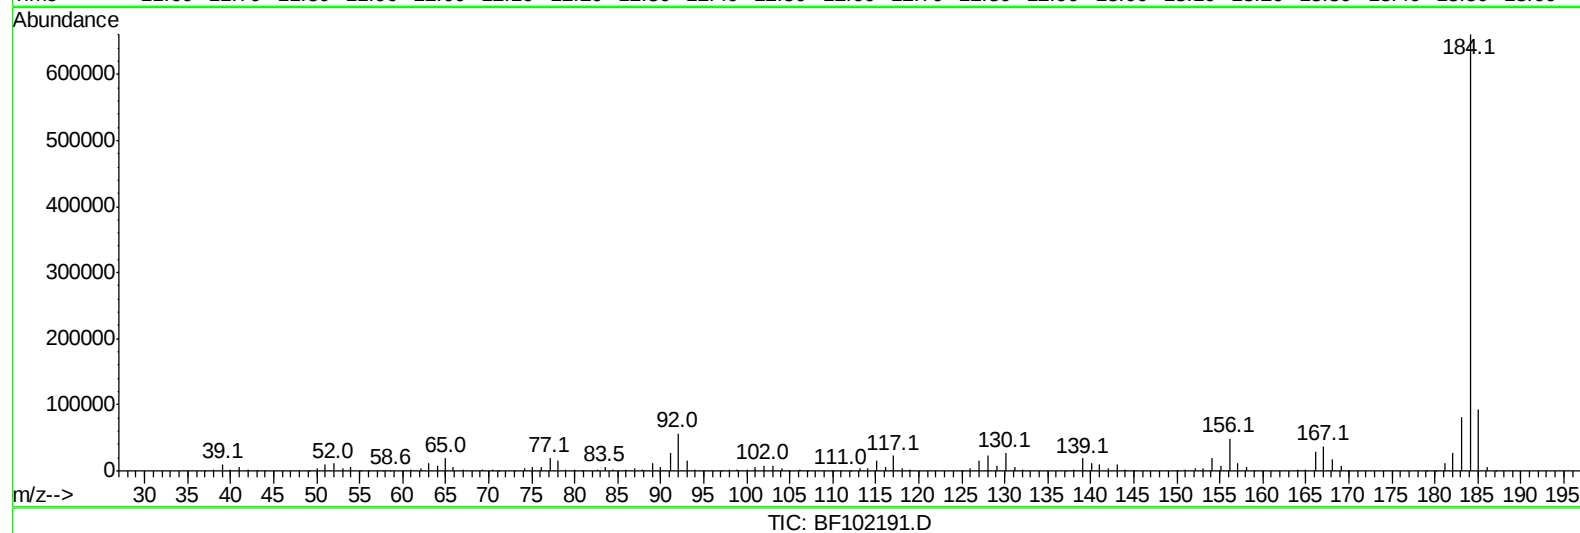


Data Path : U:\HPCHEM1\BNA F\DATA\BF011818\
Data File : BF102191.D
Acq On : 18 Jan 2018 14:39
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 19 03:17:22 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 17 15:28:18 2018
Response via : Initial Calibration

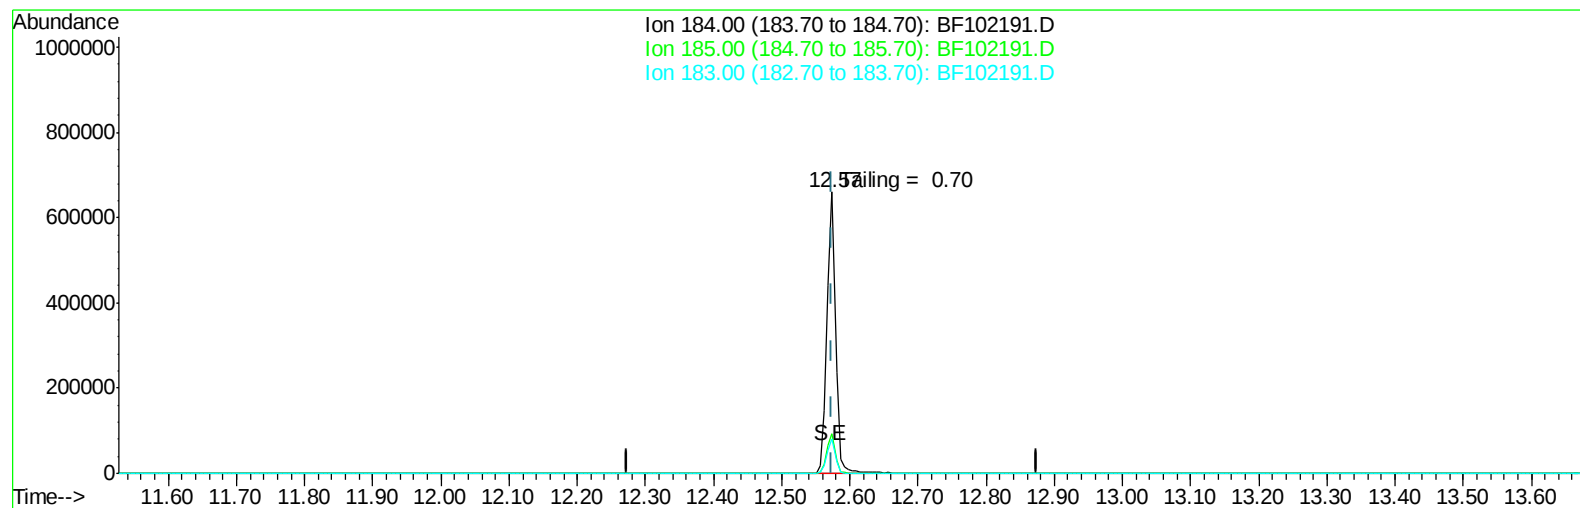

(76) Benzidine



12.574min (-0.000) 0.00ng

response 563352

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.01
183.00	11.60	12.30
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA F\DATA\BF011818\
Data File : BF102191.D
Acq On : 18 Jan 2018 14:39
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 19 03:17:22 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 17 15:28:18 2018
Response via : Initial Calibration

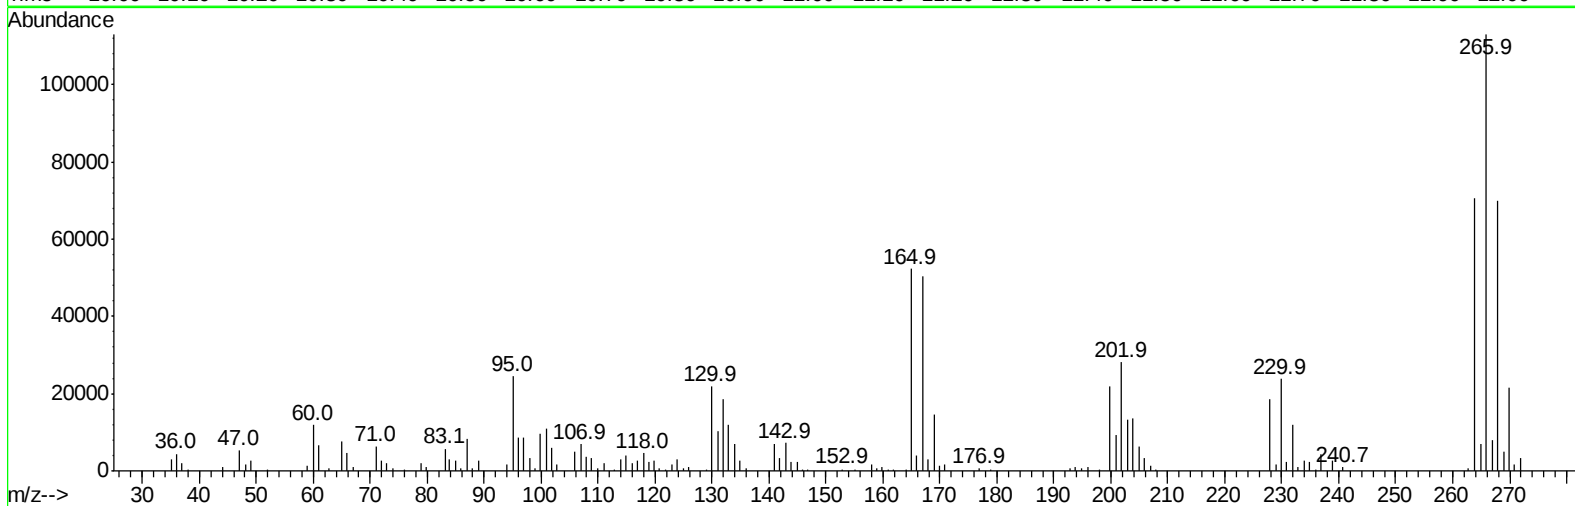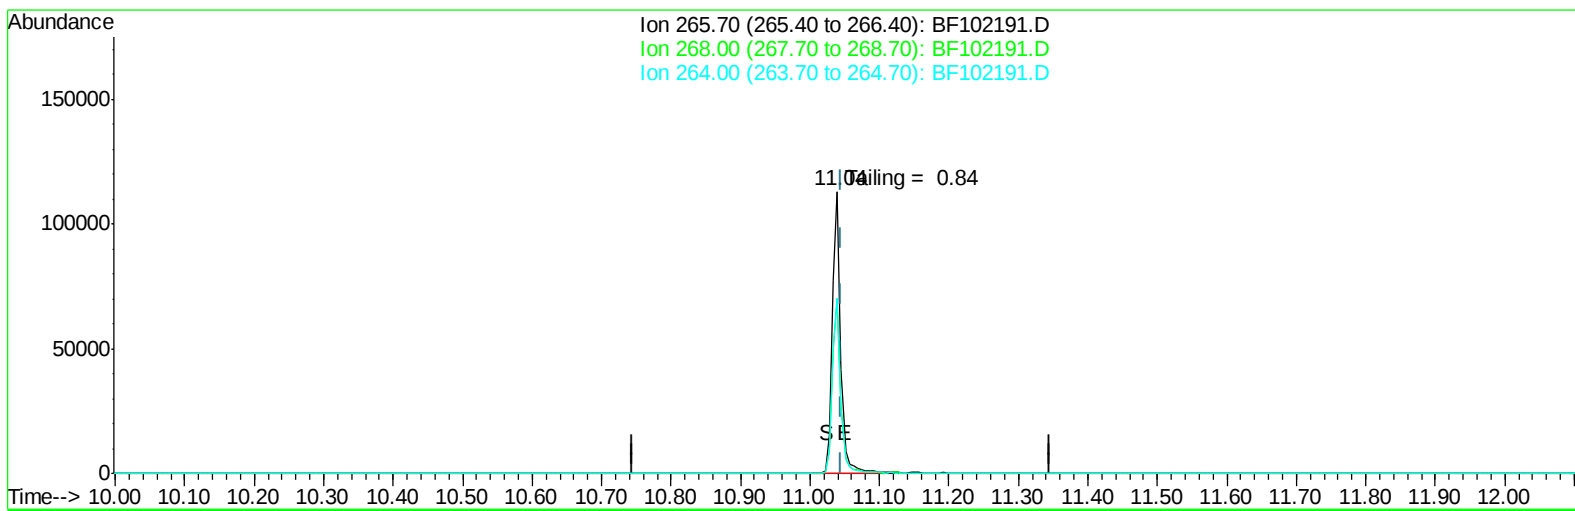

TIC: BF102191.D

(69) Pentachlorophenol (C)

11.039min (-0.006) 30680.89ng

response 95982

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.79
264.00	61.90	62.40
0.00	0.00	0.00