


Data Path : U:\HPCHEM1\BNA F\Data\BF011818\
 Data File : BF102191.D
 Acq On : 18 Jan 2018 14:39
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF010918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 17 15:28:18 2018

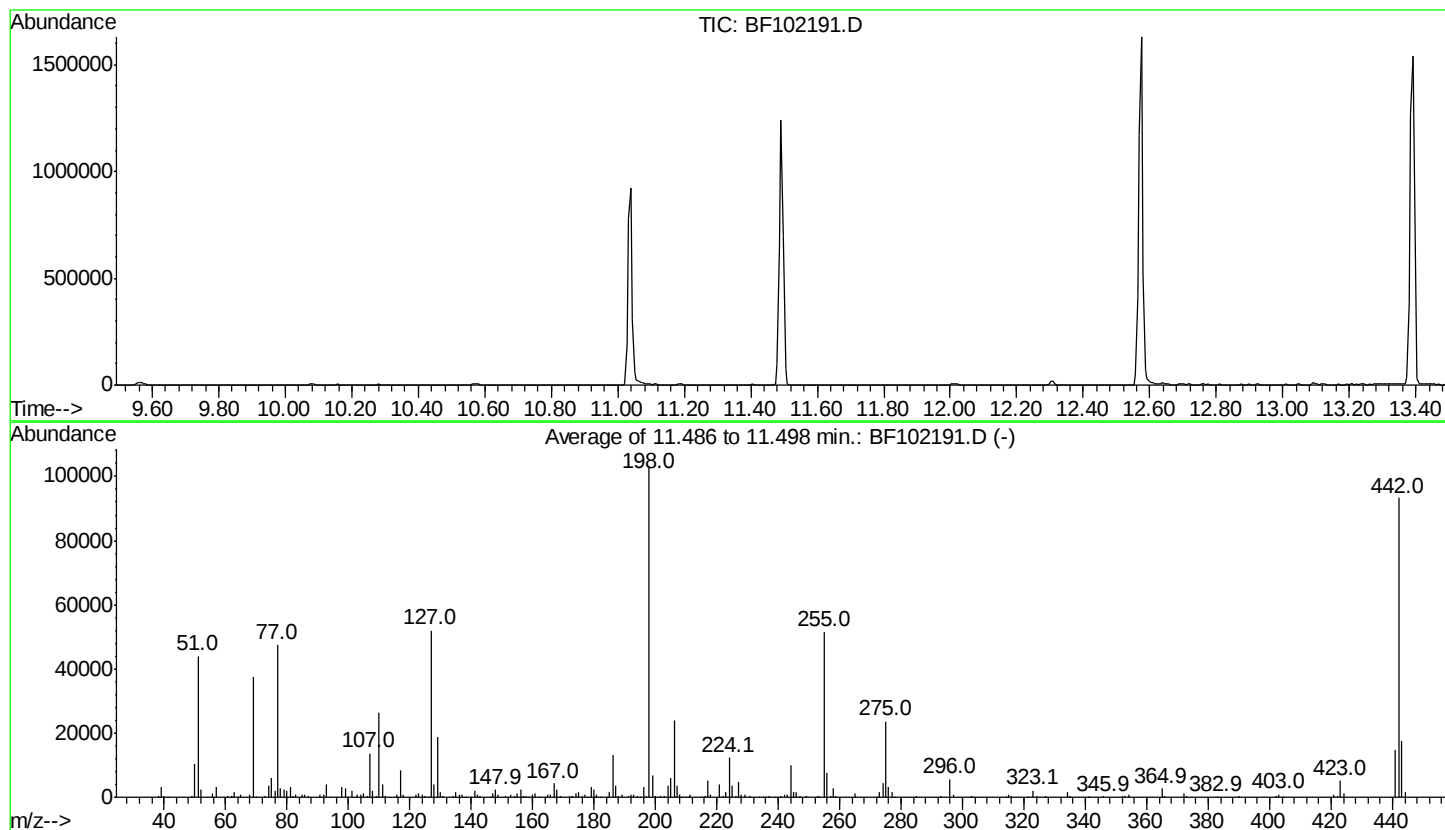

AutoFind: Scans 1598, 1599, 1600; Background Corrected with Scan 1593

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.5	43928	PASS
68	69	0.00	2	1.7	632	PASS
69	198	0.00	100	36.3	37565	PASS
70	69	0.00	2	0.4	138	PASS
127	198	10	80	50.3	51978	PASS
197	198	0.00	2	0.6	579	PASS
198	198	100	100	100.0	103378	PASS
199	198	5	9	6.5	6684	PASS
275	198	10	60	22.9	23643	PASS
365	198	1	100	2.7	2791	PASS
441	443	0.01	100	83.9	14785	PASS
442	198	50	100	90.2	93234	PASS
443	442	15	24	18.9	17613	PASS