
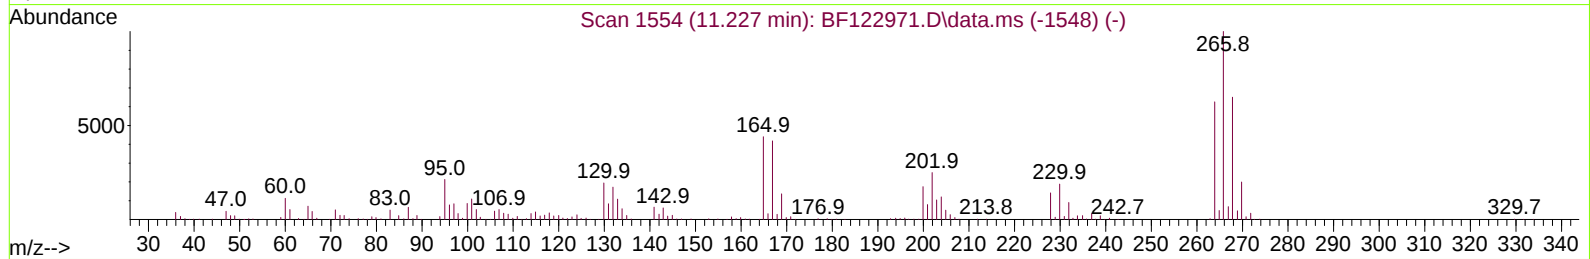
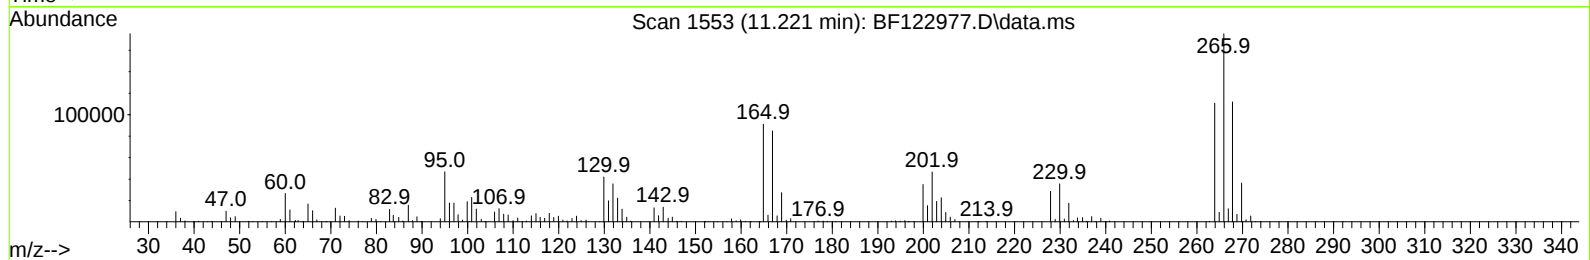


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011821\
 Data File : BF122977.D
 Acq On : 18 Jan 2021 8:44
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 19 04:41:03 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF011621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 18 13:14:08 2021
 Response via : Initial Calibration

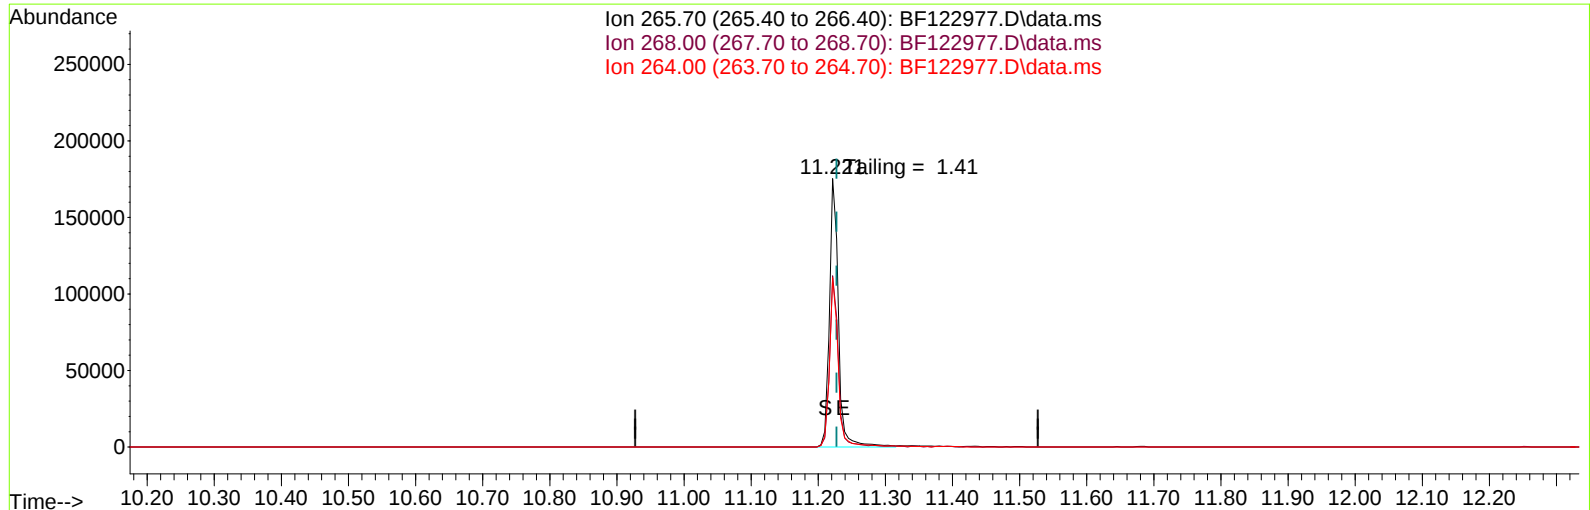

TIC: BF122977.D\data.ms

(70) Pentachlorophenol (C)




11.221min (-0.006) 132868.59 ng

response 164133

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.78
264.00	62.30	63.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011821\
 Data File : BF122977.D
 Acq On : 18 Jan 2021 8:44
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 19 04:41:03 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF011621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 18 13:14:08 2021
 Response via : Initial Calibration

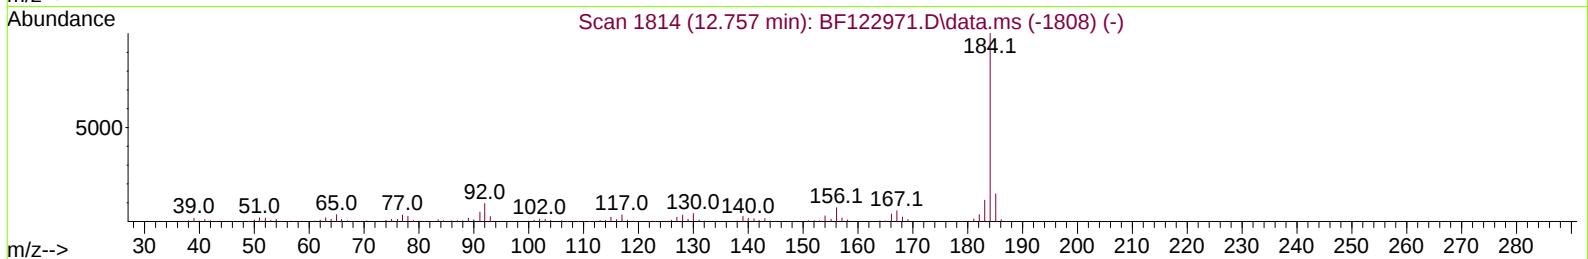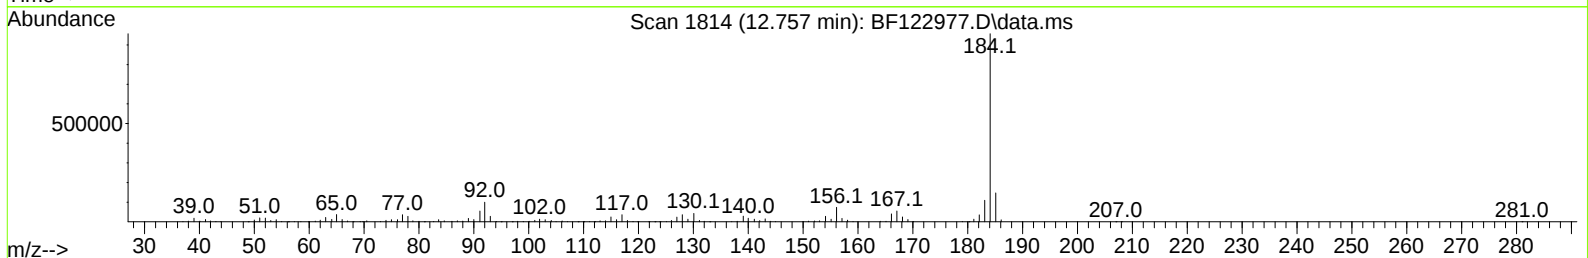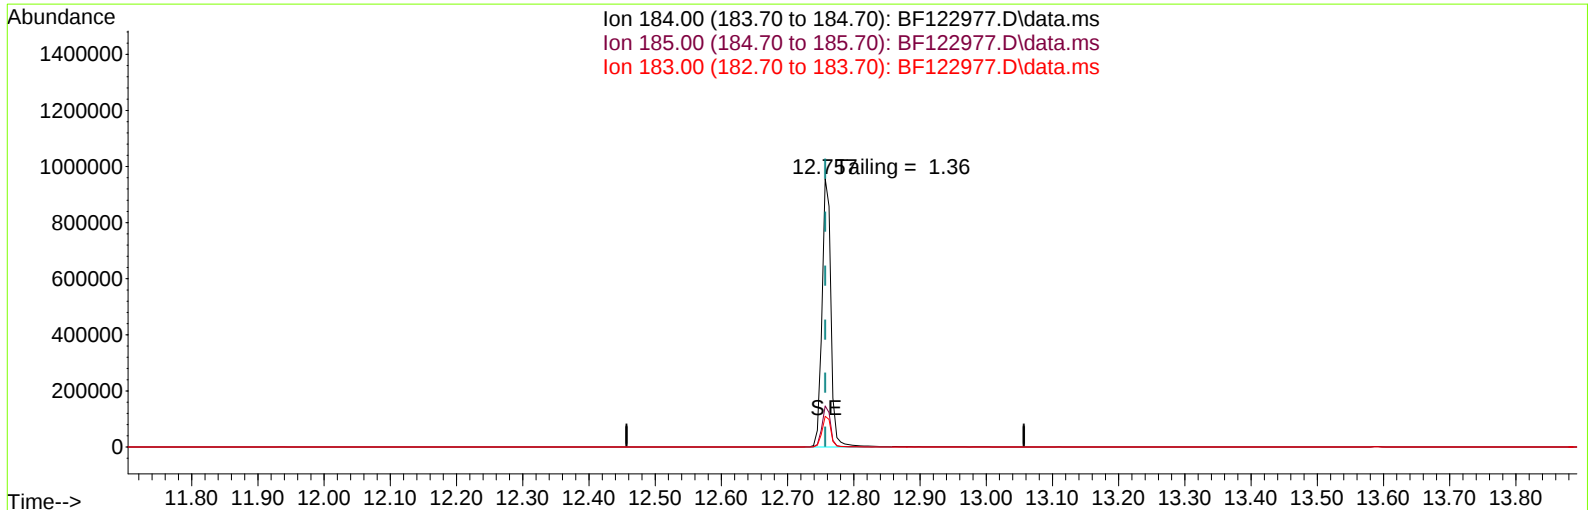

TIC: BF122977.D\data.ms

(77) Benzidine**12.757min (-0.000) 9241.07 ng****response 899031**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	15.31
183.00	12.10	11.46
0.00	0.00	0.00