
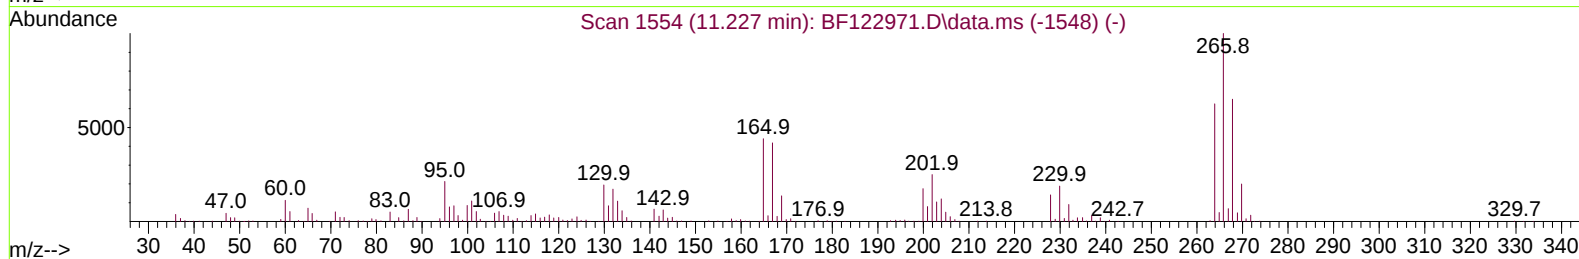
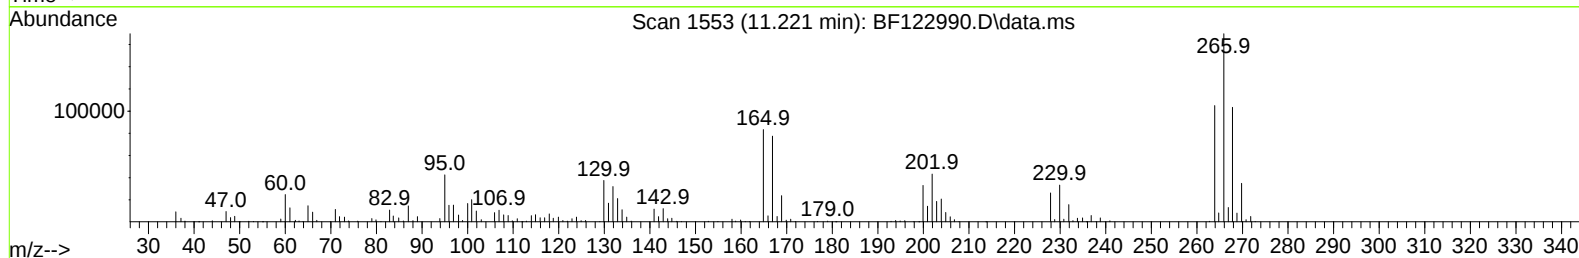


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011821\
Data File : BF122990.D
Acq On : 18 Jan 2021 16:17
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 19 04:49:18 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF011621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 18 13:14:08 2021
Response via : Initial Calibration

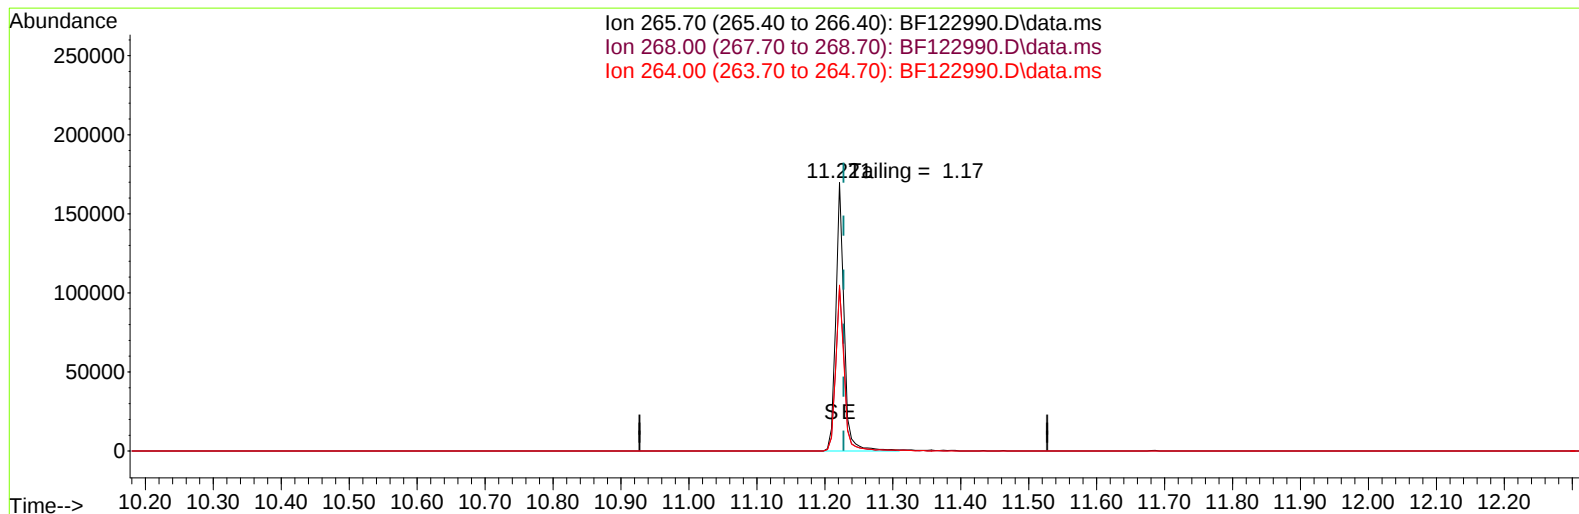

TIC: BF122990.D\data.ms

(70) Pentachlorophenol (C)




11.221min (-0.006) 53704.41 ng

response 144924

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	60.92
264.00	62.30	61.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011821\
Data File : BF122990.D
Acq On : 18 Jan 2021 16:17
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 19 04:49:18 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF011621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 18 13:14:08 2021
Response via : Initial Calibration

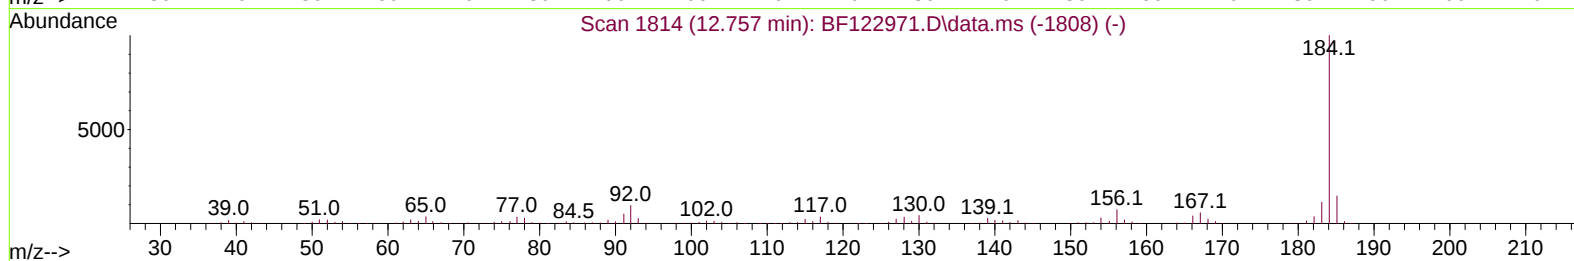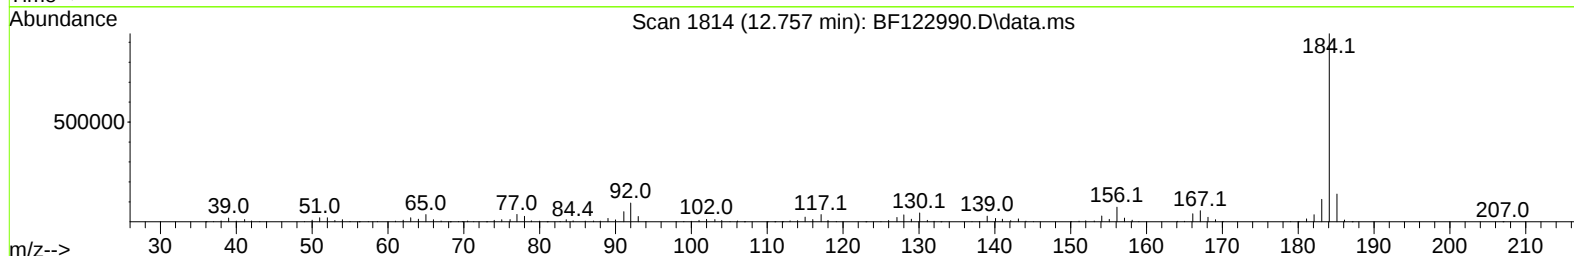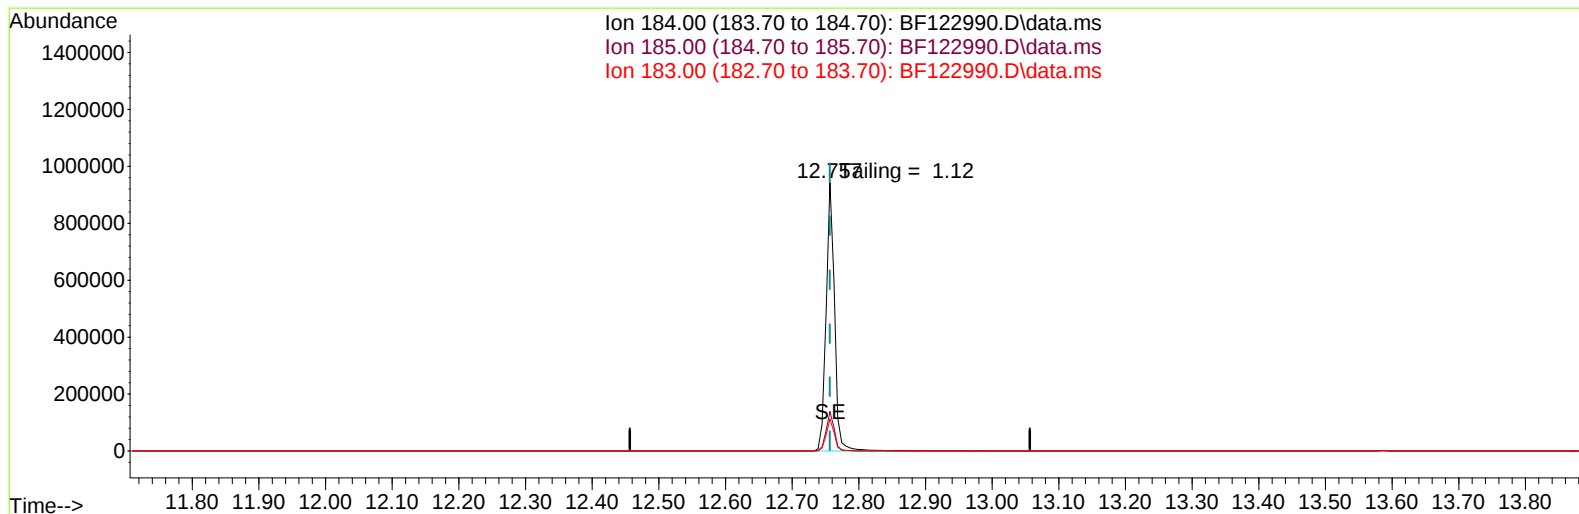

TIC: BF122990.D\data.ms

(77) Benzidine

12.757min (-0.000) 0.00 ng

response 829356

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.72
183.00	12.10	11.96
0.00	0.00	0.00