

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011821\
 Data File : BF122983.D
 Acq On : 18 Jan 2021 12:22
 Operator : JU/CG
 Sample : M1100-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TOPSOIL-RBF-DARK

Quant Time: Jan 18 13:29:33 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF011621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 18 13:14:08 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.892	152	177446	20.00	ng	0.00
21) Naphthalene-d8	8.175	136	625144	20.00	ng	# 0.00
39) Acenaphthene-d10	9.933	164	296591	20.00	ng	0.00
64) Phenanthrene-d10	11.421	188	381794	20.00	ng	# 0.00
76) Chrysene-d12	14.062	240	306442	20.00	ng	#-0.01
86) Perylene-d12	15.545	264	282324	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.516	112	718812	61.23	ng	0.00
7) Phenol-d6	6.516	99	1505912	95.45	ng	0.00
23) Nitrobenzene-d5	7.451	82	1085797	89.38	ng	-0.01
42) 2,4,6-Tribromophenol	10.722	330	251515	74.99	ng	0.00
45) 2-Fluorobiphenyl	9.257	172	1414334	66.77	ng	0.00
79) Terphenyl-d14	13.015	244	1289935	77.18	ng	0.00
Target Compounds						Qvalue
10) Phenol	6.528	94	63829	4.03	ng	91
50) Dimethylphthalate	9.645	163	243107	10.56	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011821\
Data File : BF122983.D
Acq On : 18 Jan 2021 12:22
Operator : JU/CG
Sample : M1100-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TOPSOIL-RBF-DARK

Quant Time: Jan 18 13:29:33 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF011621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 18 13:14:08 2021
Response via : Initial Calibration




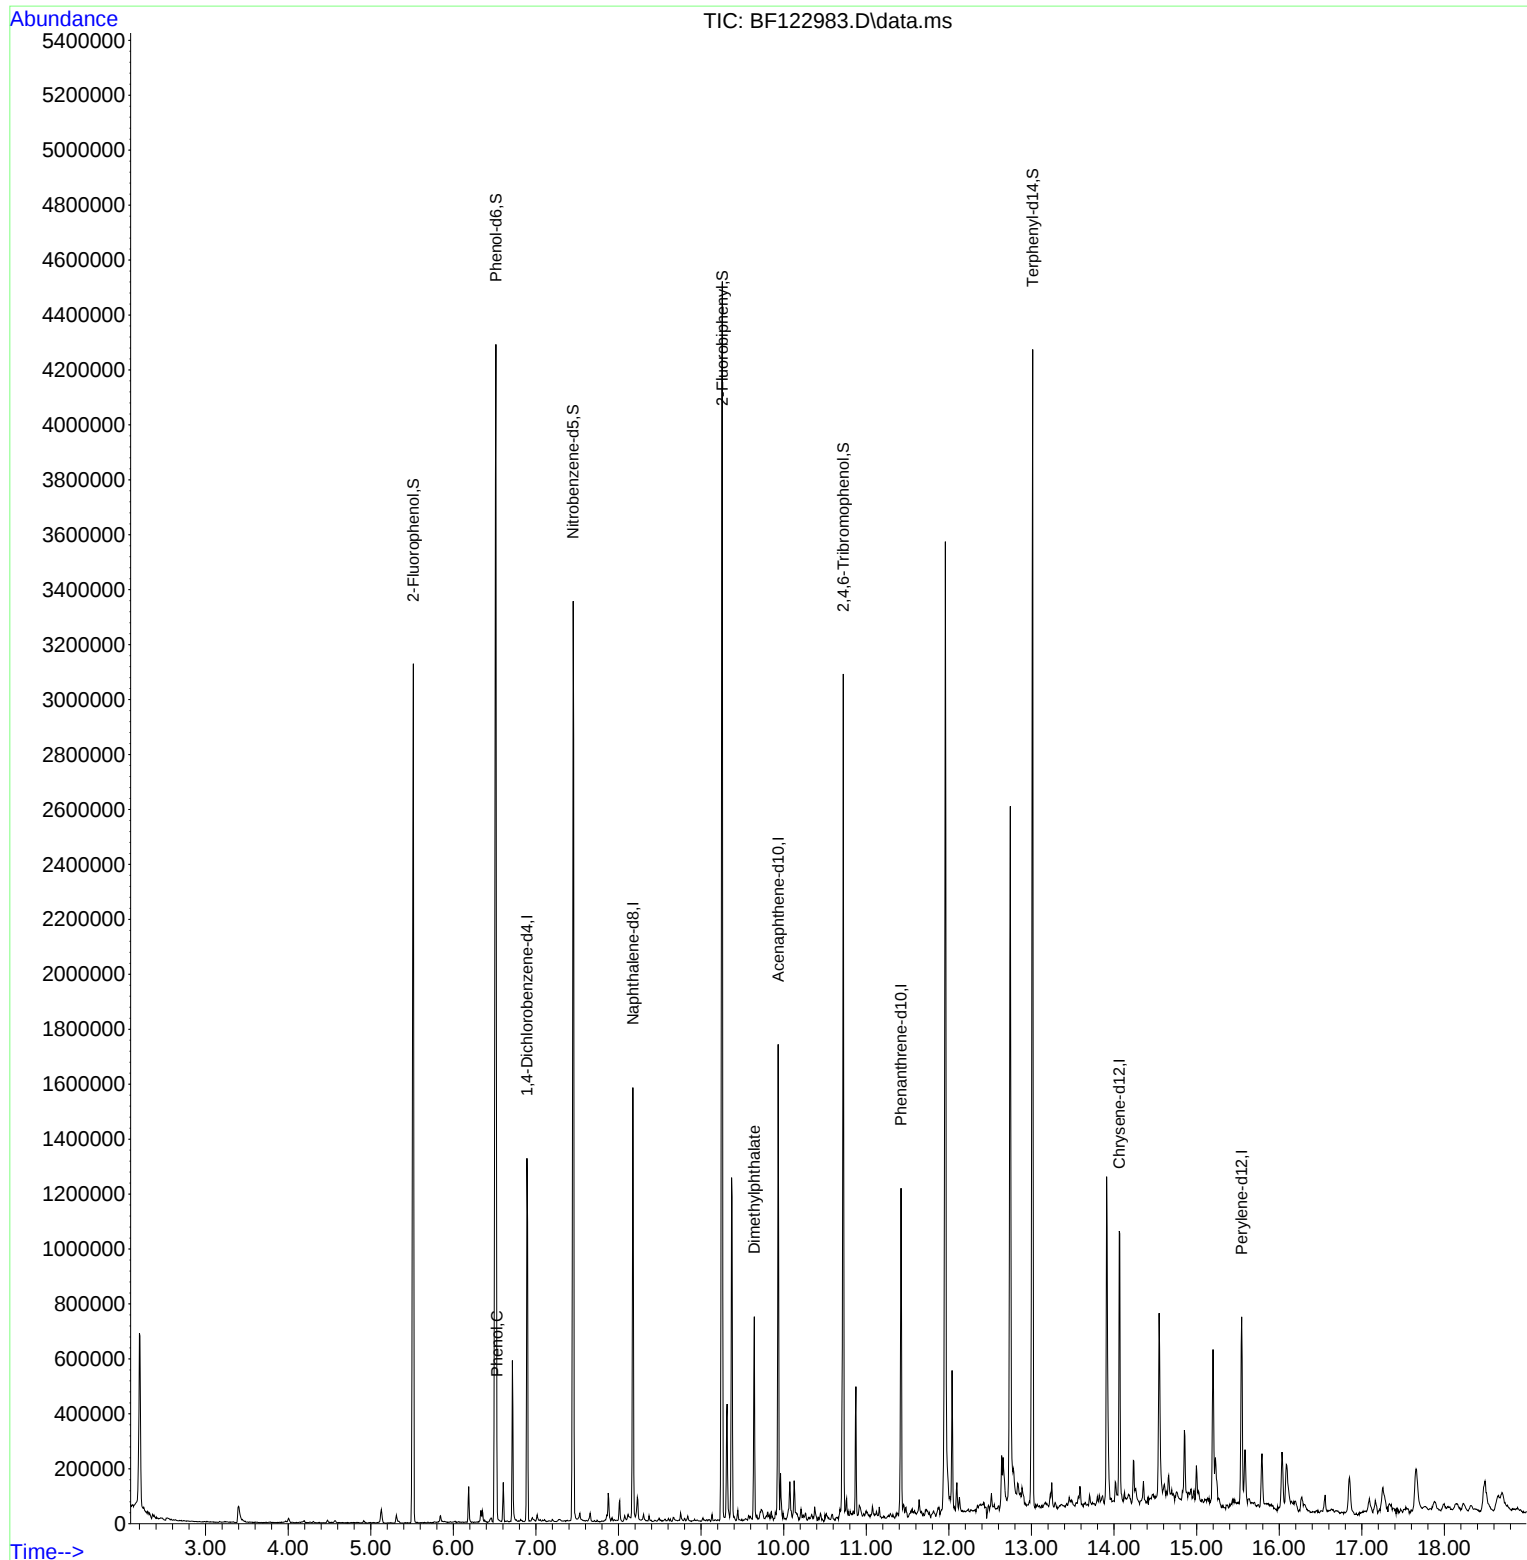


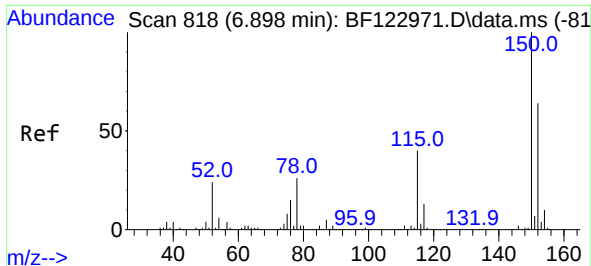

#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.892 min Scan# 817
Delta R.T. -0.006 min
Lab File: BF122983.D
Acq: 18 Jan 2021 12:22




Instrument :
BNA_F
ClientSampleId :
TOPSOIL-RBF-DARK


Tgt Ion:152 Resp: 177446
Ion Ratio Lower Upper
152 100
150 155.5 125.8 188.6
115 66.8 49.3 73.9

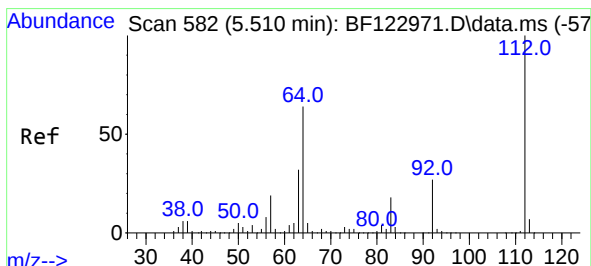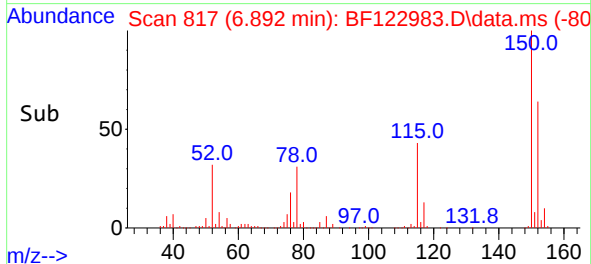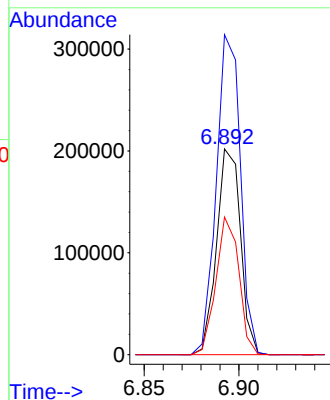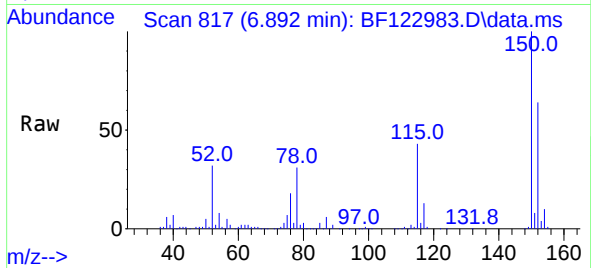

#5
2-Fluorophenol
Concen: 61.23 ng
RT: 5.516 min Scan# 583
Delta R.T. 0.006 min
Lab File: BF122983.D
Acq: 18 Jan 2021 12:22

Tgt Ion:112 Resp: 718812
Ion Ratio Lower Upper
112 100
64 81.4 46.9 70.3#
63 43.6 24.5 36.7#


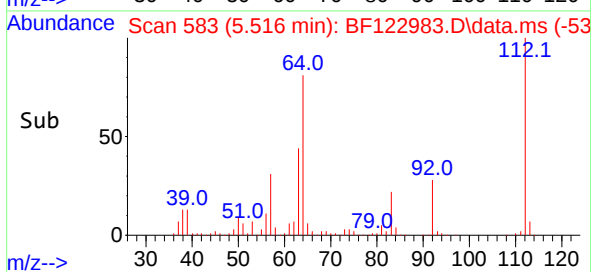
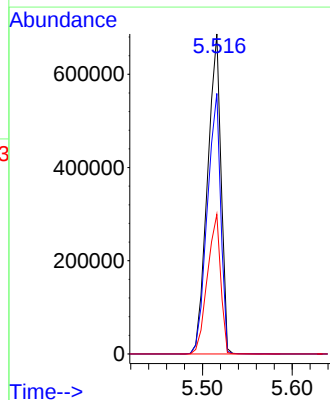
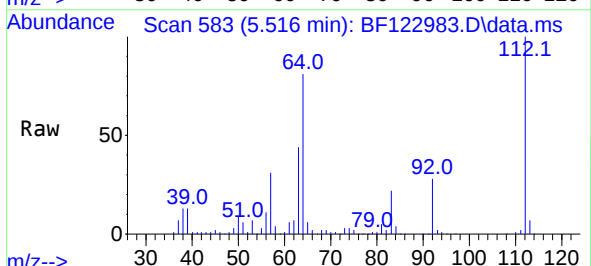


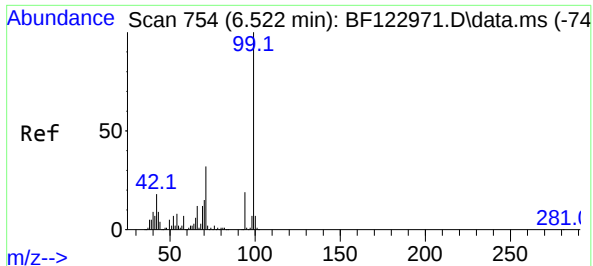

#7
Phenol-d6
Concen: 95.45 ng
RT: 6.516 min Scan# 753
Delta R.T. -0.006 min
Lab File: BF122983.D
Acq: 18 Jan 2021 12:22




Instrument :
BNA_F
ClientSampleId :
TOPSOIL-RBF-DARK


Tgt Ion: 99 Resp: 1505912
Ion Ratio Lower Upper
99 100
42 29.2 13.8 20.6#
71 37.3 26.9 40.3

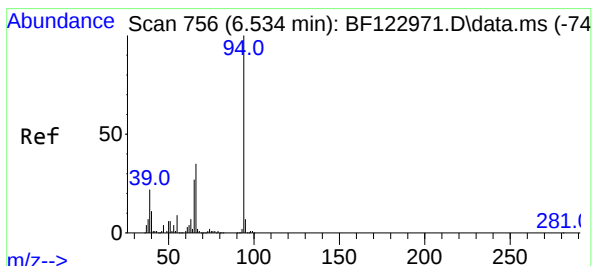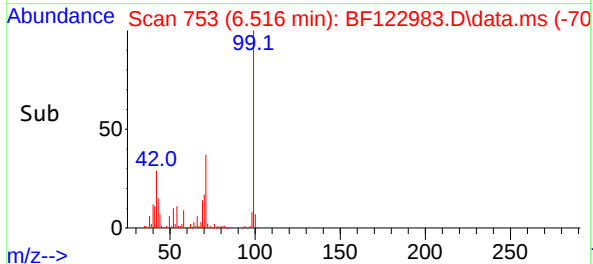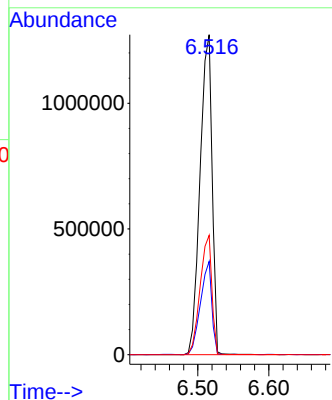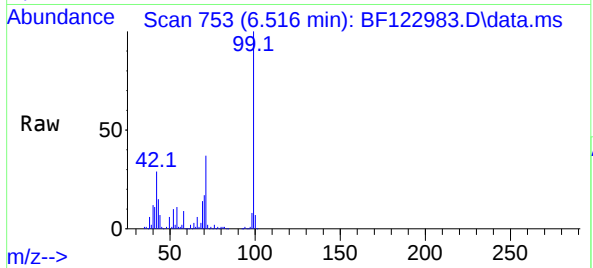

#10
Phenol
Concen: 4.03 ng
RT: 6.528 min Scan# 755
Delta R.T. -0.006 min
Lab File: BF122983.D
Acq: 18 Jan 2021 12:22

Tgt Ion: 94 Resp: 63829
Ion Ratio Lower Upper
94 100
65 29.7 11.2 51.2
66 37.0 25.8 65.8

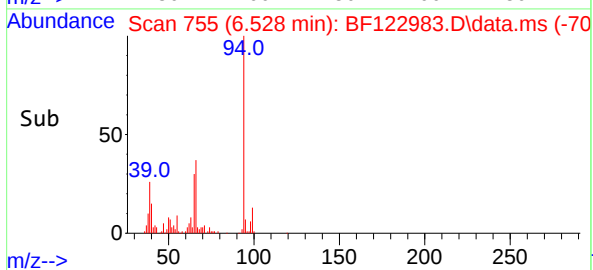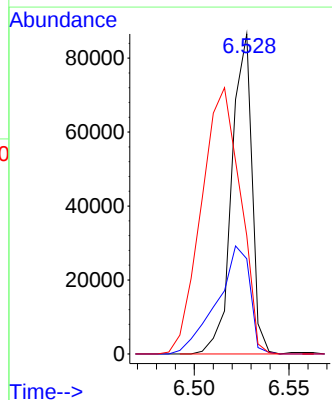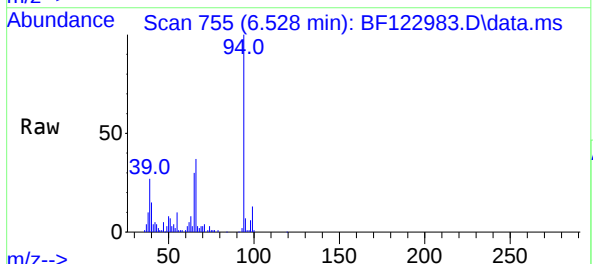




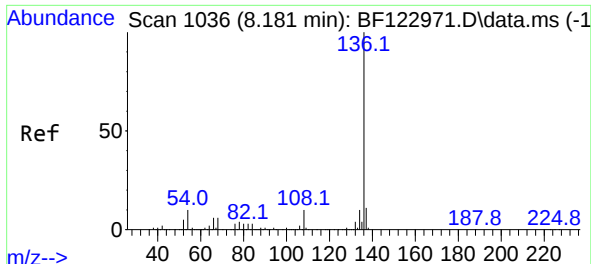


#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.175 min Scan# 1035
Delta R.T. -0.006 min
Lab File: BF122983.D
Acq: 18 Jan 2021 12:22

Instrument :
BNA_F
ClientSampleId :
TOPSOIL-RBF-DARK

Tgt Ion:136 Resp: 625144




Ion	Ratio	Lower	Upper
136	100		
137	10.7	8.8	13.2
54	12.1	5.5	8.3#
68	7.4	4.6	6.8#

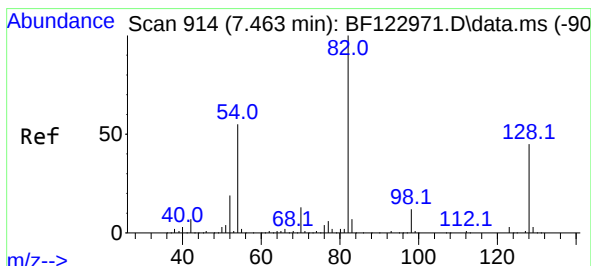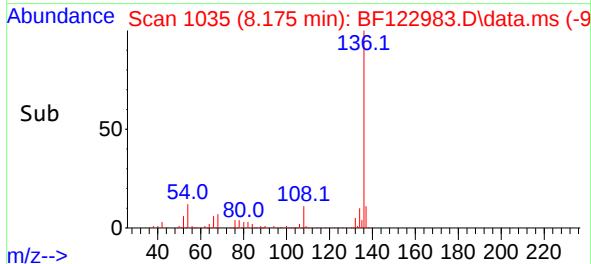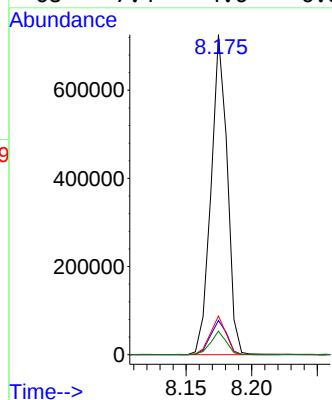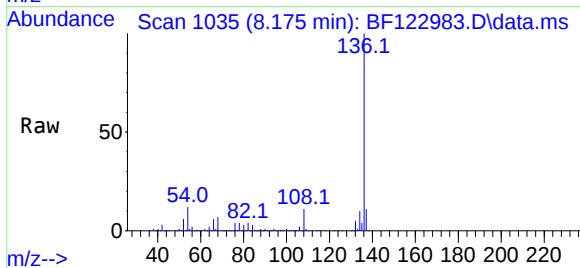


#23
Nitrobenzene-d5
Concen: 89.38 ng
RT: 7.451 min Scan# 912
Delta R.T. -0.012 min
Lab File: BF122983.D
Acq: 18 Jan 2021 12:22

Tgt Ion: 82 Resp: 1085797

Ion	Ratio	Lower	Upper
82	100		
128	41.3	37.0	55.4
54	63.9	38.4	57.6#


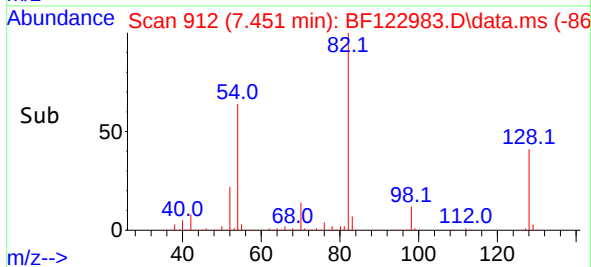
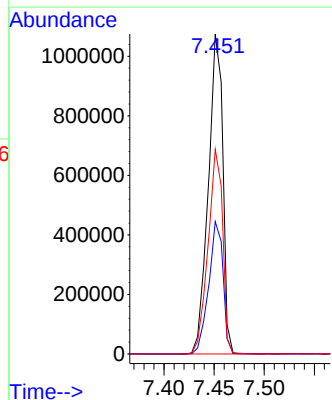
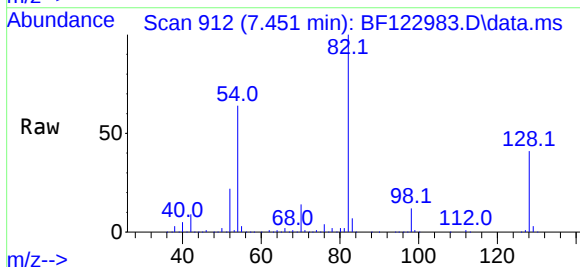


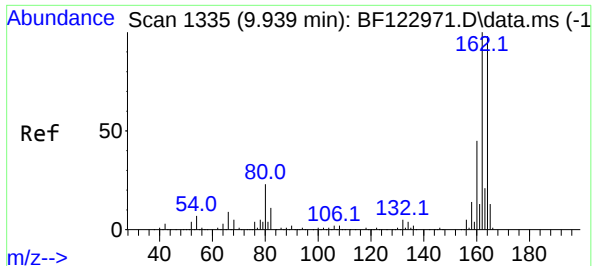

#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.933 min Scan# 1334
Delta R.T. -0.006 min
Lab File: BF122983.D
Acq: 18 Jan 2021 12:22




Instrument :
BNA_F
ClientSampleId :
TOPSOIL-RBF-DARK


Tgt Ion:164 Resp: 296591
Ion Ratio Lower Upper
164 100
162 103.3 80.8 121.2
160 45.4 35.4 53.0

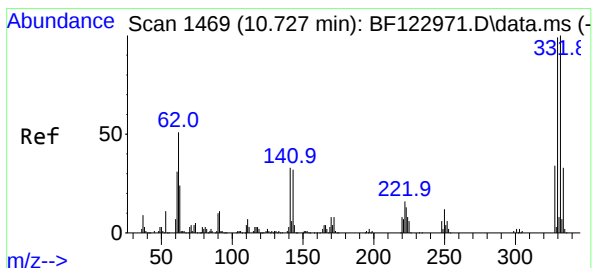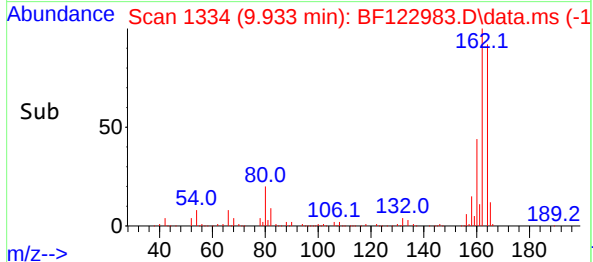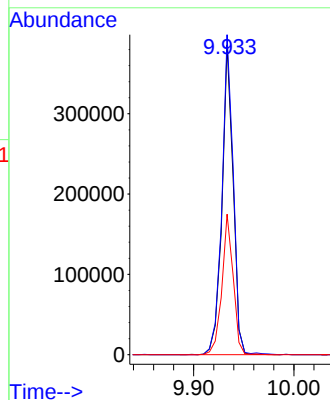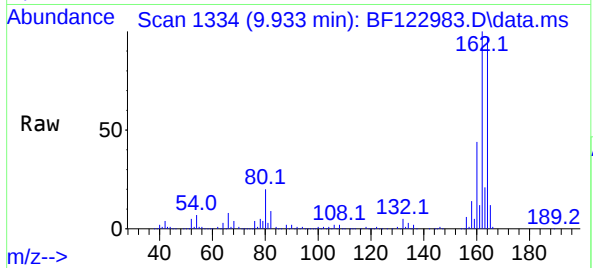

#42
2,4,6-Tribromophenol
Concen: 74.99 ng
RT: 10.722 min Scan# 1468
Delta R.T. -0.005 min
Lab File: BF122983.D
Acq: 18 Jan 2021 12:22

Tgt Ion:330 Resp: 251515
Ion Ratio Lower Upper
330 100
332 100.8 77.5 116.3
141 45.0 23.8 35.8#


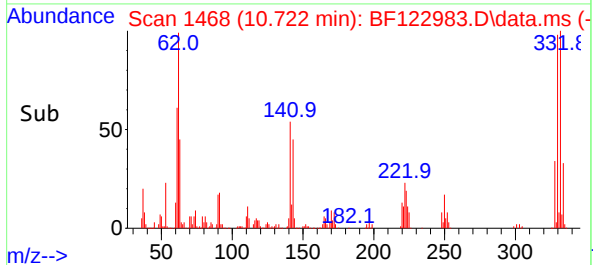
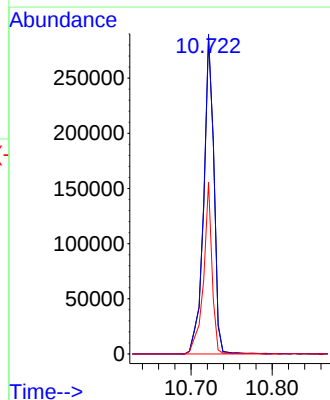
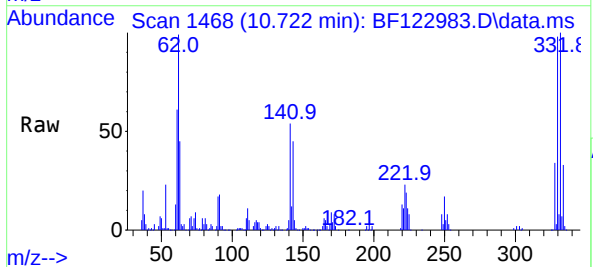


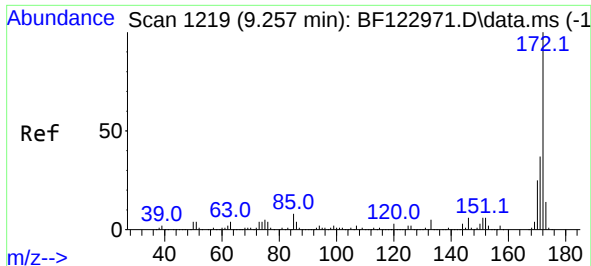

#45
2-Fluorobiphenyl
Concen: 66.77 ng
RT: 9.257 min Scan# 1219
Delta R.T. -0.000 min
Lab File: BF122983.D
Acq: 18 Jan 2021 12:22




Instrument :
BNA_F
ClientSampleId :
TOPSOIL-RBF-DARK


Tgt Ion:172 Resp: 1414334
Ion Ratio Lower Upper
172 100
171 35.8 29.6 44.4
170 24.4 19.5 29.3

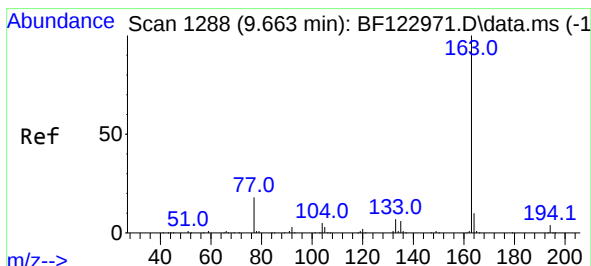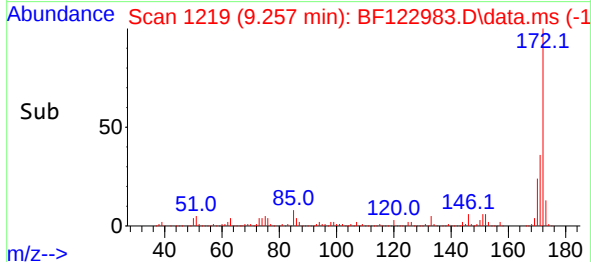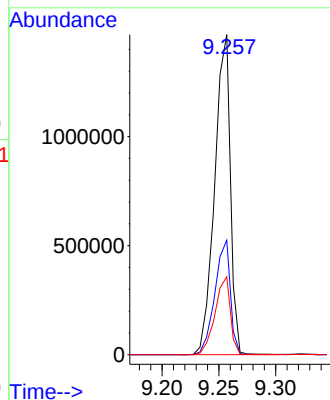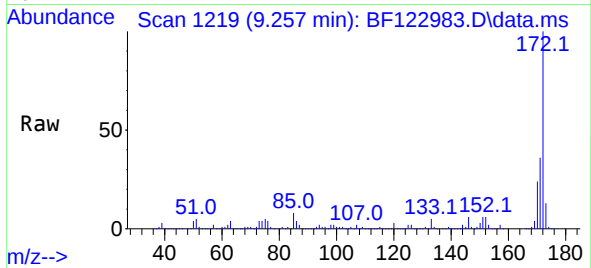

#50
Dimethylphthalate
Concen: 10.56 ng
RT: 9.645 min Scan# 1285
Delta R.T. -0.018 min
Lab File: BF122983.D
Acq: 18 Jan 2021 12:22

Tgt Ion:163 Resp: 243107
Ion Ratio Lower Upper
163 100
194 3.7 3.4 5.0
164 10.0 8.1 12.1


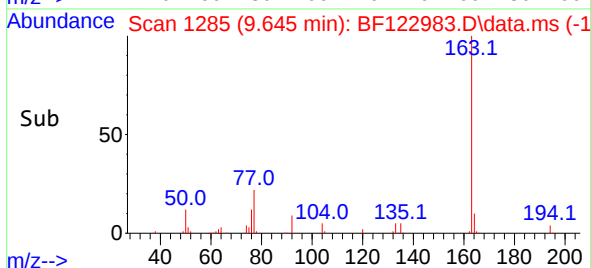
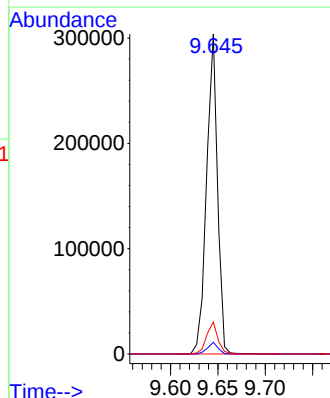
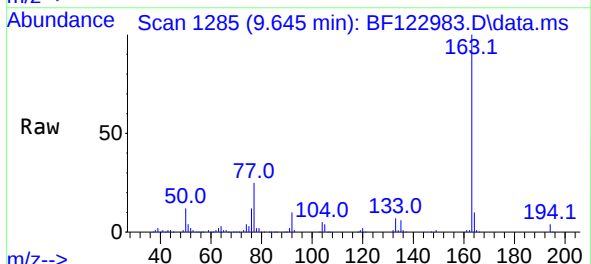


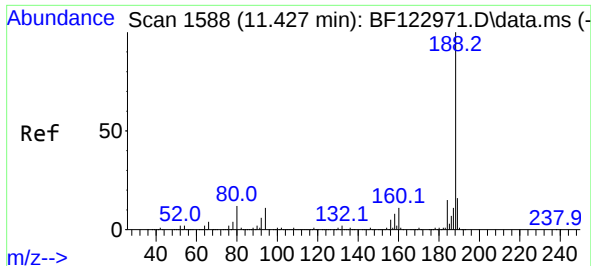

#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.421 min Scan# 1587
Delta R.T. -0.006 min
Lab File: BF122983.D
Acq: 18 Jan 2021 12:22




Instrument :
BNA_F
ClientSampleId :
TOPSOIL-RBF-DARK


Tgt Ion:188 Resp: 381794
Ion Ratio Lower Upper
188 100
94 12.6 7.4 11.2#
80 15.4 8.2 12.4#

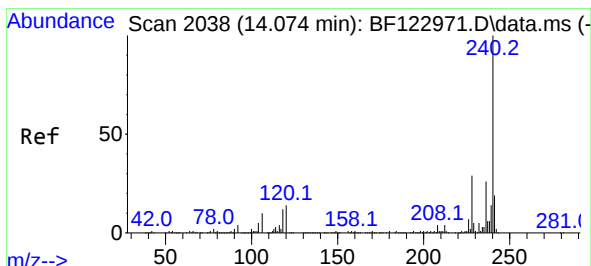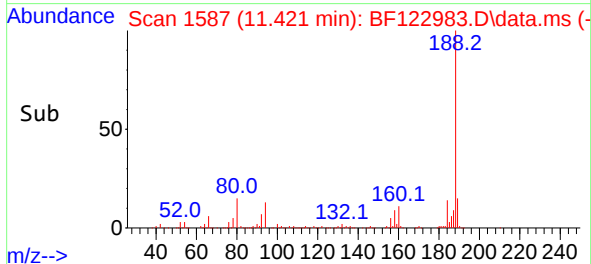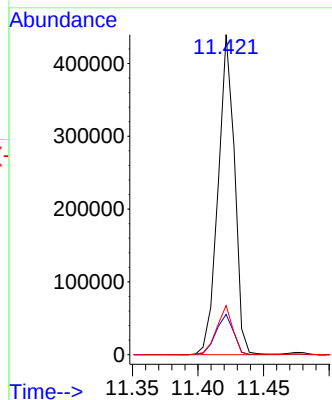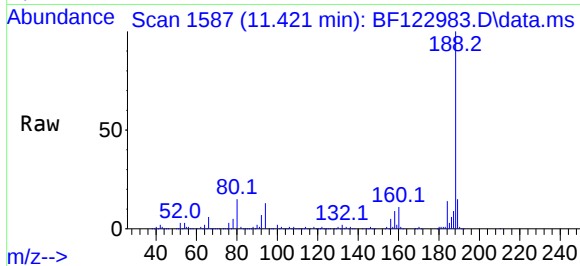

#76
Chrysene-d12
Concen: 20.00 ng
RT: 14.062 min Scan# 2036
Delta R.T. -0.012 min
Lab File: BF122983.D
Acq: 18 Jan 2021 12:22

Tgt Ion:240 Resp: 306442
Ion Ratio Lower Upper
240 100
120 15.7 8.6 12.8#
236 26.1 20.3 30.5


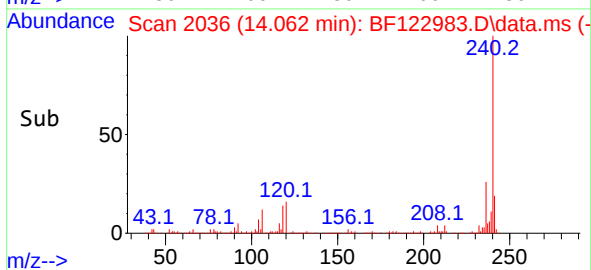
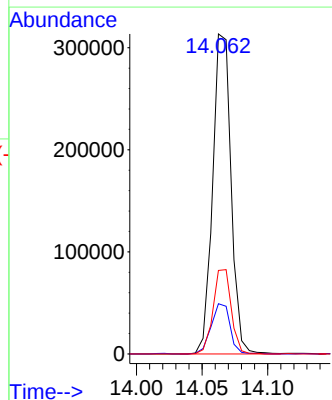
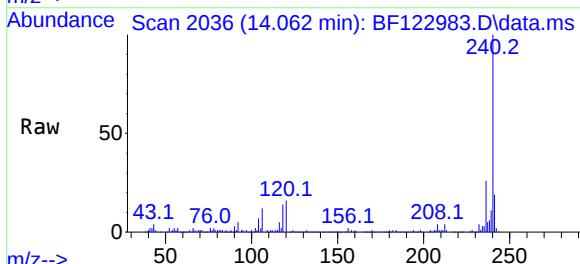


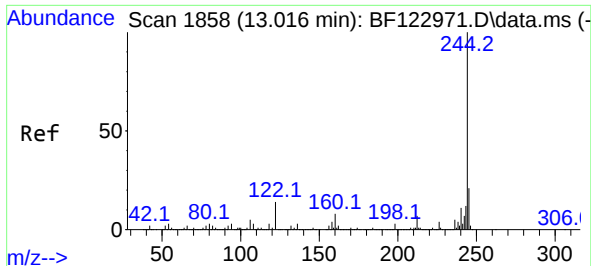

#79
Terphenyl-d14
Concen: 77.18 ng
RT: 13.015 min Scan# 1858
Delta R.T. -0.001 min
Lab File: BF122983.D
Acq: 18 Jan 2021 12:22

Instrument :
BNA_F
ClientSampleId :
TOPSOIL-RBF-DARK

Tgt Ion:244 Resp: 1289935
Ion Ratio Lower Upper
244 100
212 7.2 5.7 8.5
122 13.3 8.3 12.5#

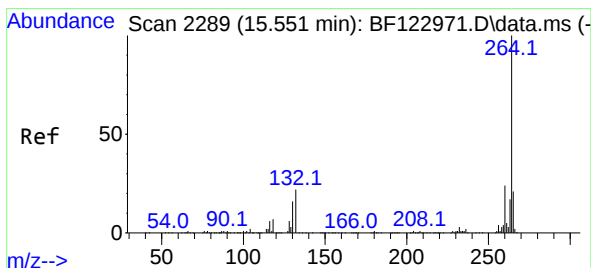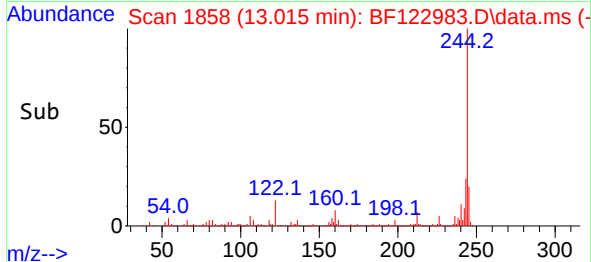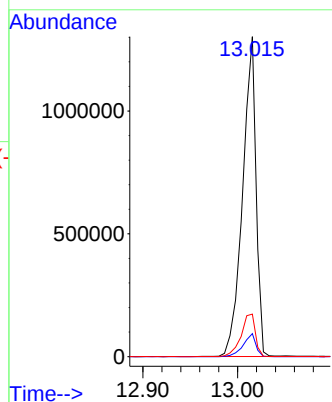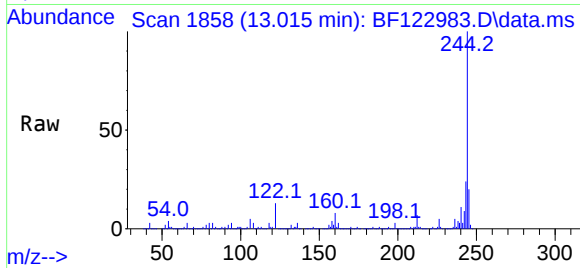

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.545 min Scan# 2288
Delta R.T. -0.006 min
Lab File: BF122983.D
Acq: 18 Jan 2021 12:22

Tgt Ion:264 Resp: 282324
Ion Ratio Lower Upper
264 100
260 24.5 18.6 28.0
265 21.7 17.0 25.6

