

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011821\
 Data File : BF122980.D
 Acq On : 18 Jan 2021 10:18
 Operator : JU/CG
 Sample : PB134164BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB134164BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF011621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122980.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.522	578	584	587	rBV	7580667	8056067	84.16%	13.220%
2	6.516	747	753	756	rBV	6877511	8051074	84.11%	13.212%
3	6.892	814	817	821	rVB	2017758	1780464	18.60%	2.922%
4	7.457	907	913	916	rBV	4899511	5262045	54.97%	8.635%
5	8.175	1030	1035	1039	rBV	2486489	2474713	25.85%	4.061%
6	9.257	1213	1219	1222	rBV	8651518	9230525	96.43%	15.148%
7	9.933	1328	1334	1338	rBV	2958315	2813602	29.39%	4.617%
8	10.722	1462	1468	1472	rBV	5561839	6213170	64.91%	10.196%
9	11.422	1582	1587	1591	rBV	3078204	2750317	28.73%	4.513%
10	13.021	1851	1859	1862	rBV	8708818	9572422	100.00%	15.709%
11	14.068	2032	2037	2049	rBV	2745222	2435849	25.45%	3.997%
12	15.545	2282	2288	2304	rBV	1774630	2296253	23.99%	3.768%




Sum of corrected areas: 60936501

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011821\
Data File : BF122980.D
Acq On : 18 Jan 2021 10:18
Operator : JU/CG
Sample : PB134164BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB134164BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF011621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

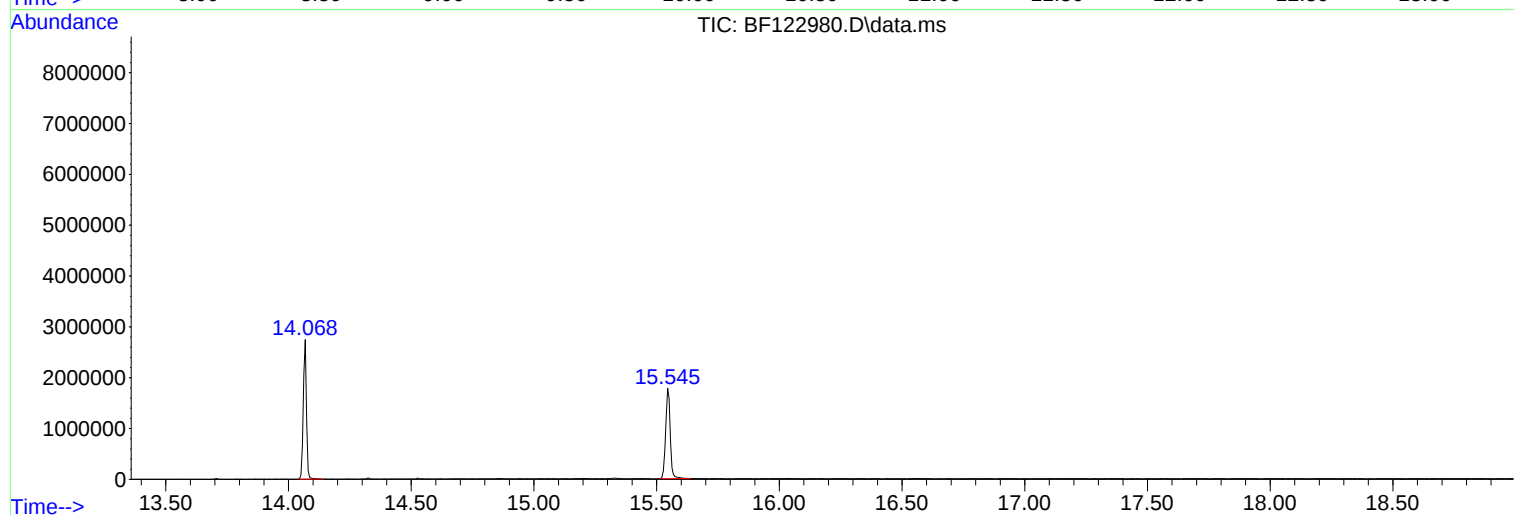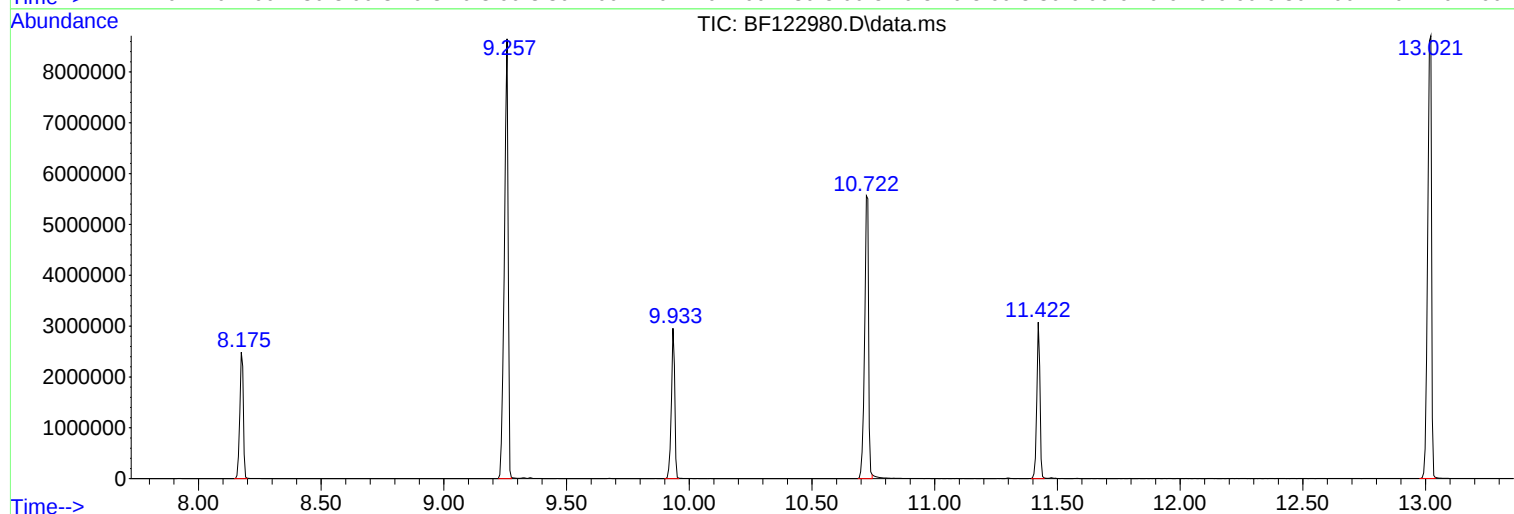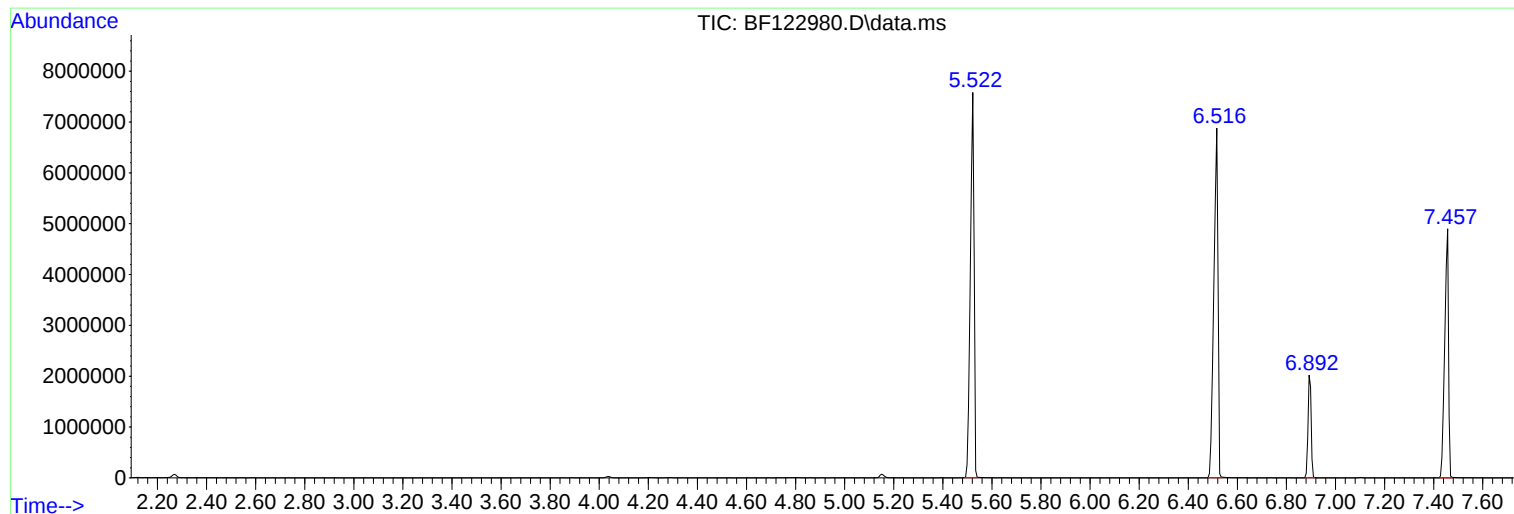

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011821\
Data File : BF122980.D
Acq On : 18 Jan 2021 10:18
Operator : JU/CG
Sample : PB134164BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB134164BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF011621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011821\
Data File : BF122980.D
Acq On : 18 Jan 2021 10:18
Operator : JU/CG
Sample : PB134164BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB134164BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF011621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------