
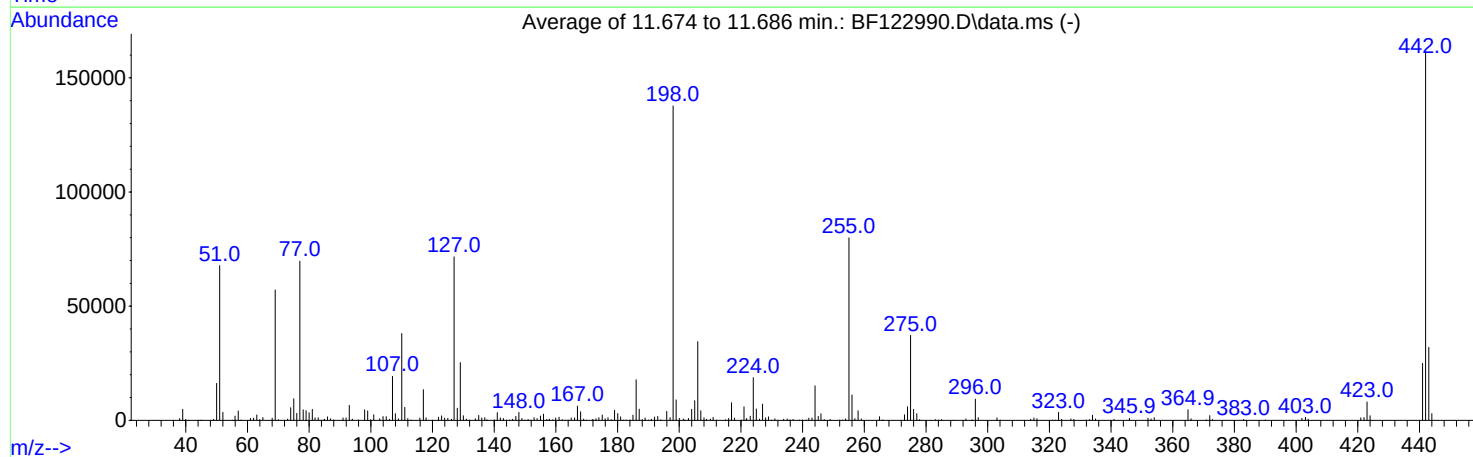


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011821\
 Data File : BF122990.D
 Acq On : 18 Jan 2021 16:17
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF011621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 18 13:14:08 2021

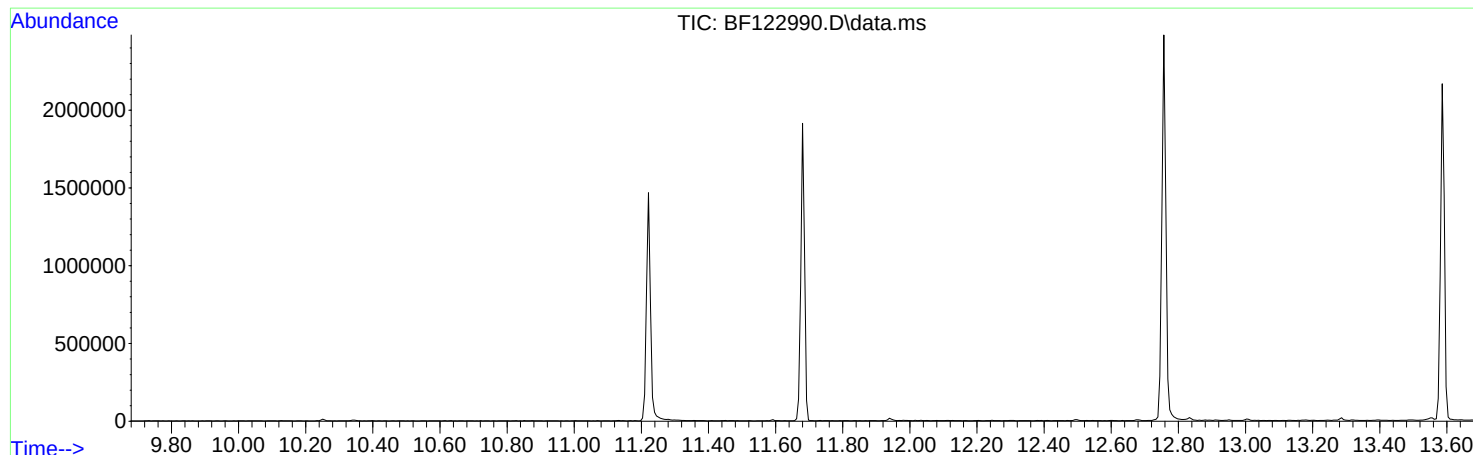

AutoFind: Scans 1630, 1631, 1632; Background Corrected with Scan 1625

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.2	67731	PASS
68	69	0.00	2	1.8	1021	PASS
69	198	0.00	100	41.5	57109	PASS
70	69	0.00	2	0.6	317	PASS
127	198	10	80	52.0	71605	PASS
197	198	0.00	2	0.9	1211	PASS
198	198	100	100	100.0	137677	PASS
199	198	5	9	6.5	9007	PASS
275	198	10	60	27.0	37203	PASS
365	198	1	100	3.4	4722	PASS
441	198	0.01	100	18.1	24972	PASS
442	442	50	100	100.0	161096	PASS
443	442	15	24	19.8	31925	PASS