
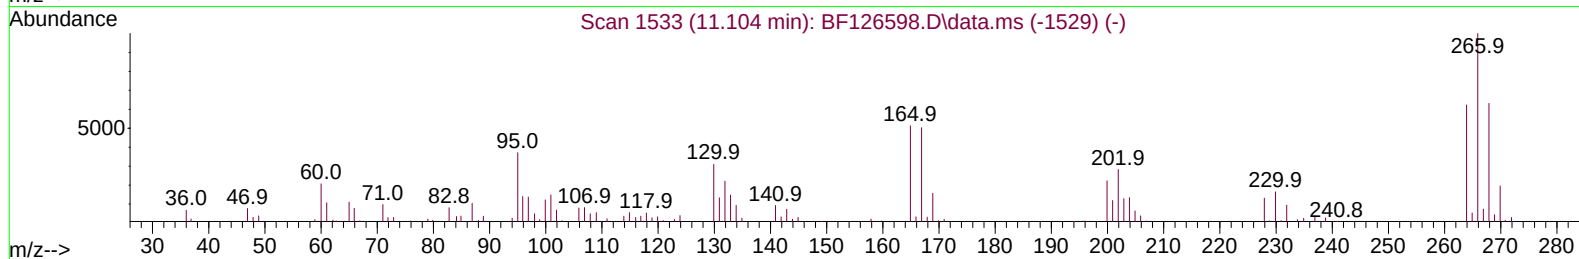
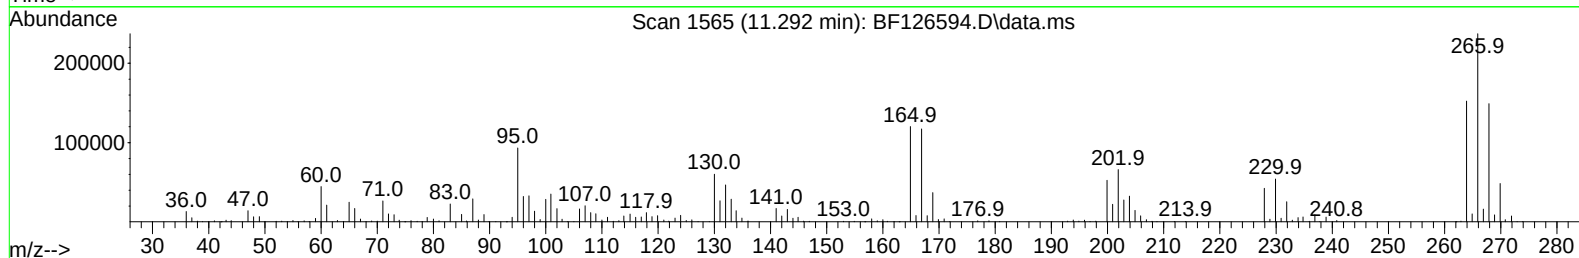


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011822\
Data File : BF126594.D
Acq On : 18 Jan 2022 10:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 12:08:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 18 12:08:17 2022
Response via : Initial Calibration

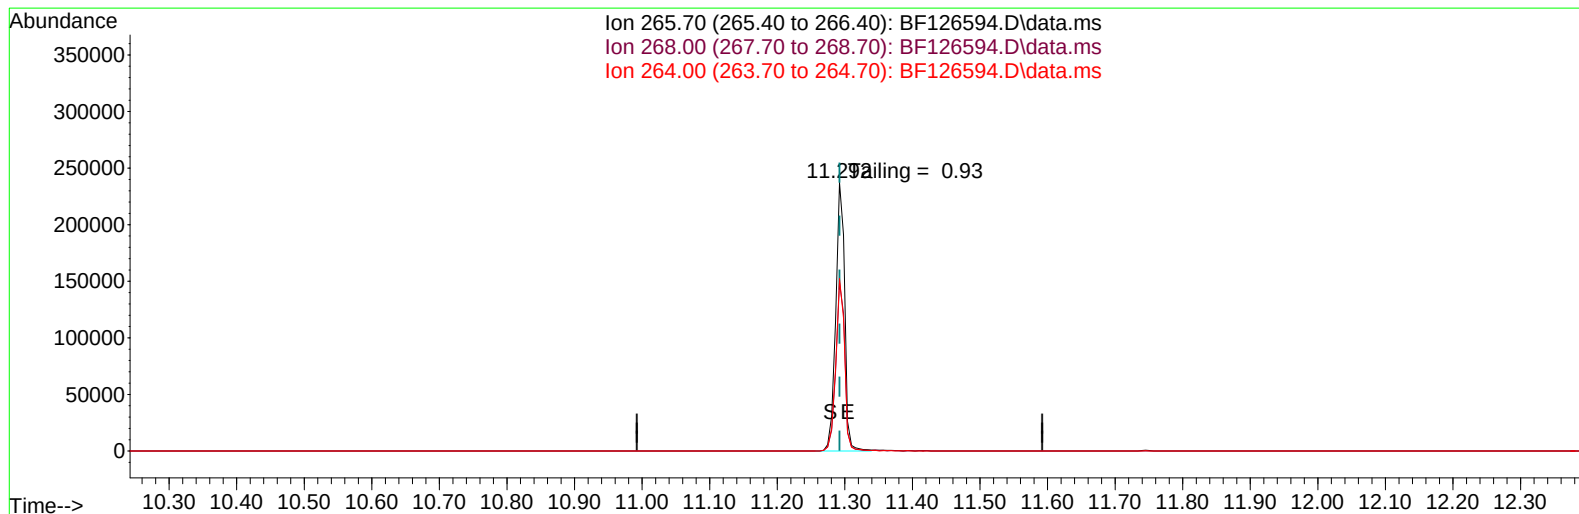

TIC: BF126594.D\data.ms

(70) Pentachlorophenol (C)




11.292min (0.000) 0.00 ng

response 219725

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	62.84
264.00	63.00	64.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011822\
Data File : BF126594.D
Acq On : 18 Jan 2022 10:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 12:08:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 18 12:08:17 2022
Response via : Initial Calibration

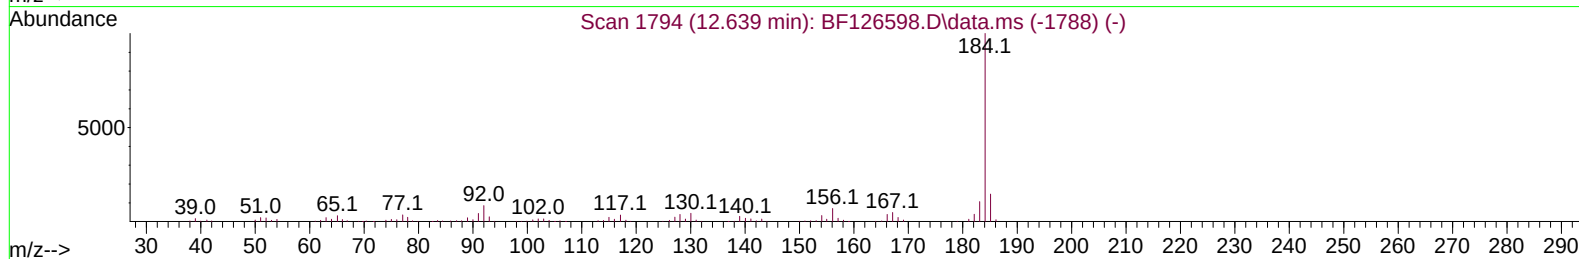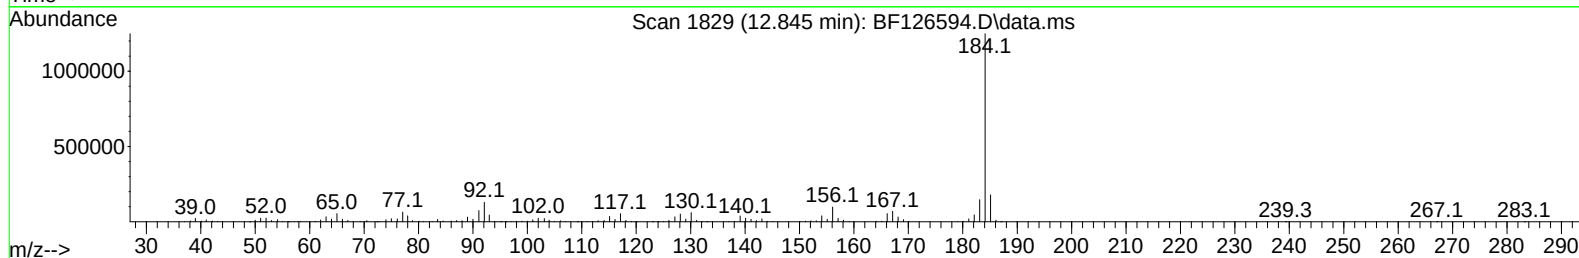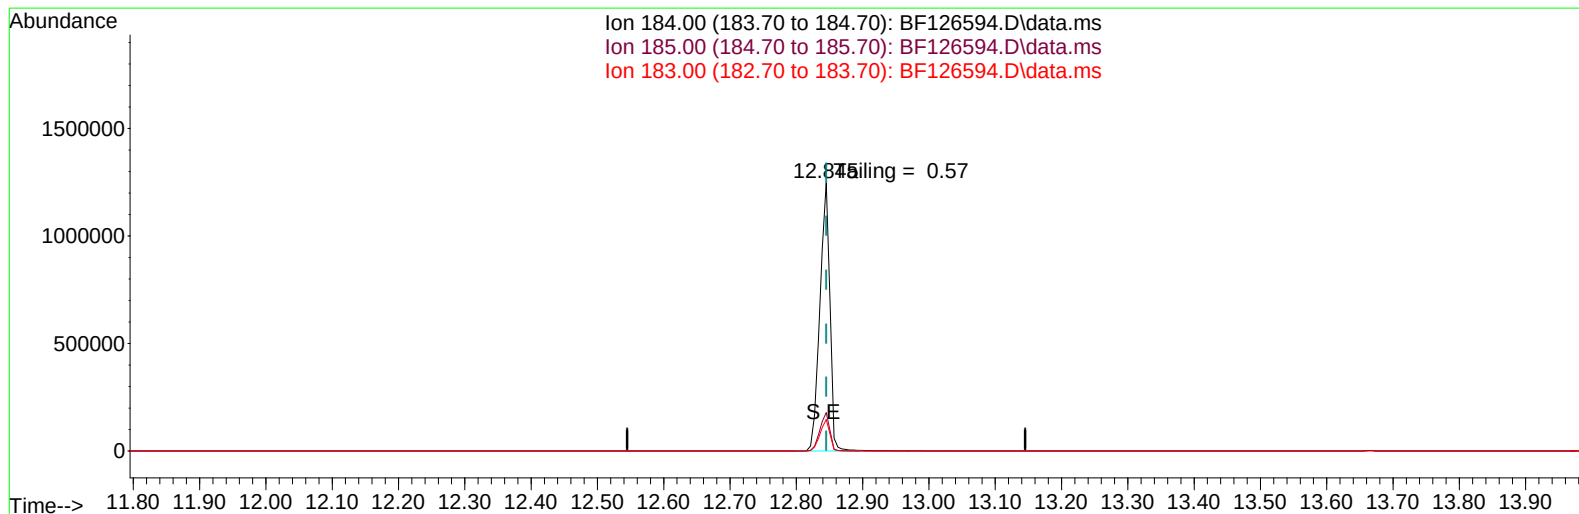

TIC: BF126594.D\data.ms

(77) Benzidine

12.845min (0.000) 0.00 ng

response 1310900

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.29
183.00	10.20	11.74
0.00	0.00	0.00