

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011822\
 Data File : BF126604.D
 Acq On : 18 Jan 2022 16:42
 Operator : CG/JU
 Sample : PB142011BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB142011BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF126604.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.375	40	49	54	rVB	103193	152012	2.87%	0.492%
2	5.593	590	596	599	rBV	3466873	3961172	74.78%	12.811%
3	6.575	757	763	766	rBV	3400407	4154786	78.44%	13.437%
4	6.963	825	829	832	rVB	947839	785647	14.83%	2.541%
5	7.522	919	924	927	rBV	2391254	2710695	51.18%	8.767%
6	8.245	1042	1047	1050	rBV	1096718	1070406	20.21%	3.462%
7	9.322	1224	1230	1233	rBV	4071305	4580033	86.47%	14.812%
8	10.004	1341	1346	1350	rBV	1352928	1275645	24.08%	4.126%
9	10.798	1474	1481	1484	rBV	2755601	3065559	57.88%	9.914%
10	11.498	1594	1600	1603	rBV	1572448	1375884	25.98%	4.450%
11	13.092	1863	1871	1874	rBV	4935673	5296834	100.00%	17.130%
12	14.168	2050	2054	2058	rBV	1481370	1279787	24.16%	4.139%
13	14.763	2147	2155	2165	rBV4	18433	62154	1.17%	0.201%
14	15.739	2314	2321	2325	rBV	861614	1150005	21.71%	3.719%


Sum of corrected areas: 30920619

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011822\
Data File : BF126604.D
Acq On : 18 Jan 2022 16:42
Operator : CG/JU
Sample : PB142011BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142011BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

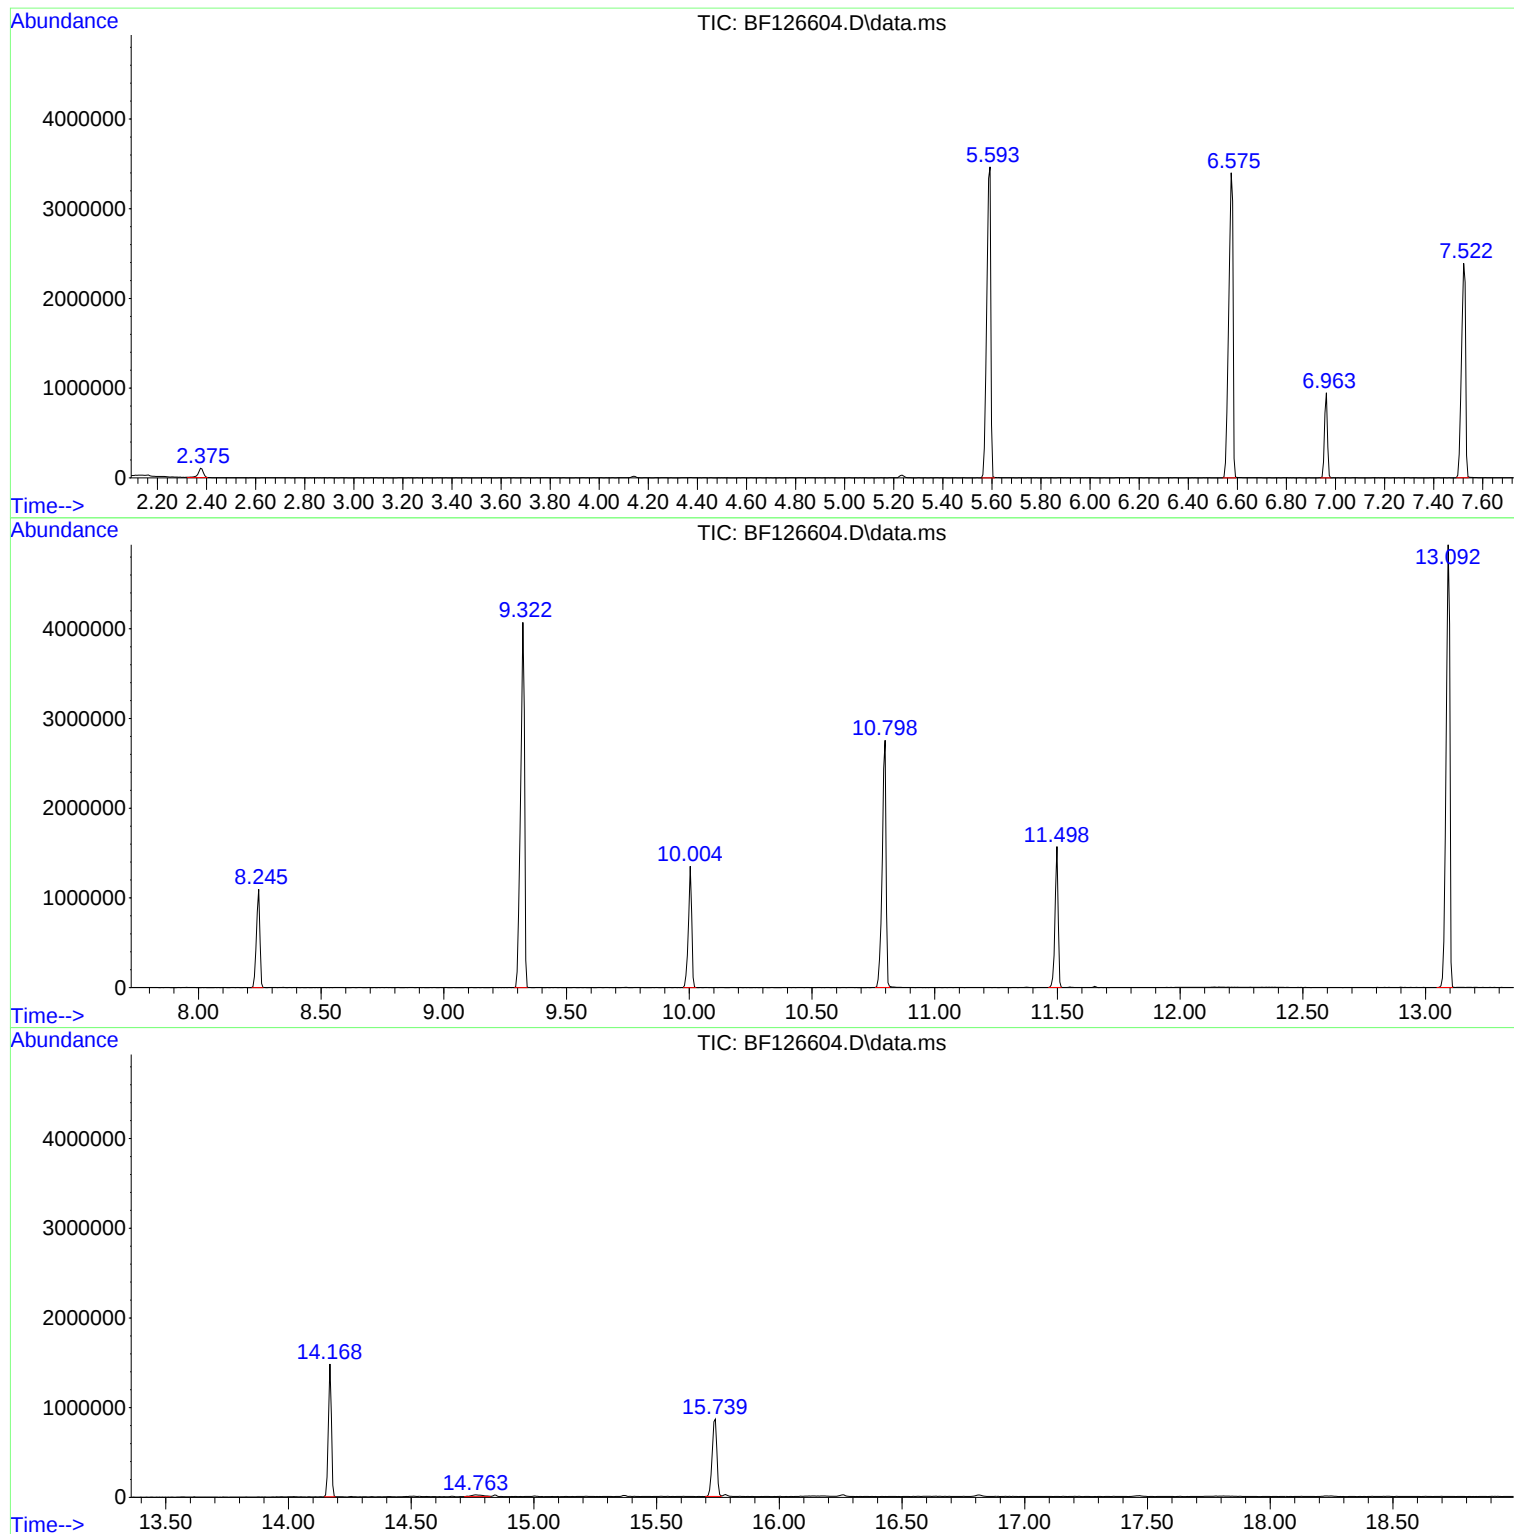

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011822\
Data File : BF126604.D
Acq On : 18 Jan 2022 16:42
Operator : CG/JU
Sample : PB142011BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142011BL









Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.375	3.87 ng	152012	1,4-Dichlorobenzene-d4	6.963

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	43
3			1,3-Dioxolane, 2-propyl-	116	C6H12O2	003390-13-4	23
4			N-Ethylformamide	73	C3H7NO	000627-45-2	9
5			Borane, dimethoxy-	74	C2H7BO2	004542-61-4	9

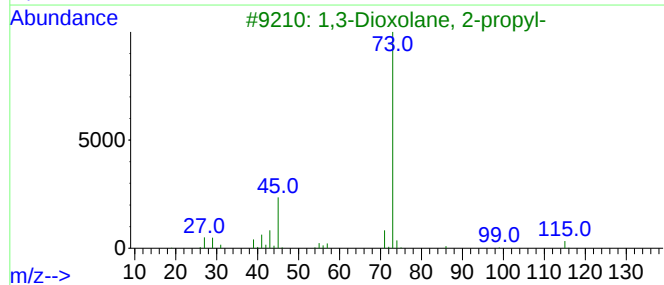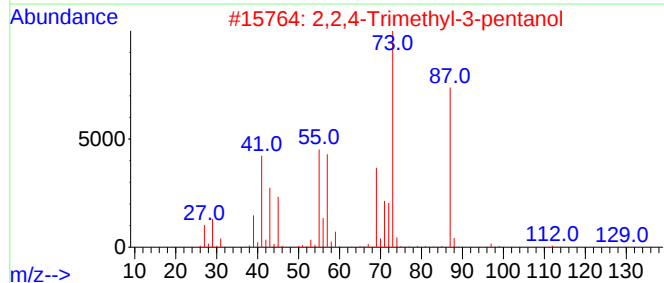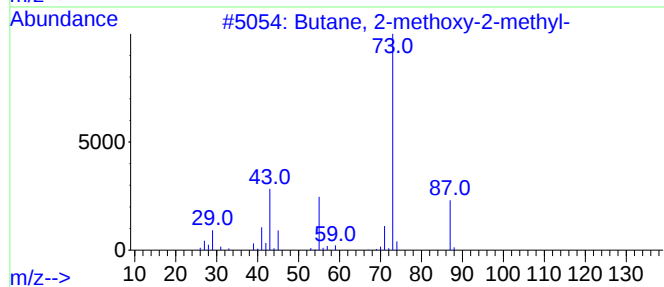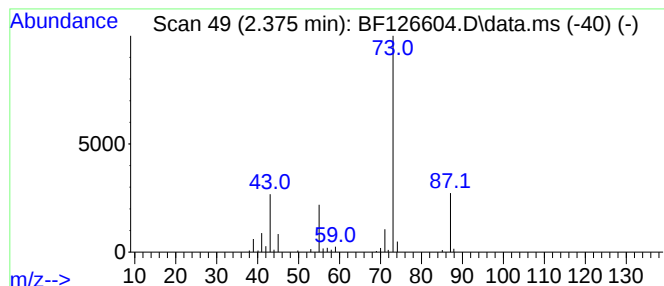

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011822\
Data File : BF126604.D
Acq On : 18 Jan 2022 16:42
Operator : CG/JU
Sample : PB142011BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142011BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.375	3.9	ng	152012	1	6.963	785647	20.0