


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011822\
 Data File : BF126594.D
 Acq On : 18 Jan 2022 10:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 19 07:04:14 2022

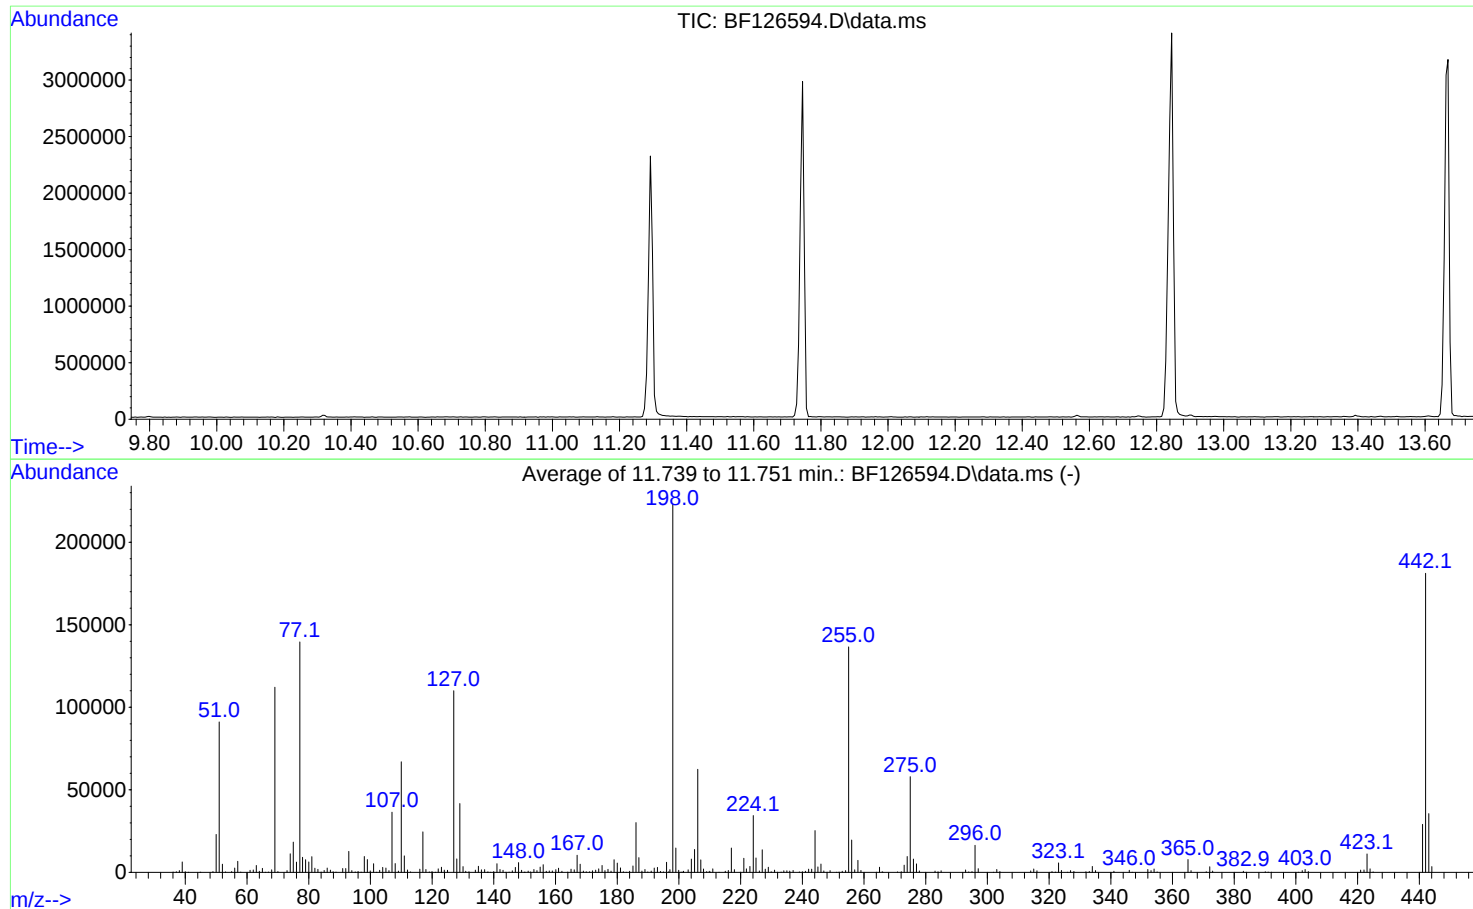




AutoFind: Scans 1641, 1642, 1643; Background Corrected with Scan 1635

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.9	91080	PASS
68	69	0.00	2	1.4	1584	PASS
69	198	0.00	100	50.3	112164	PASS
70	69	0.00	2	0.4	490	PASS
127	198	10	80	49.4	110069	PASS
197	198	0.00	2	0.7	1611	PASS
198	198	100	100	100.0	222869	PASS
199	198	5	9	6.6	14709	PASS
275	198	10	60	26.0	58000	PASS
365	198	1	100	3.5	7715	PASS
441	198	0.01	100	13.1	29107	PASS
442	442	50	100	100.0	181221	PASS
443	442	15	24	19.6	35565	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011822\
Data File : BF126594.D
Acq On : 18 Jan 2022 10:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 18 12:08:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 18 12:08:17 2022
Response via : Initial Calibration

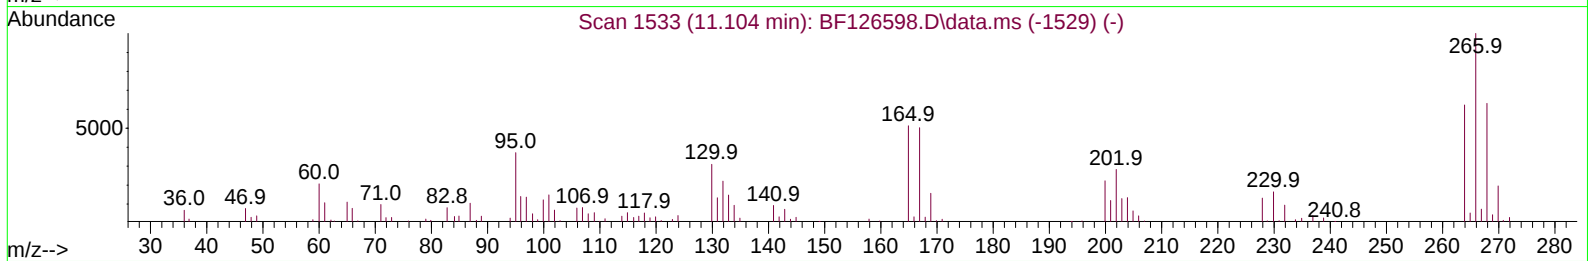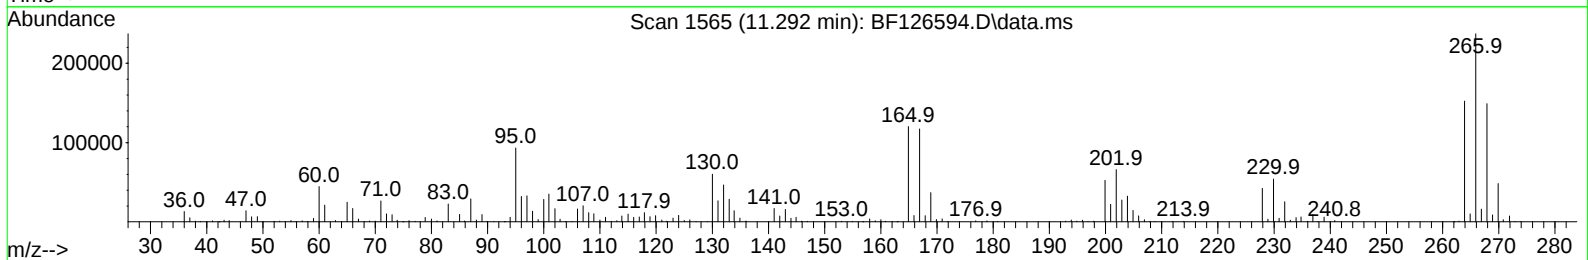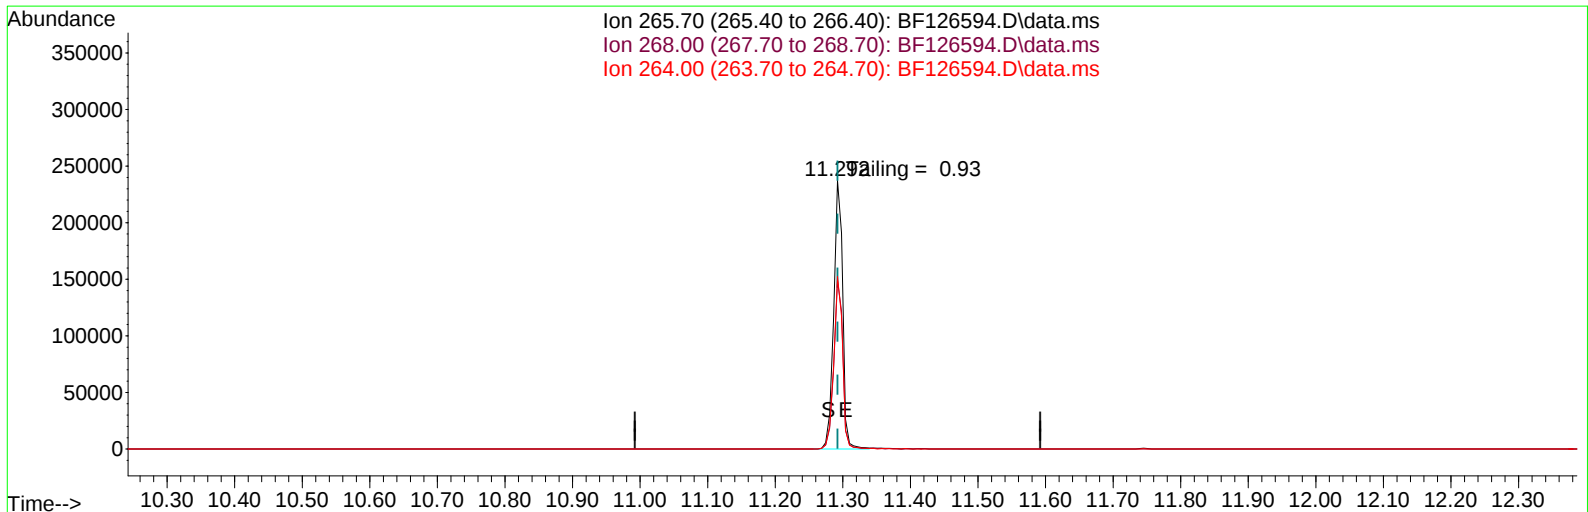

TIC: BF126594.D\data.ms

(70) Pentachlorophenol (C)

11.292min (0.000) 0.00 ng




response 219725

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	62.84
264.00	63.00	64.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011822\
 Data File : BF126594.D
 Acq On : 18 Jan 2022 10:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jan 18 12:08:35 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 18 12:08:17 2022
 Response via : Initial Calibration

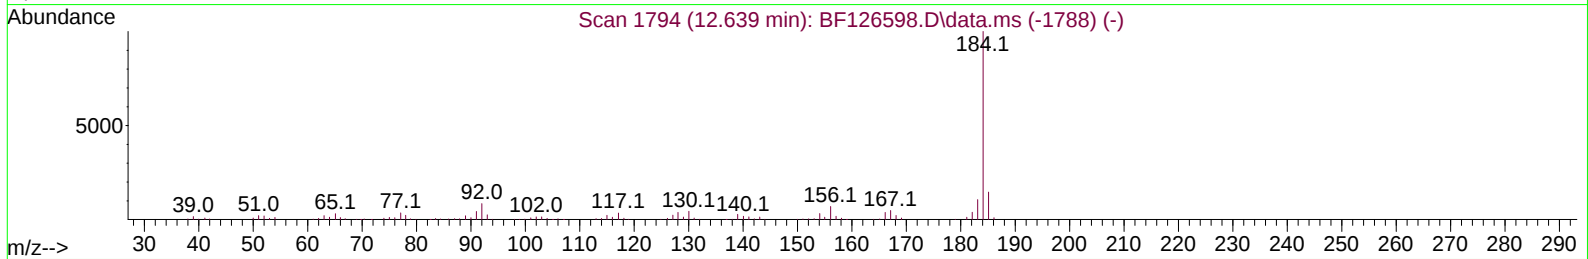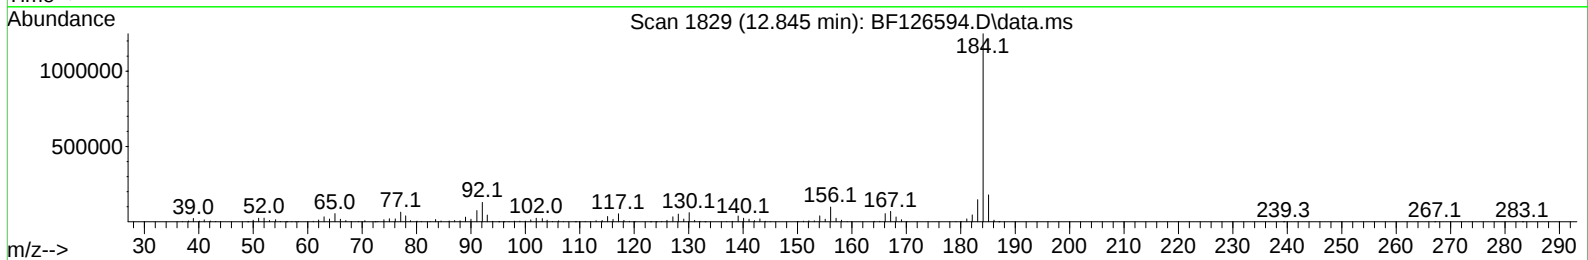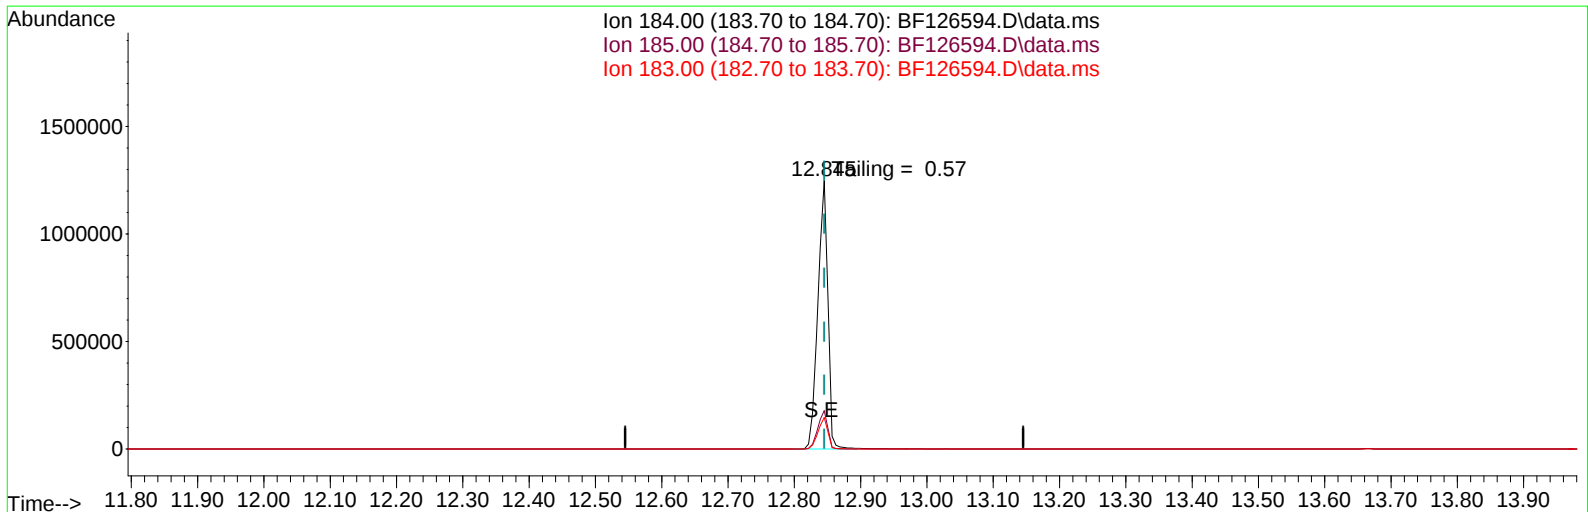

TIC: BF126594.D\data.ms

(77) Benzidine

12.845min (0.000) 0.00 ng

response 1310900

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.29
183.00	10.20	11.74
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/18/2022	BNA_F	<u>BF126594.D</u>
Compound Name	Response	Retention Time
DDT	524911	13.66
DDD	869	13.35
DDE	0	12.96
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
869	525780	0.17

Instrument :
BNA_F
ClientSampleId :
DFTPP