

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011915\
 Data File : BF076927.D
 Acq On : 19 Jan 2015 13:39
 Operator : IZ / TP
 Sample : G1101-07
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TE-PMW-2-22

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.464	31	33	42	rBV	29308	63814	5.12%	0.837%
2	4.104	261	264	273	rVB	20480	46350	3.72%	0.608%
3	5.030	342	345	353	rBV	195824	375191	30.12%	4.920%
4	7.362	547	549	555	rBV	128675	218123	17.51%	2.861%
5	7.465	555	558	567	rVB	499830	798014	64.07%	10.465%
6	7.968	599	602	608	rVB	108760	183476	14.73%	2.406%
7	8.299	627	631	634	rBV	459850	781907	62.78%	10.254%
8	9.271	712	716	719	rBV	427499	634680	50.96%	8.323%
9	10.882	853	857	860	rBV	170020	260565	20.92%	3.417%
10	13.534	1085	1089	1092	rBV	855237	1245470	100.00%	16.334%
11	15.008	1215	1218	1222	rBV	191876	287339	23.07%	3.768%
12	16.677	1361	1364	1367	rBV	496688	624765	50.16%	8.193%
13	17.123	1401	1403	1405	rVB	14399	15004	1.20%	0.197%
14	17.774	1457	1460	1463	rBV	277469	300405	24.12%	3.940%
15	18.746	1543	1545	1551	rBV2	20538	29133	2.34%	0.382%
16	20.003	1652	1655	1658	rBV	1017904	1064755	85.49%	13.964%
17	21.180	1756	1758	1761	rVB3	12135	14808	1.19%	0.194%
18	21.272	1761	1766	1769	rBV	287830	374662	30.08%	4.913%
19	22.049	1831	1834	1838	rBV2	7580	18567	1.49%	0.243%
20	22.941	1909	1912	1916	rVB	226374	274648	22.05%	3.602%
21	24.369	2035	2037	2043	rVB4	3834	13560	1.09%	0.178%


Sum of corrected areas: 7625236

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011915\
Data File : BF076927.D
Acq On : 19 Jan 2015 13:39
Operator : IZ / TP
Sample : G1101-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TE-PMW-2-22

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

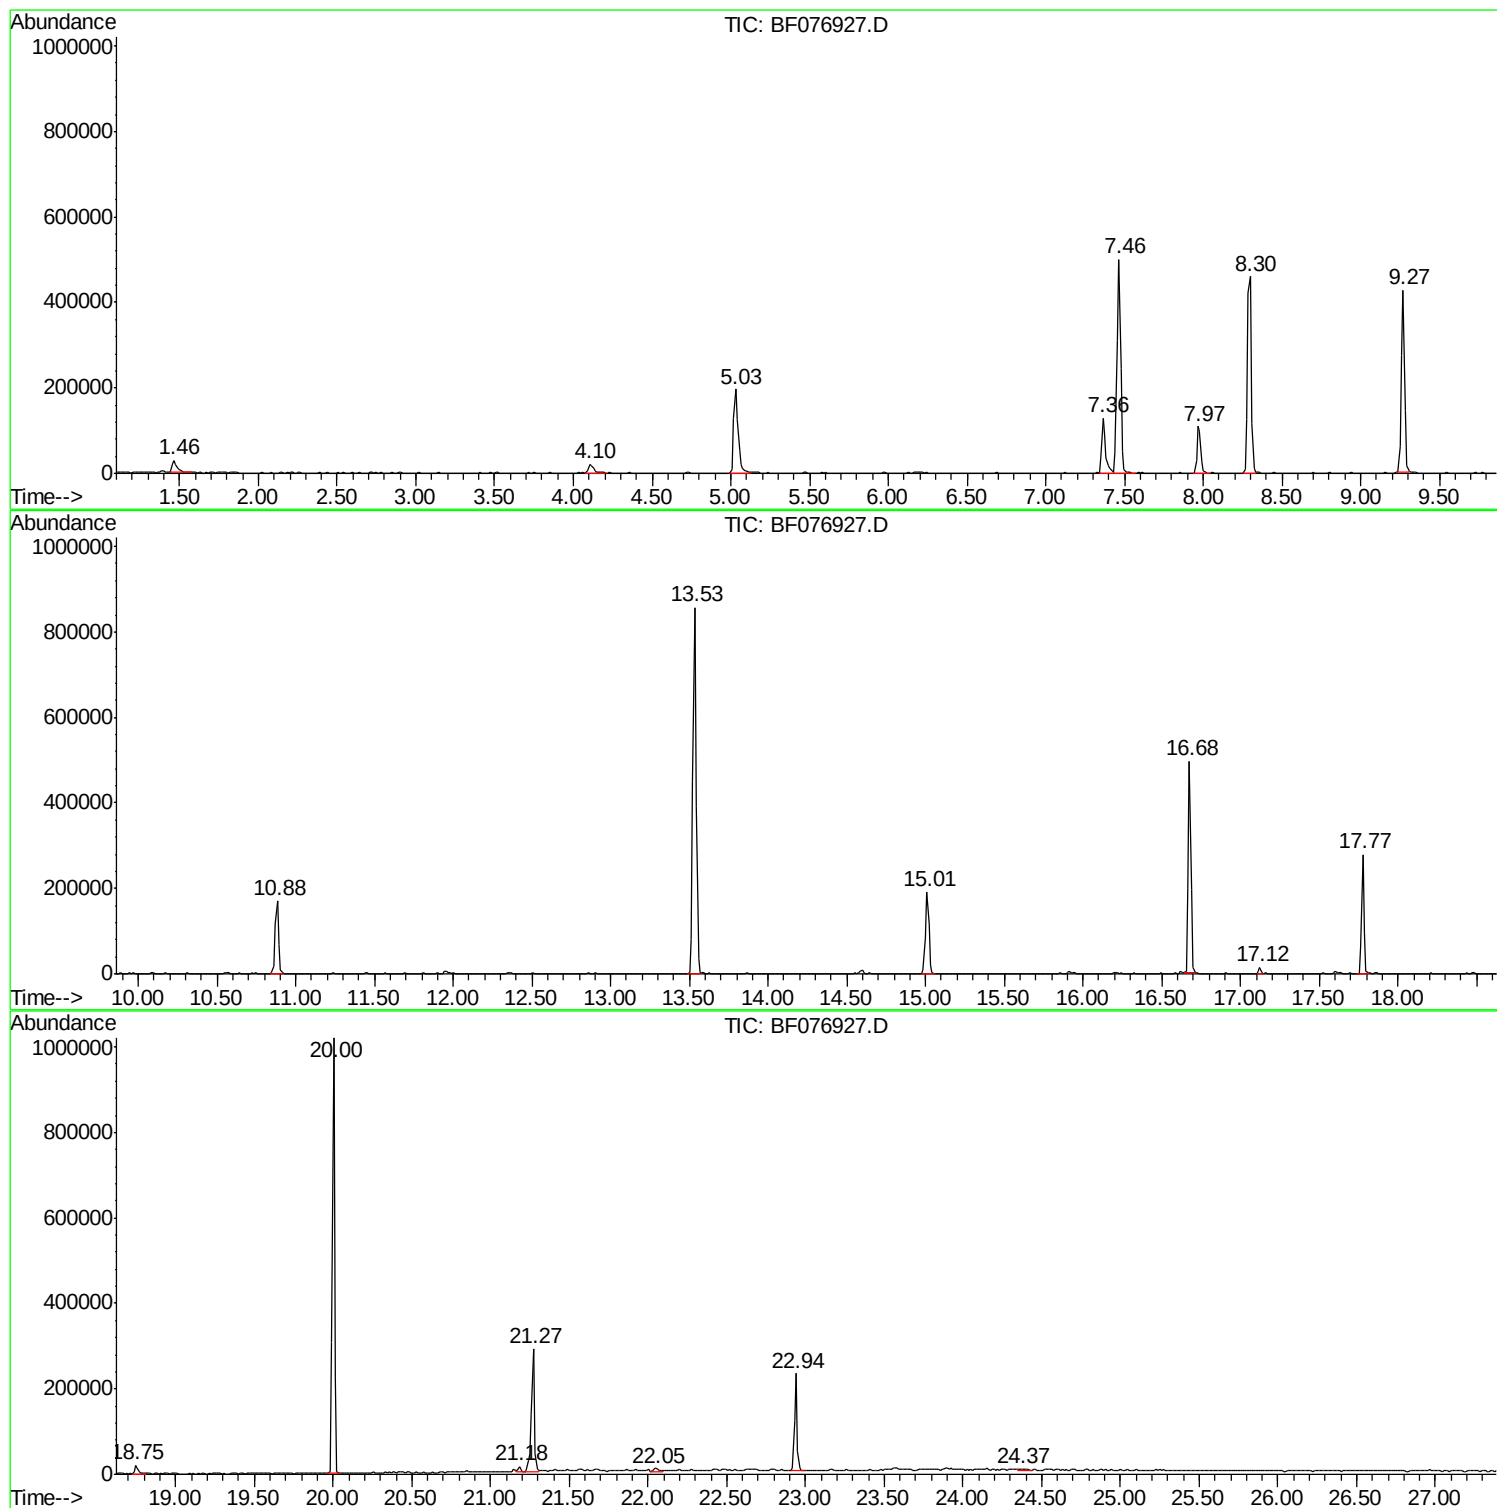

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011915\
Data File : BF076927.D
Acq On : 19 Jan 2015 13:39
Operator : IZ / TP
Sample : G1101-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TE-PMW-2-22










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown4.10 Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.10	5.05 ng	46350	1,4-Dichlorobenzene-d4	7.97

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Oxirane, [(1-methylethoxy)methyl]-	116	C6H12O2	004016-14-2	43
2			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	9
3			3-Hexanol	102	C6H14O	000623-37-0	9
4			Acetone	58	C3H6O	000067-64-1	5
5			Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	5

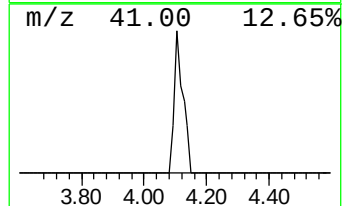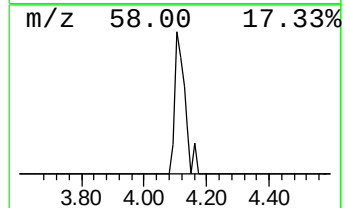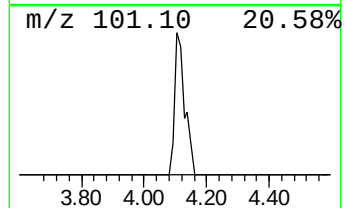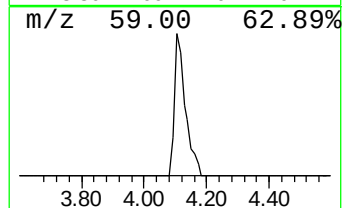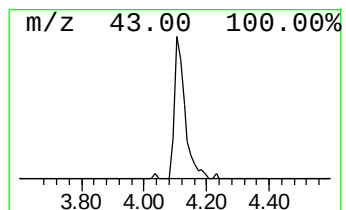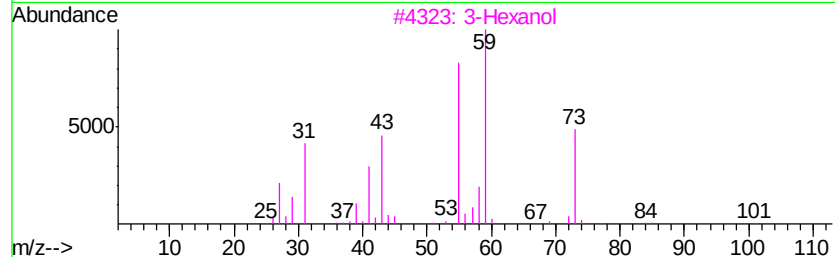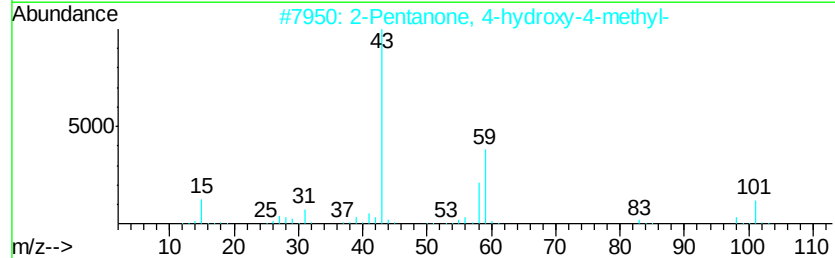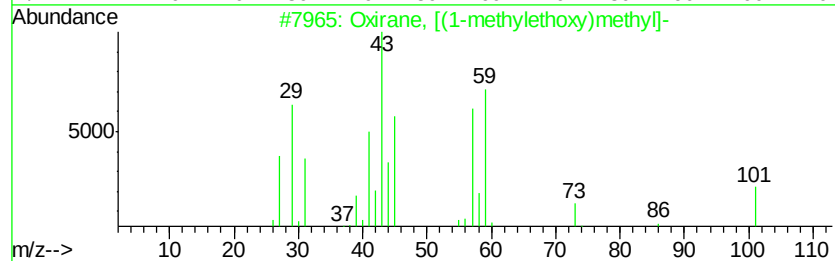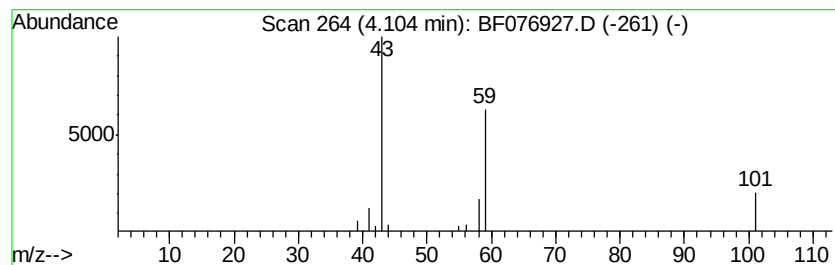

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011915\
Data File : BF076927.D
Acq On : 19 Jan 2015 13:39
Operator : IZ / TP
Sample : G1101-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TE-PMW-2-22










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 unknown7.46 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.46	86.99 ng	798014	1,4-Dichlorobenzene-d4	7.97

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
3		Tranvlcypromine-propionyl	189	C12H15NO	1000123-86-3	10
4		5-Aminoindole	132	C8H8N2	005192-03-0	10
5		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

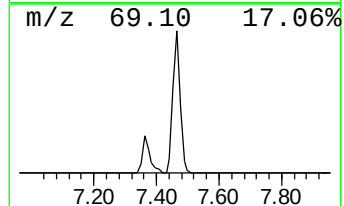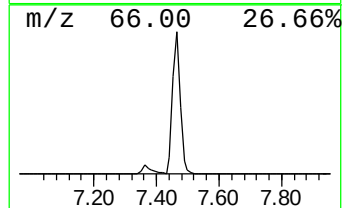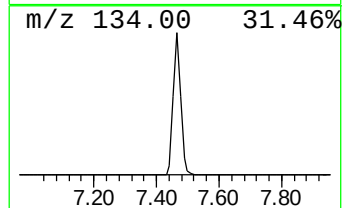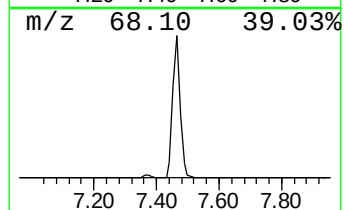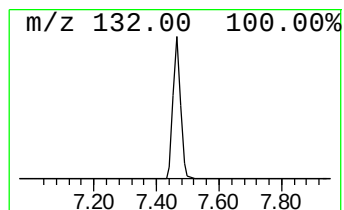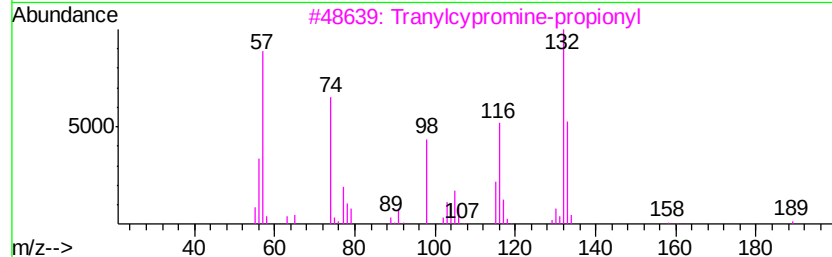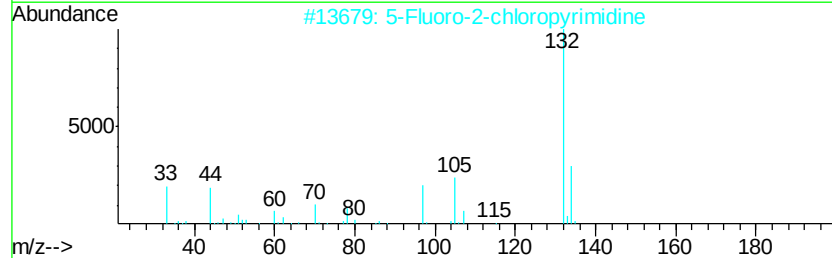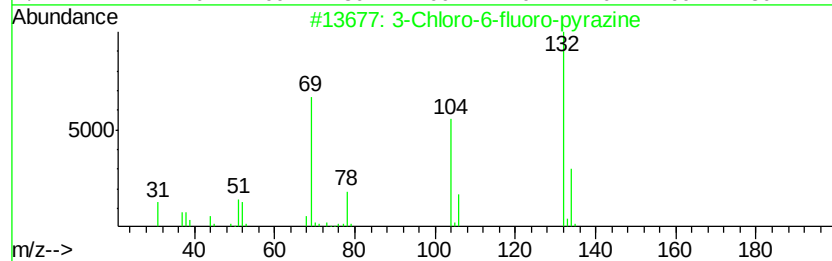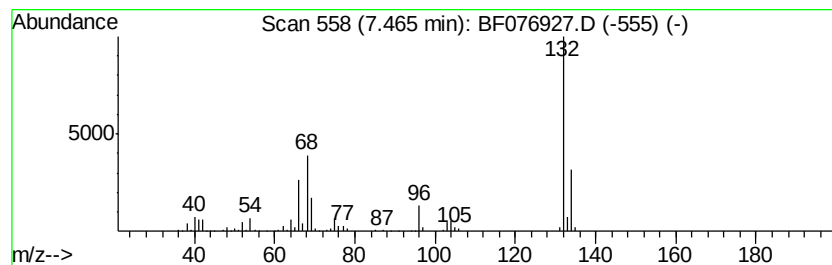

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011915\
Data File : BF076927.D
Acq On : 19 Jan 2015 13:39
Operator : IZ / TP
Sample : G1101-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TE-PMW-2-22

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown4.10	4.10	5.0	ng	46350	1	7.97	183476	20.0
unknown7.46	7.46	87.0	ng	798014	1	7.97	183476	20.0