


Data Path : Z:\HPCHEM1\BNA F\Data\BF011915\
 Data File : BF076941.D
 Acq On : 19 Jan 2015 22:51
 Operator : IZ / TP
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 15 11:52:04 2015

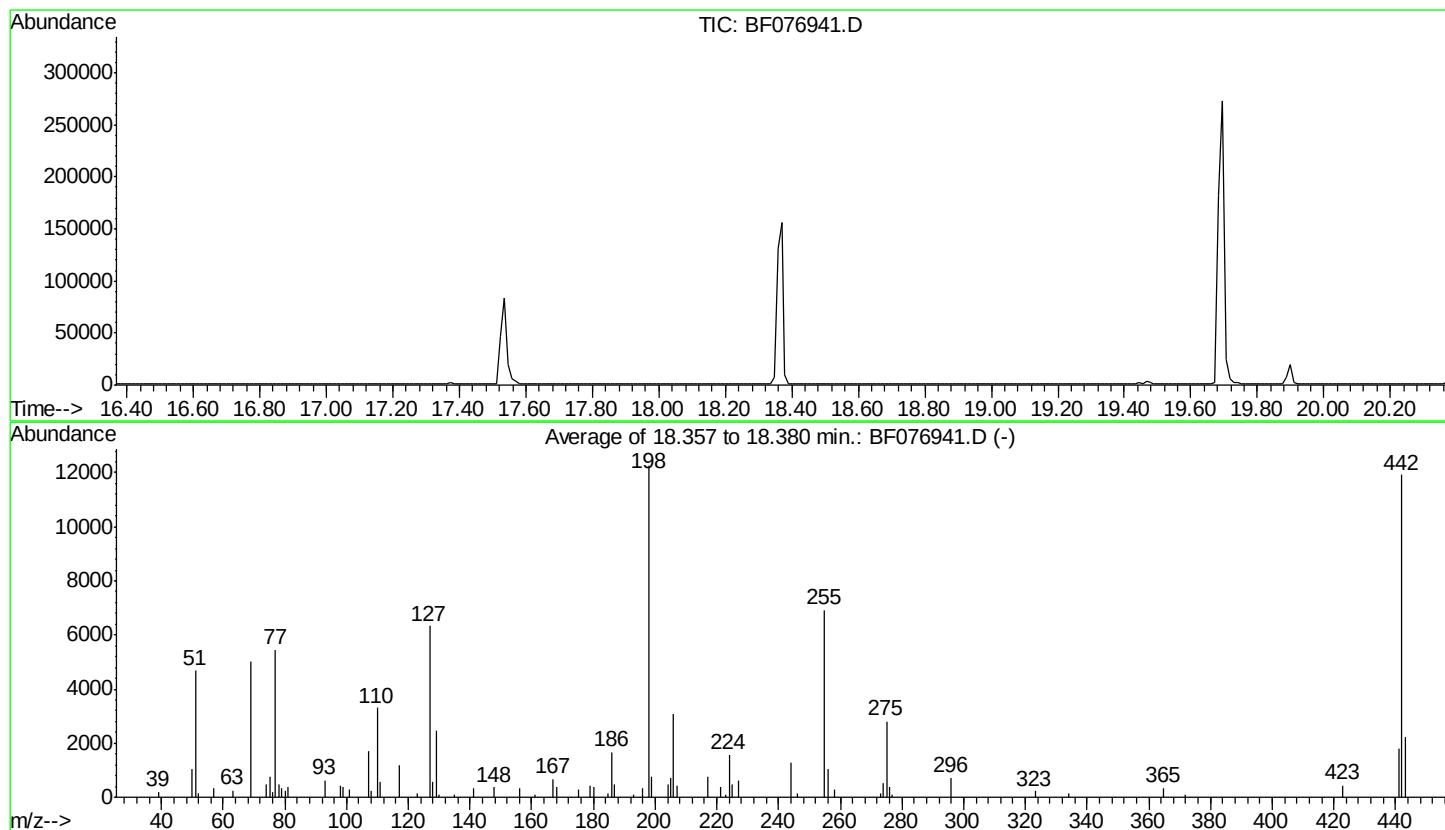

AutoFind: Scans 1511, 1512, 1513; Background Corrected with Scan 1507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.1	4675	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	40.9	5013	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.6	6321	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	12261	PASS
199	198	5	9	6.1	744	PASS
275	198	10	60	23.0	2815	PASS
365	198	1	100	2.8	347	PASS
441	442	0.01	24	14.9	1781	PASS
442	198	50	100	97.3	11925	PASS
443	442	15	24	18.8	2240	PASS