
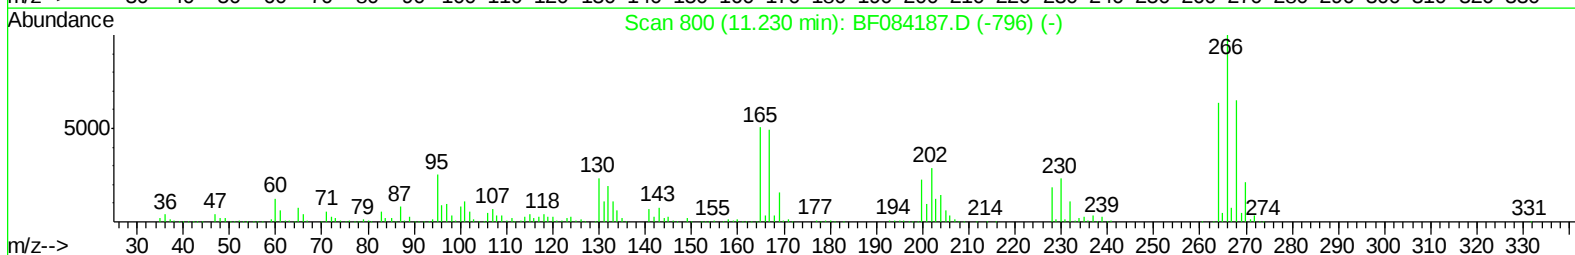
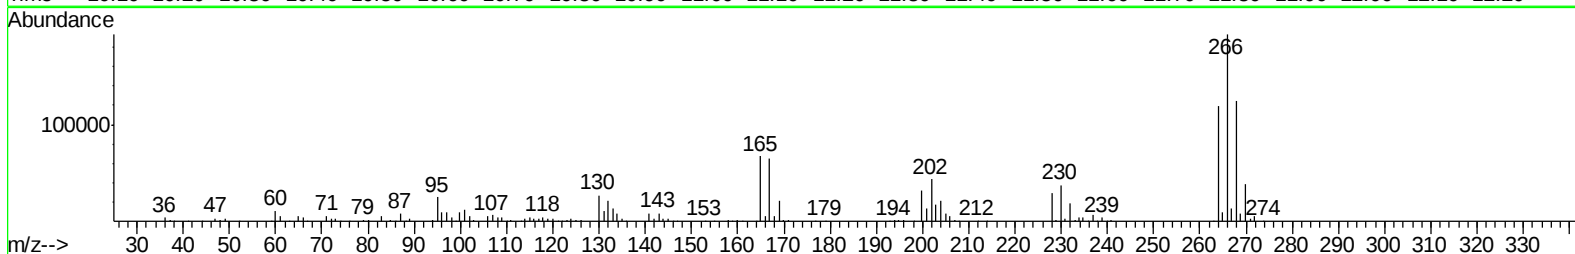


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011916\
Data File : BF084543.D
Acq On : 19 Jan 2016 9:02
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 19 17:12:48 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 14 14:15:52 2016
Response via : Initial Calibration

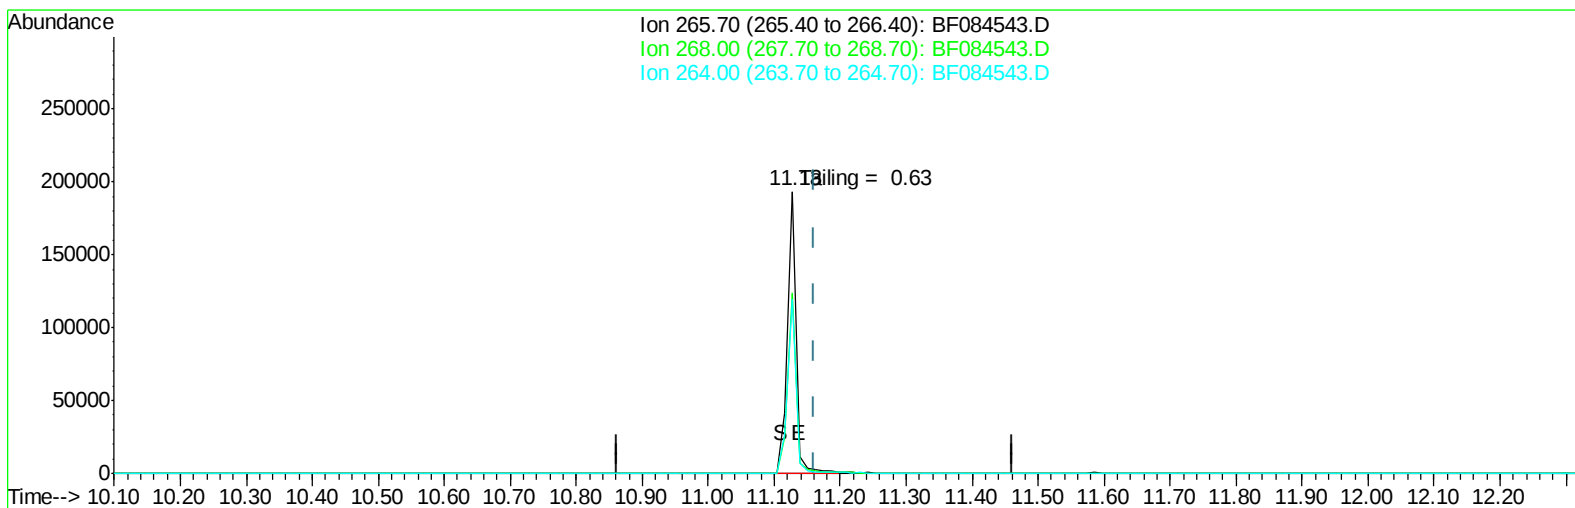

TIC: BF084543.D

(69) Pentachlorophenol (C)




11.128min (-0.034) 125610.47ng

response 179106

Ion	Exp%	Act%
265.70	100	100
268.00	65.50	64.24
264.00	62.70	61.78
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011916\
Data File : BF084543.D
Acq On : 19 Jan 2016 9:02
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 19 17:12:48 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 14 14:15:52 2016
Response via : Initial Calibration

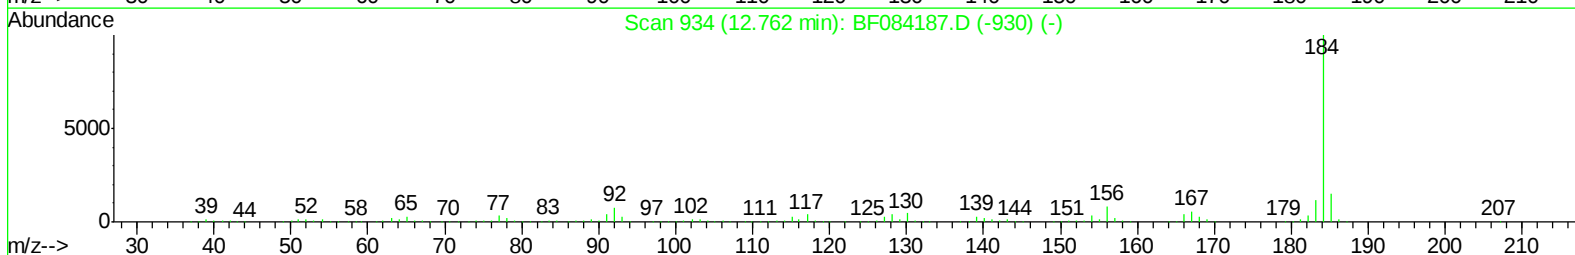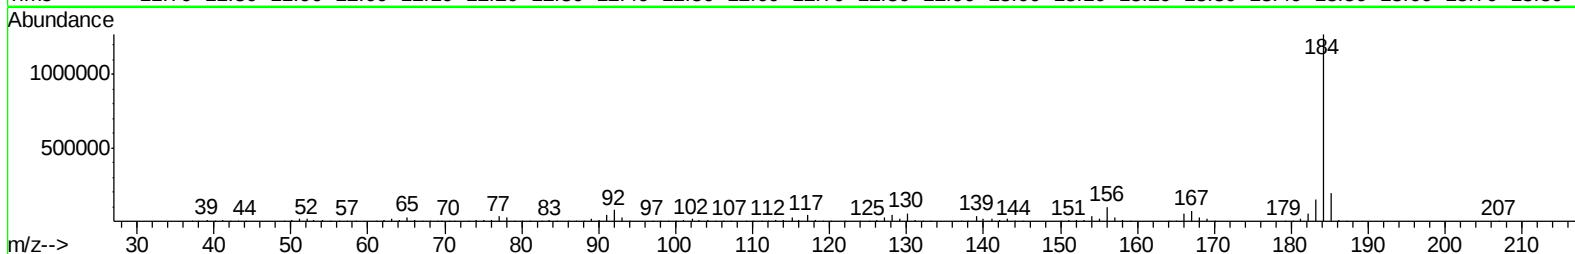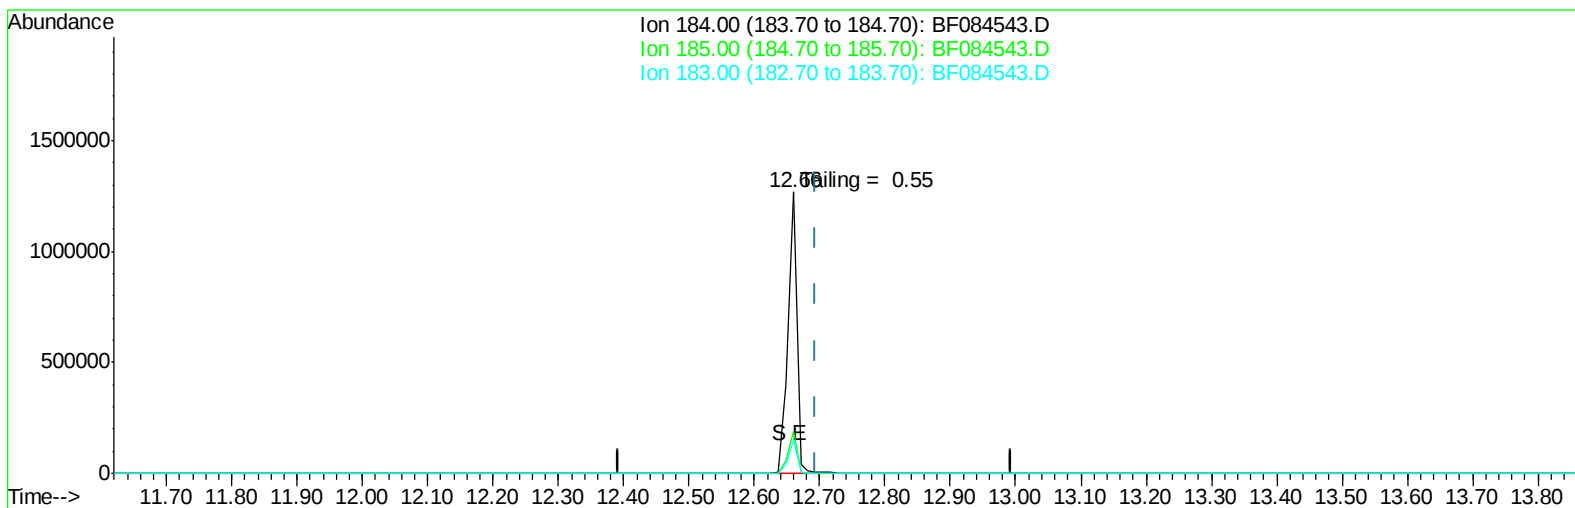

TIC: BF084543.D

(76) Benzidine

12.659min (-0.034) 24478.82ng

response 1203312

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.79
183.00	12.30	11.78
0.00	0.00	0.00