


Data Path : Z:\HPCHEM1\BNA F\DATA\BF011916\
 Data File : BF084548.D
 Acq On : 19 Jan 2016 13:25
 Operator : SJ/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 14 14:15:52 2016

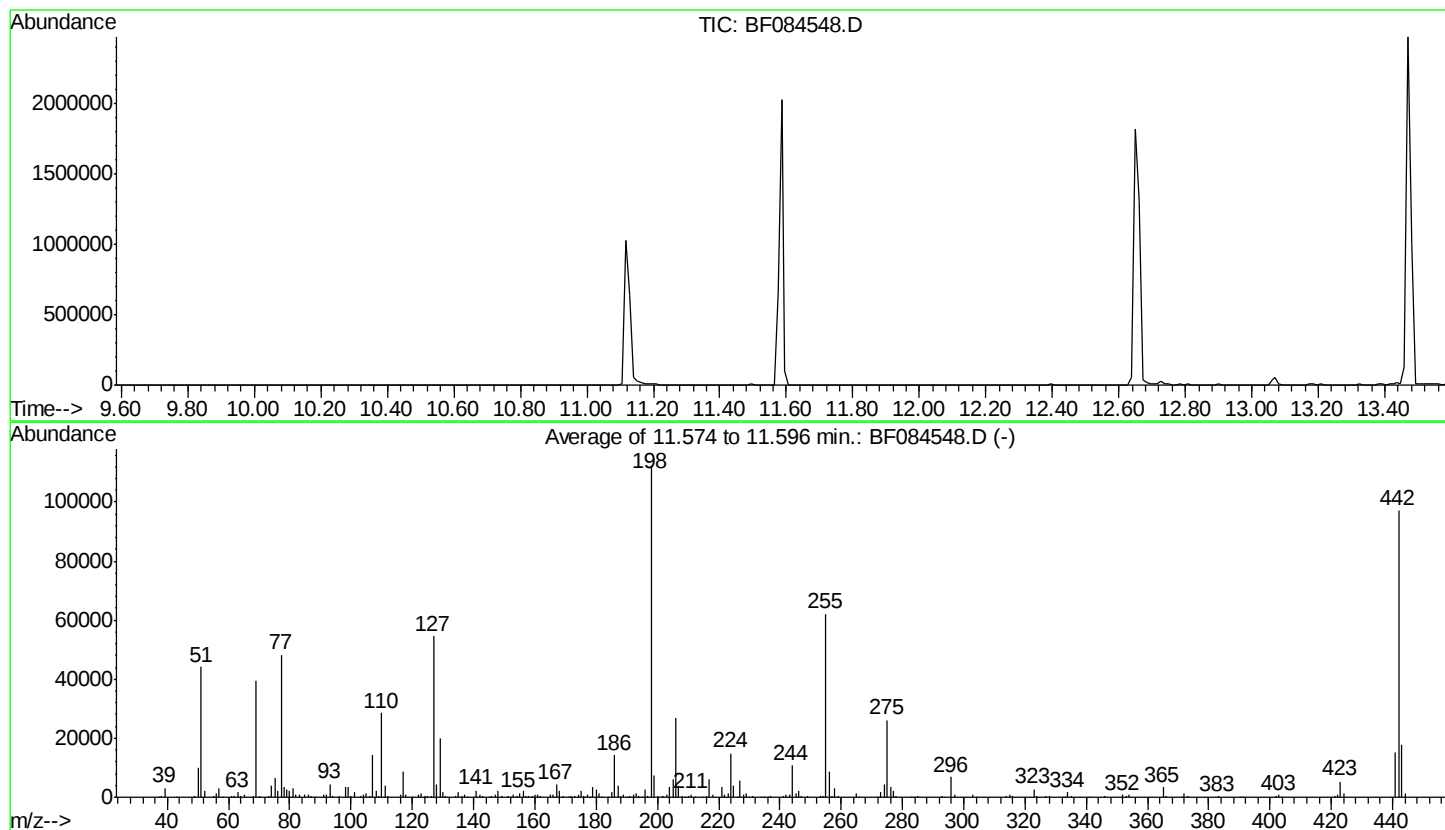

AutoFind: Scans 830, 831, 832; Background Corrected with Scan 827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.3	44214	PASS
68	69	0.00	2	1.4	569	PASS
69	198	0.00	100	35.0	39364	PASS
70	69	0.00	2	0.7	287	PASS
127	198	10	80	48.6	54615	PASS
197	198	0.00	2	0.5	572	PASS
198	198	100	100	100.0	112365	PASS
199	198	5	9	6.5	7295	PASS
275	198	10	60	23.3	26209	PASS
365	198	1	100	2.9	3286	PASS
441	442	0.01	24	15.8	15346	PASS
442	198	50	100	86.4	97045	PASS
443	442	15	24	18.3	17751	PASS