
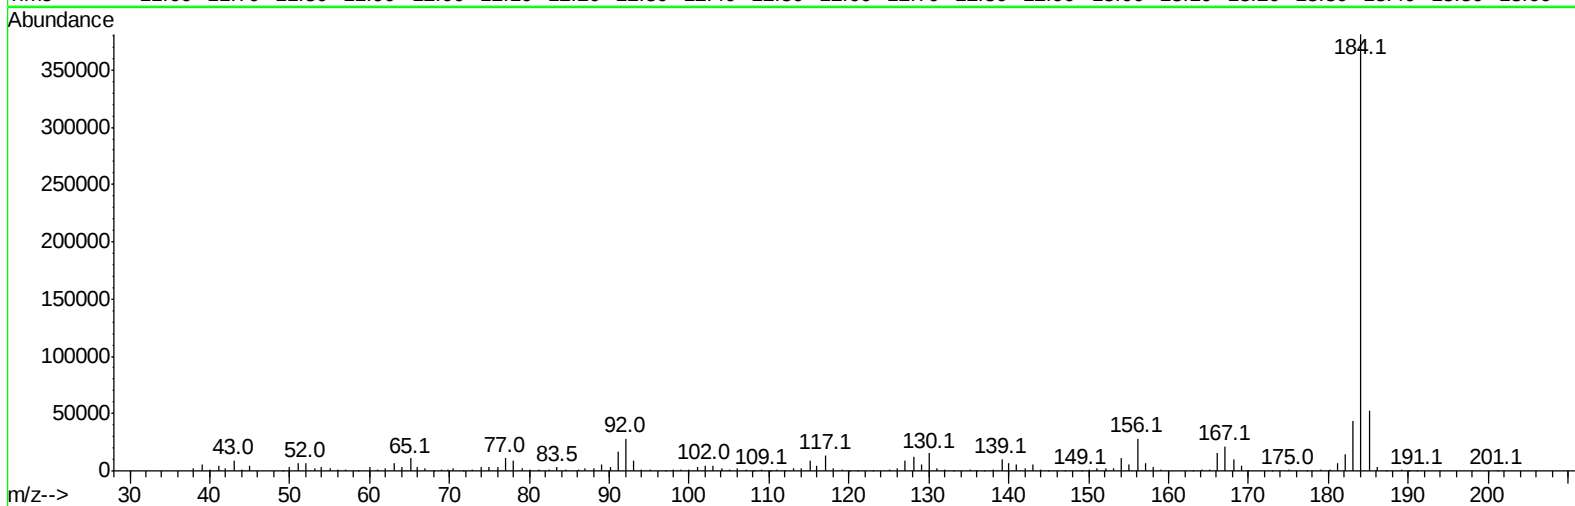


Data Path : U:\HPCHEM1\BNA F\DATA\BF011918\
Data File : BF102210.D
Acq On : 19 Jan 2018 9:17
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 20 02:47:16 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 19 13:31:35 2018
Response via : Initial Calibration

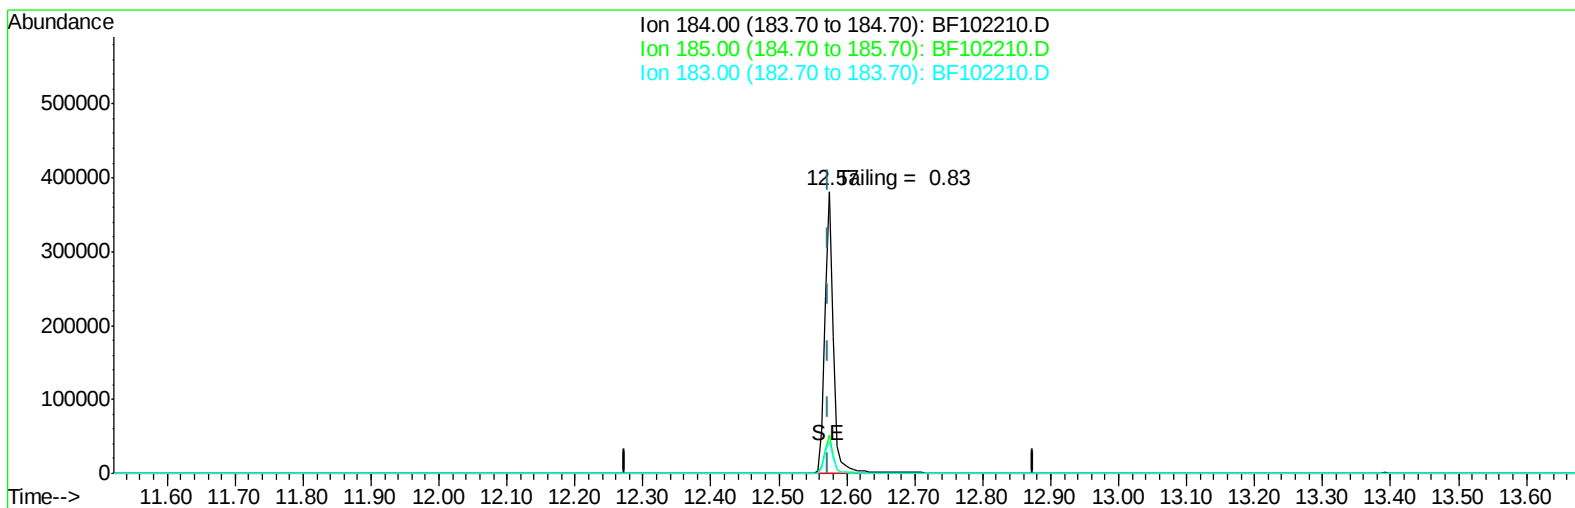

TIC: BF102210.D

(76) Benzidine



12.574min (+0.000) 0.00ng

response 342579

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.82
183.00	11.60	11.40
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA F\DATA\BF011918\
Data File : BF102210.D
Acq On : 19 Jan 2018 9:17
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 20 02:47:16 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 19 13:31:35 2018
Response via : Initial Calibration

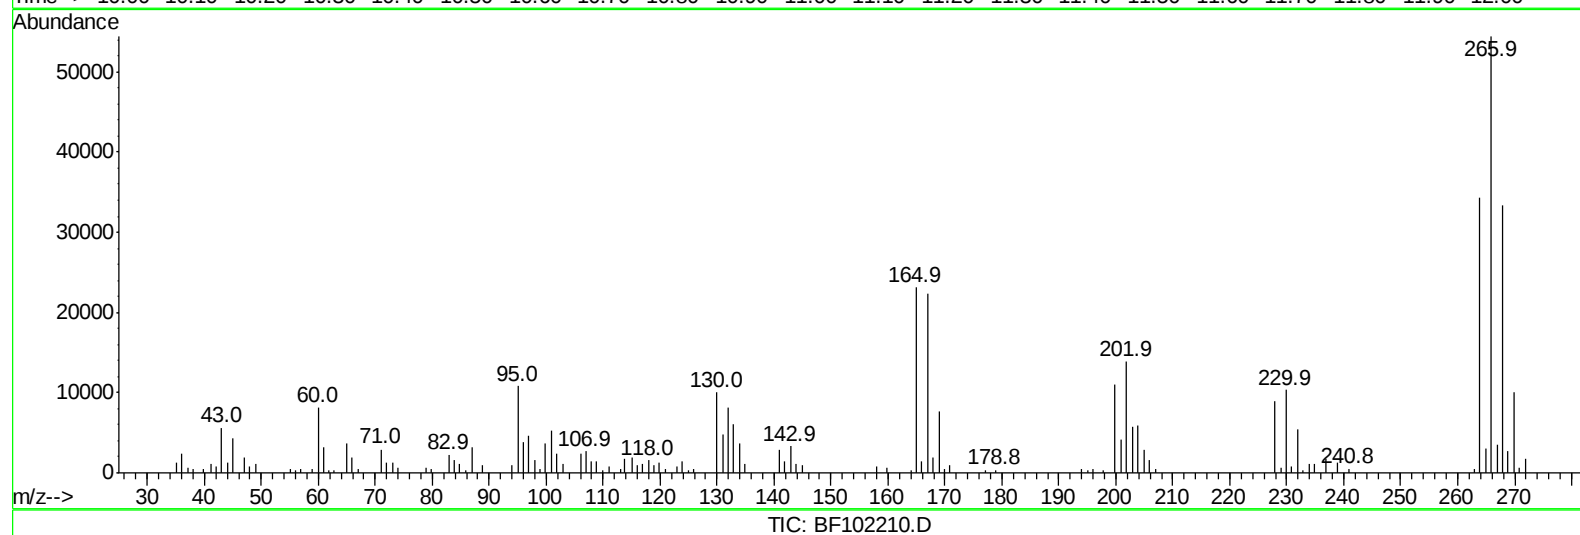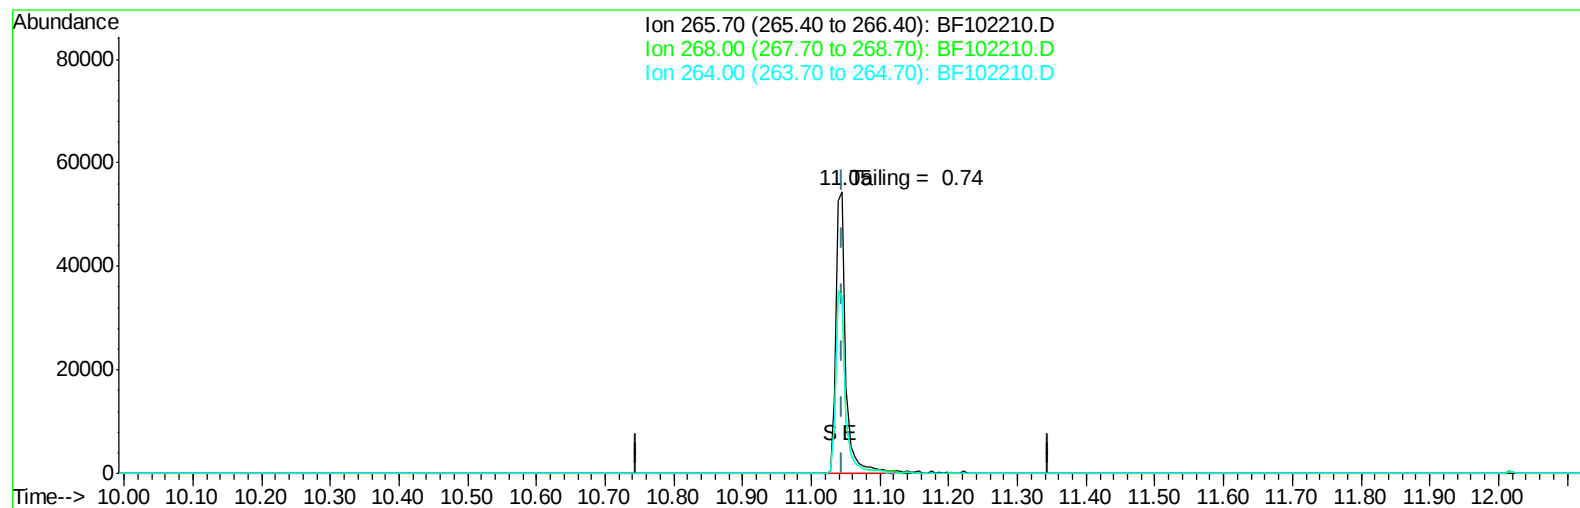

(69) Pentachlorophenol (C)

11.045min (+0.000) 21252.45ng

response 55430

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.42
264.00	61.90	63.14
0.00	0.00	0.00