


Data Path : Z:\HPCHEM1\BNA F\Data\BF011918\
 Data File : BF102210.D
 Acq On : 19 Jan 2018 9:17
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF010918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 19 13:31:35 2018

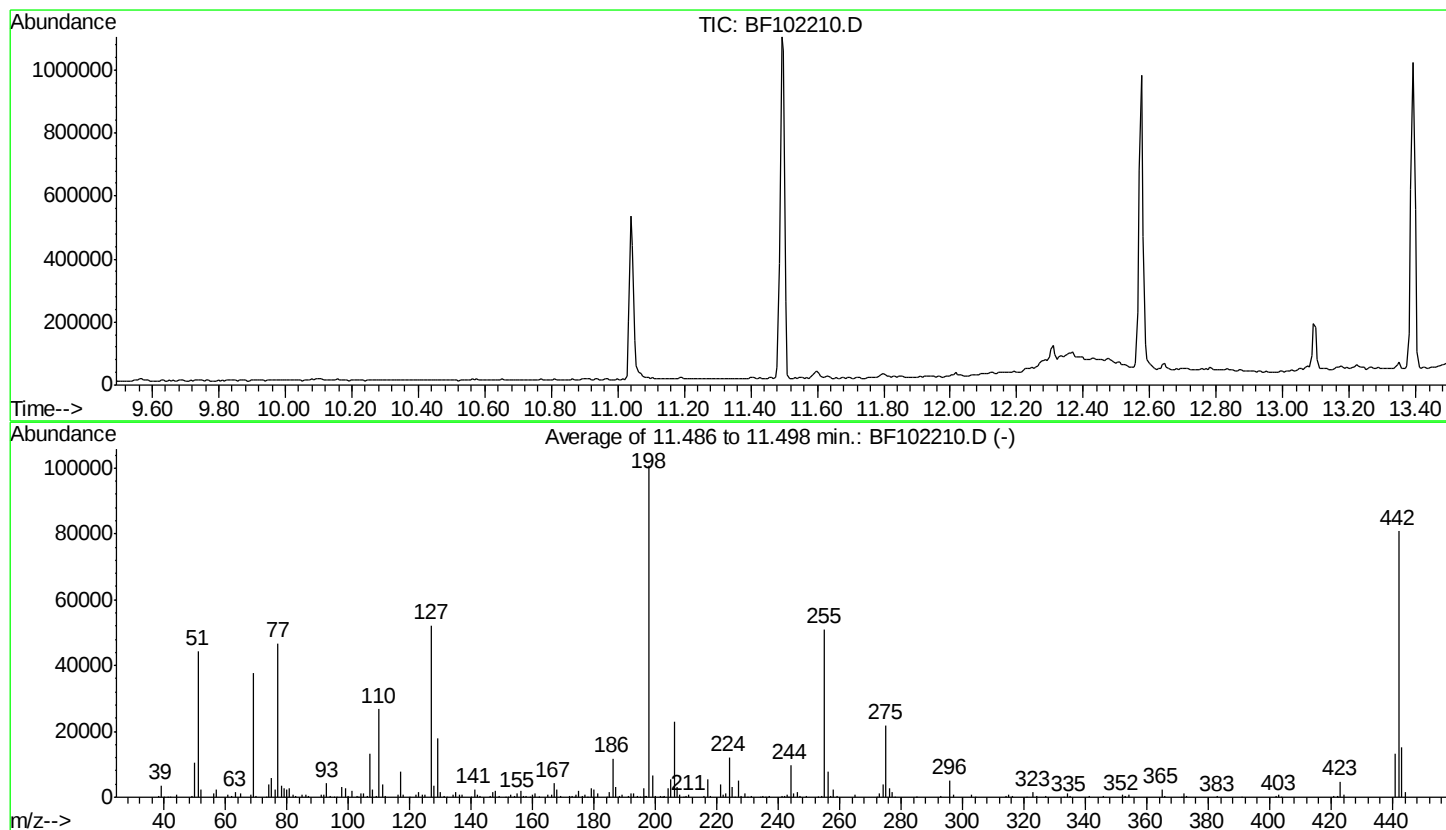

AutoFind: Scans 1598, 1599, 1600; Background Corrected with Scan 1593

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.1	44413	PASS
68	69	0.00	2	2.0	772	PASS
69	198	0.00	100	37.6	37897	PASS
70	69	0.00	2	0.7	264	PASS
127	198	10	80	51.8	52210	PASS
197	198	0.00	2	0.5	502	PASS
198	198	100	100	100.0	100714	PASS
199	198	5	9	6.7	6733	PASS
275	198	10	60	21.7	21827	PASS
365	198	1	100	2.5	2521	PASS
441	443	0.01	100	88.0	13218	PASS
442	198	50	100	80.4	81001	PASS
443	442	15	24	18.5	15018	PASS