

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011921\
 Data File : BF123014.D
 Acq On : 19 Jan 2021 11:57
 Operator : JU/CG
 Sample : PB134201TB
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB134201TB

Quant Time: Jan 19 15:59:12 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF011621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 18 13:14:08 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.90	152	136489	20.00	ng	0.00
21) Naphthalene-d8	8.18	136	724081	20.00	ng	0.00
39) Acenaphthene-d10	9.94	164	298737	20.00	ng	0.00
64) Phenanthrene-d10	11.43	188	491327	20.00	ng	0.00
76) Chrysene-d12	14.08	240	326481	20.00	ng	0.00
86) Perylene-d12	15.57	264	360837	20.00	ng	0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.53	112	1092014	120.94	ng	0.02
7) Phenol-d6	6.52	99	1376090	113.39	ng	0.00
23) Nitrobenzene-d5	7.46	82	1187086	84.36	ng	0.00
42) 2,4,6-Tribromophenol	10.73	330	352027	104.20	ng	0.00
45) 2-Fluorobiphenyl	9.26	172	1687129	79.08	ng	0.00
79) Terphenyl-d14	13.03	244	1417330	79.60	ng	0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
9) Benzaldehyde	6.52	77	2515	Below Cal	#	1
19) n-Nitroso-di-n-propylamine	7.46	70	168763	23.476	ng	# 77
25) Isophorone	7.46	82	1183090	47.126	ng	# 65
51) 2,6-Dinitrotoluene	9.94	165	36930	7.282	ng	# 31
57) 2,4-Dinitrotoluene	9.94	165	36930	5.661	ng	# 25
67) 4-Bromophenyl-phenylether	10.73	248	20690	3.444	ng	# 1
77) Benzidine	13.03	184	20075	2.322	ng	# 85

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011921\
Data File : BF123014.D
Acq On : 19 Jan 2021 11:57
Operator : JU/CG
Sample : PB134201TB
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB134201TB

Quant Time: Jan 19 15:59:12 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF011621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 18 13:14:08 2021
Response via : Initial Calibration

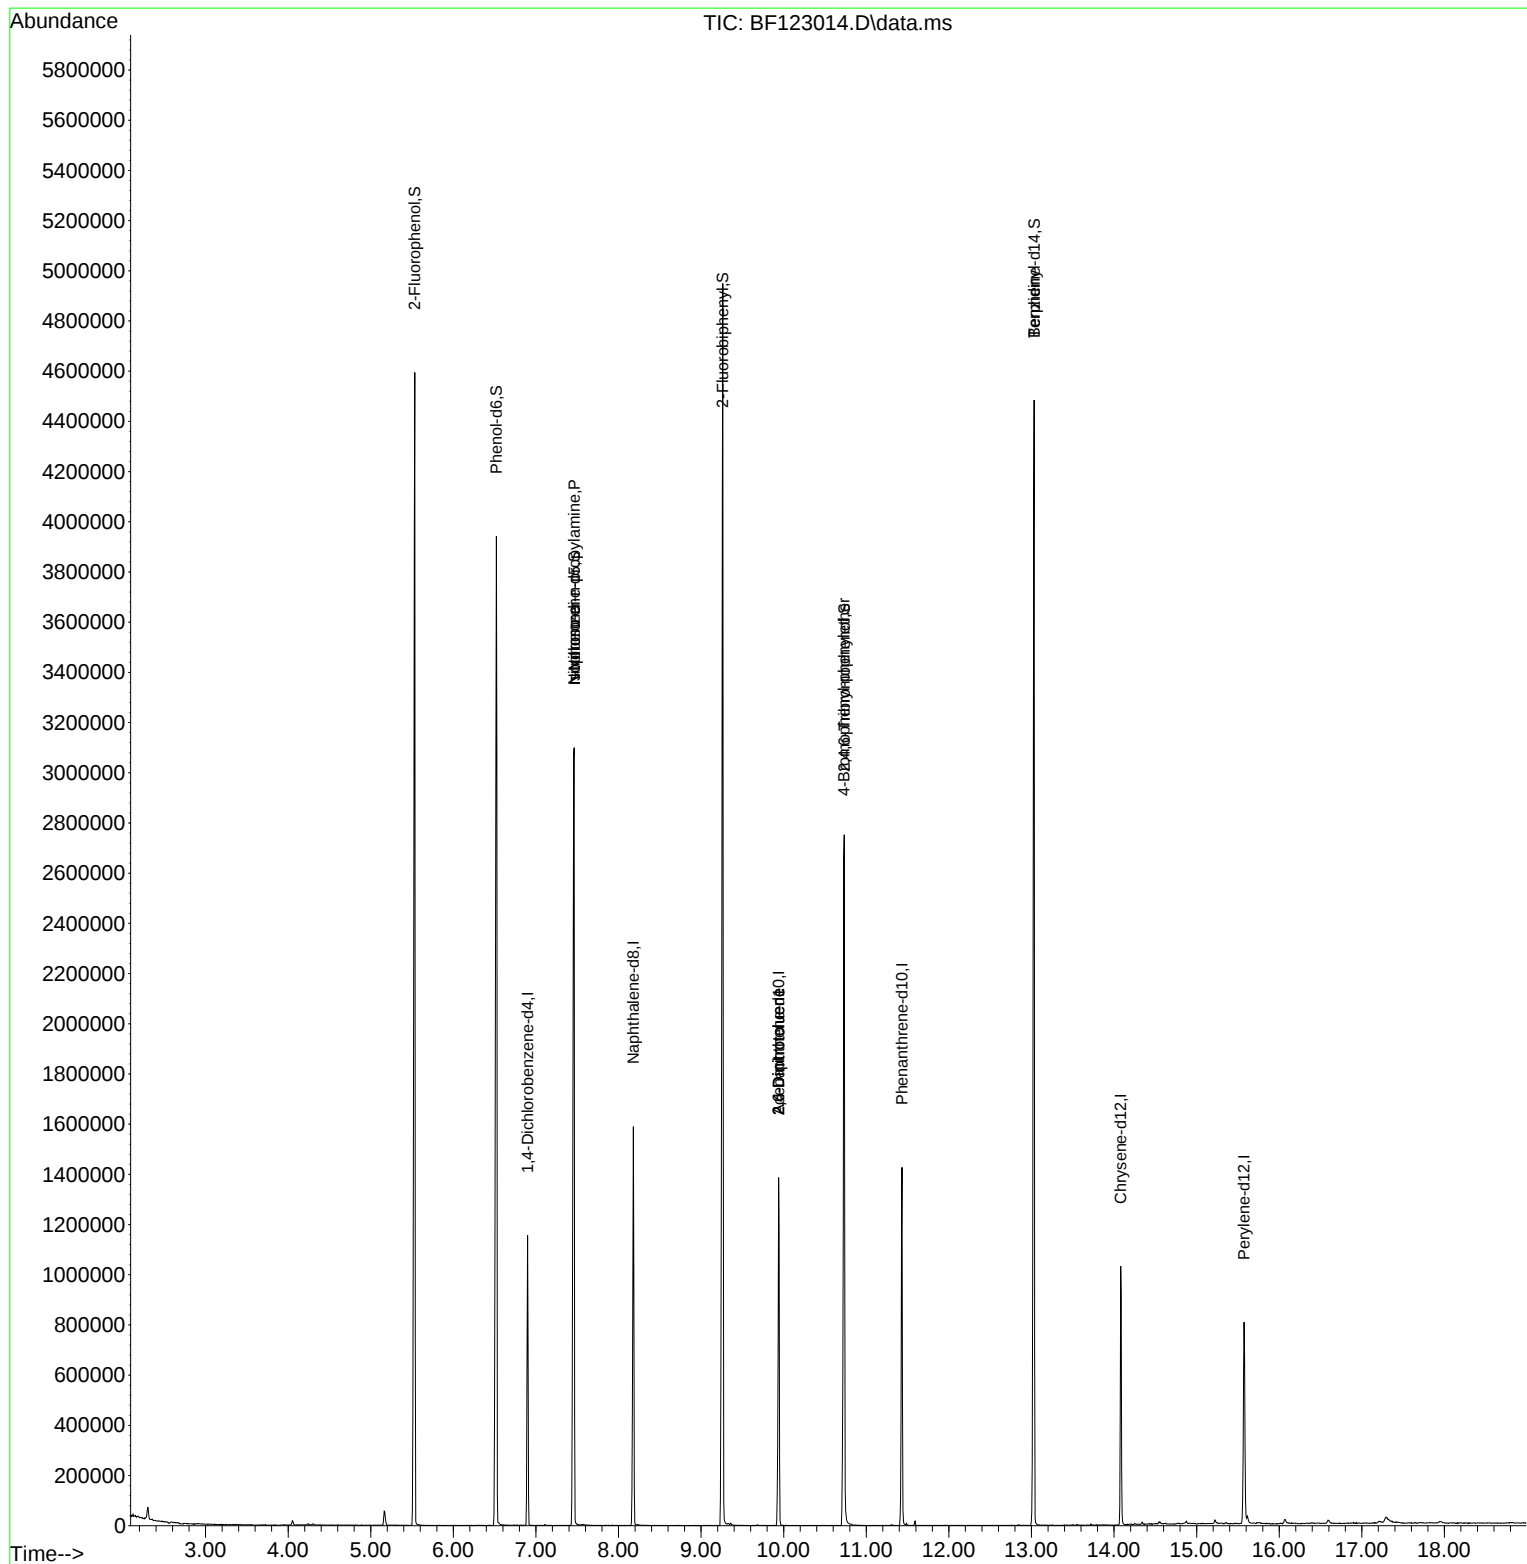

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng

Instrument :
BNA_F
ClientSampleId :
PB134201TB