
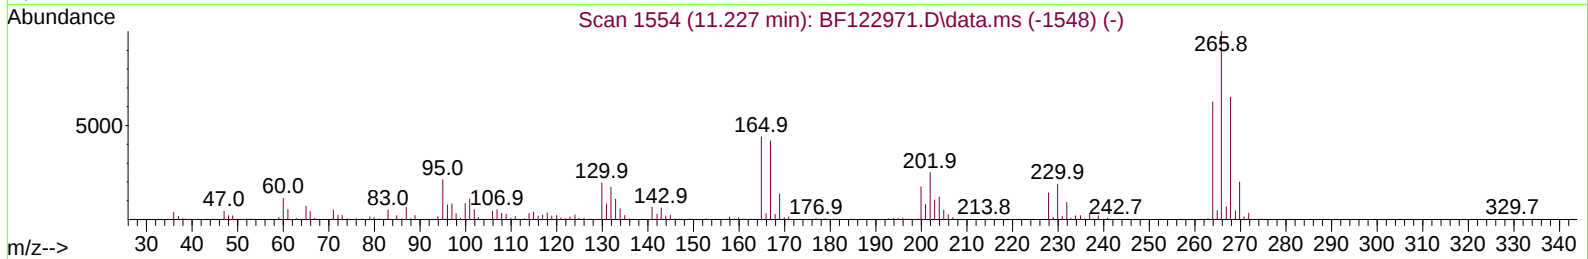
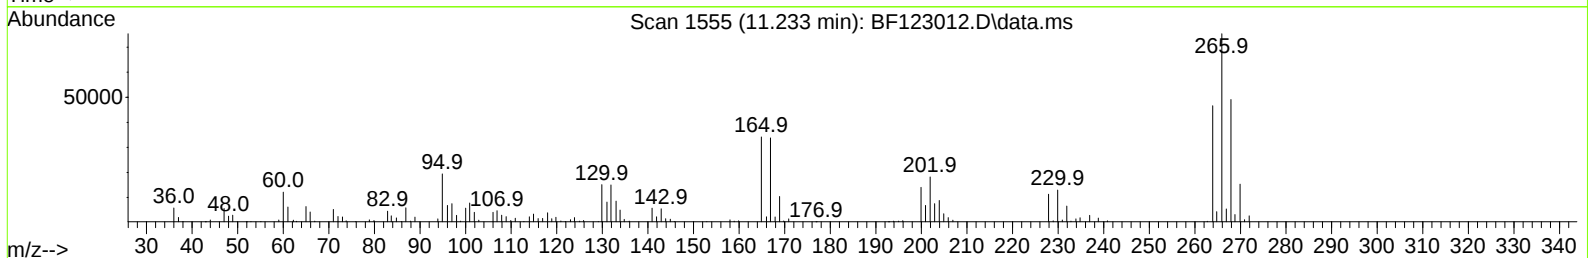


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011921\
 Data File : BF123012.D
 Acq On : 19 Jan 2021 10:43
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 20 05:30:50 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF011621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 18 13:14:08 2021
 Response via : Initial Calibration

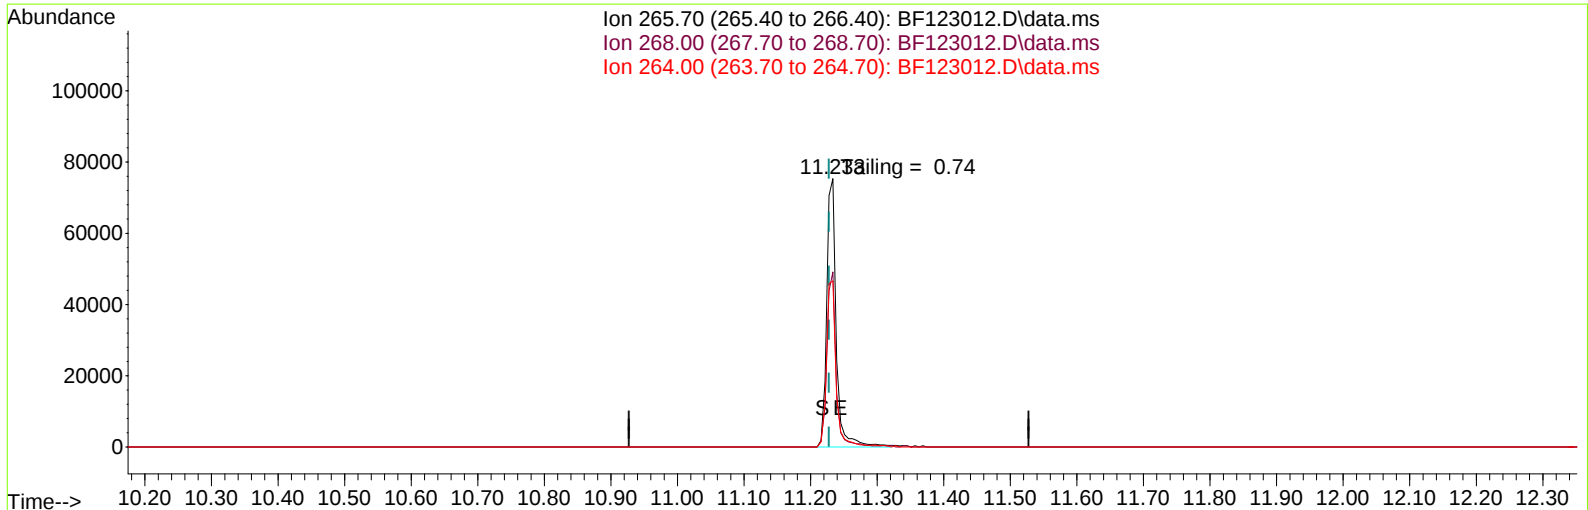

TIC: BF123012.D\data.ms

(70) Pentachlorophenol (C)




11.233min (+ 0.006) 36051.11 ng

response 76079

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	65.21
264.00	62.30	61.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011921\
 Data File : BF123012.D
 Acq On : 19 Jan 2021 10:43
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 20 05:30:50 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF011621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 18 13:14:08 2021
 Response via : Initial Calibration

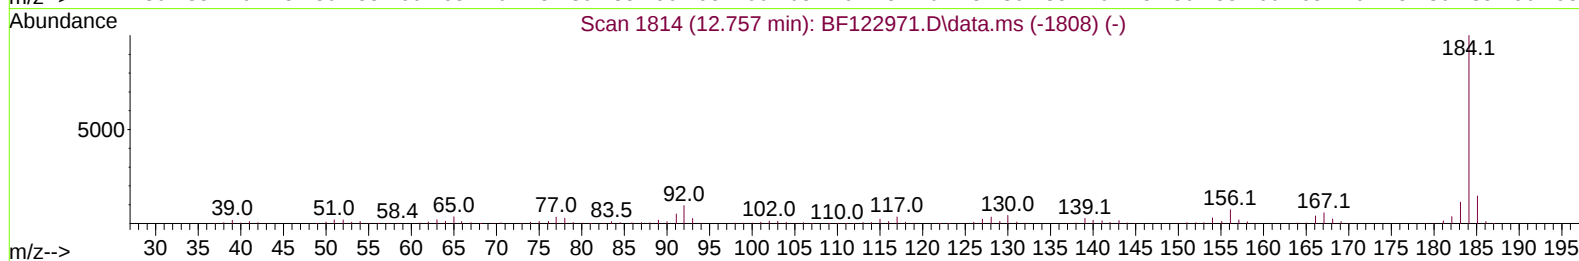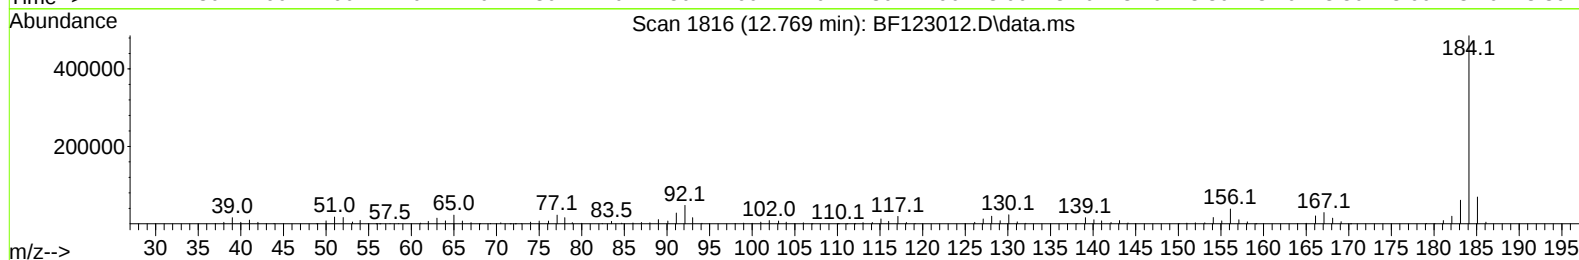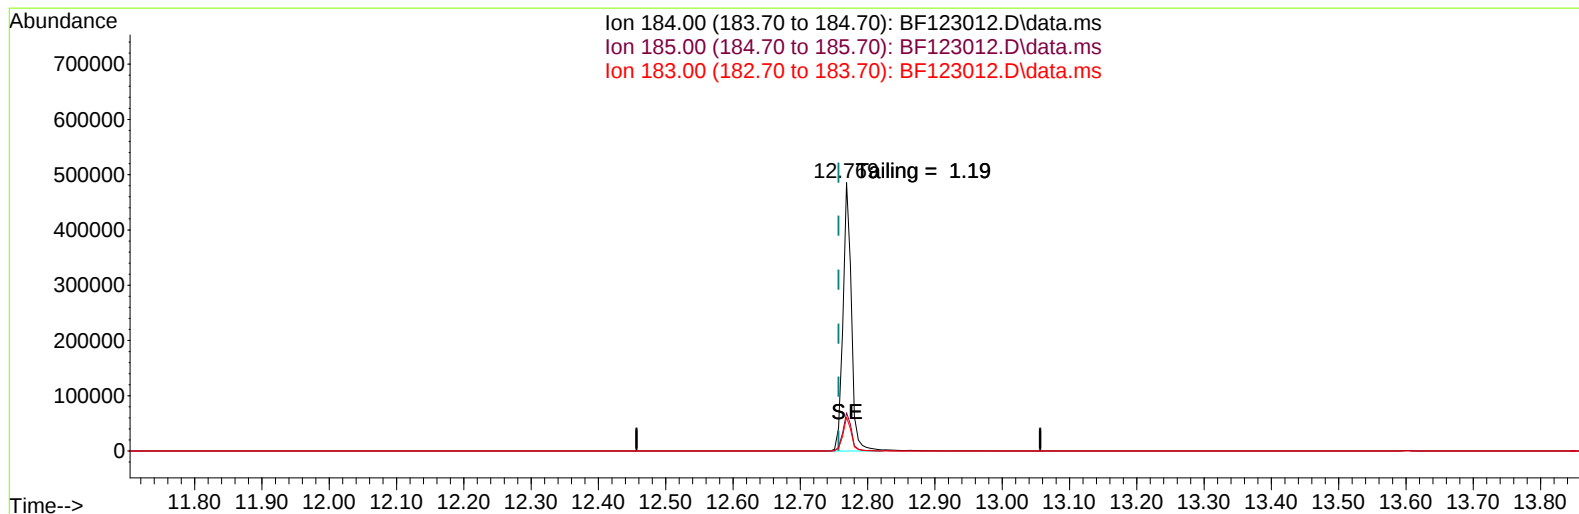

TIC: BF123012.D\data.ms

(77) Benzidine

12.769min (+ 0.012) 0.00 ng

response 425489

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.28
183.00	12.10	12.57
0.00	0.00	0.00